


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100818\
Data File : BF109650.D
Acq On : 8 Oct 2018 16:18
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 08 16:02:11 2018

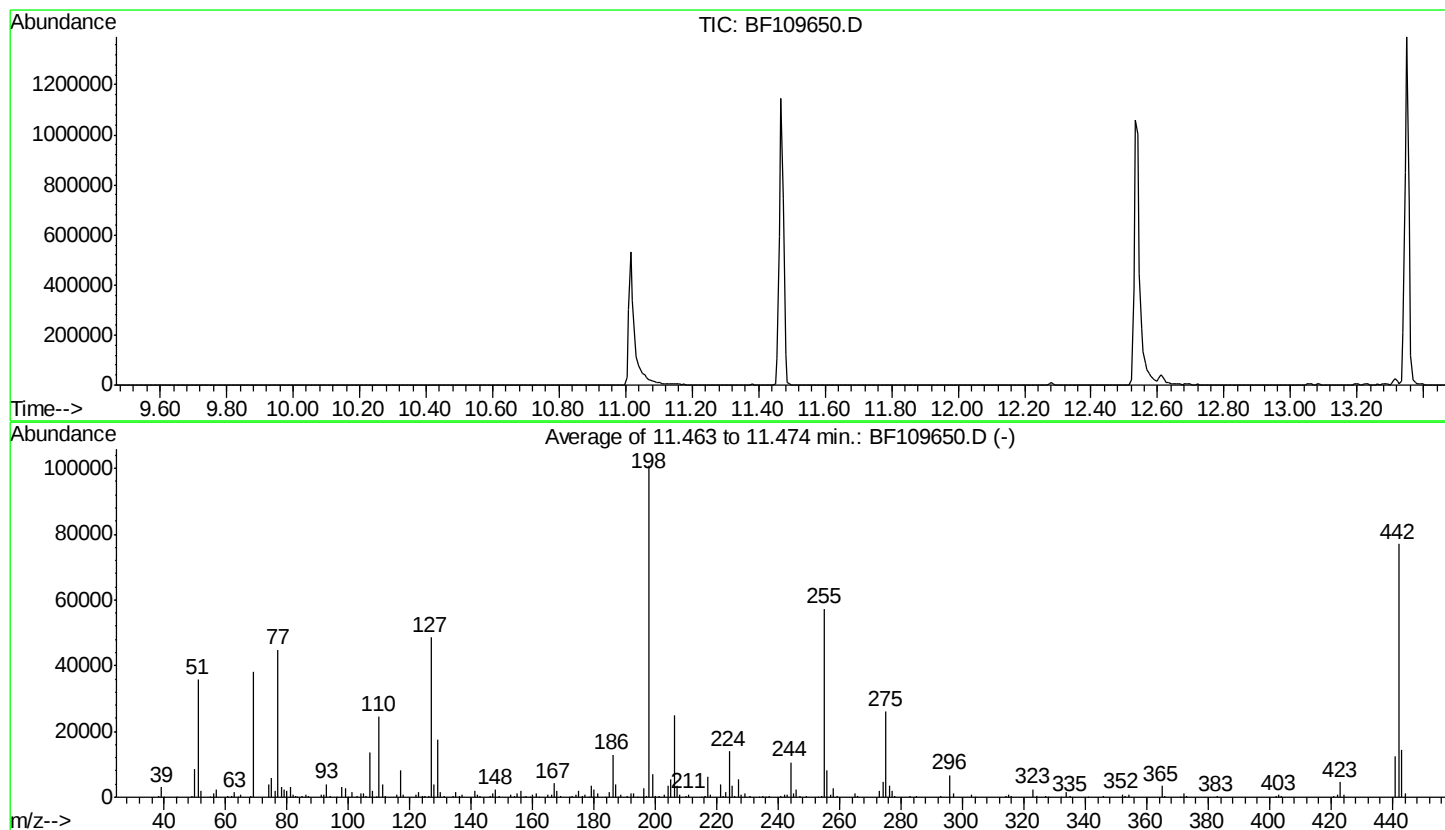

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	35672	PASS
68	69	0.00	2	1.4	542	PASS
69	198	0.00	100	37.9	38173	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	48504	PASS
197	198	0.00	2	0.5	468	PASS
198	198	100	100	100.0	100834	PASS
199	198	5	9	6.8	6831	PASS
275	198	10	60	25.8	26060	PASS
365	198	1	100	3.3	3337	PASS
441	198	0.01	100	12.3	12359	PASS
442	198	50	100	76.4	77010	PASS
443	442	15	24	18.9	14574	PASS