
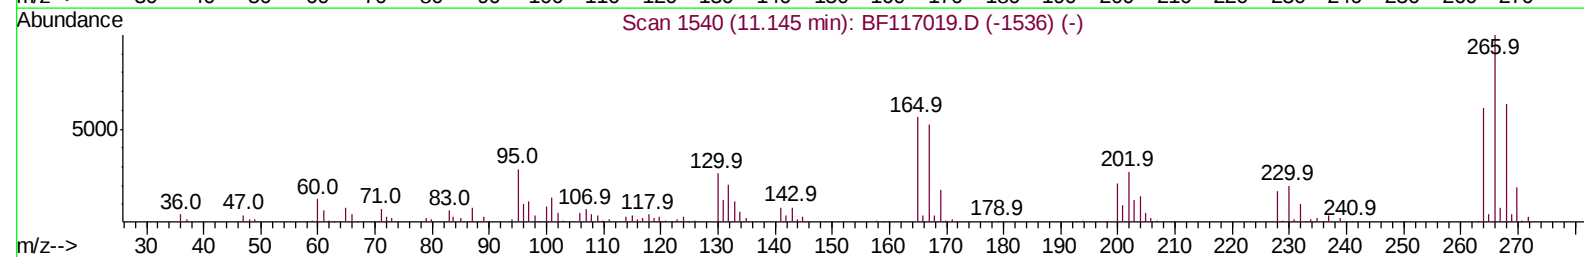
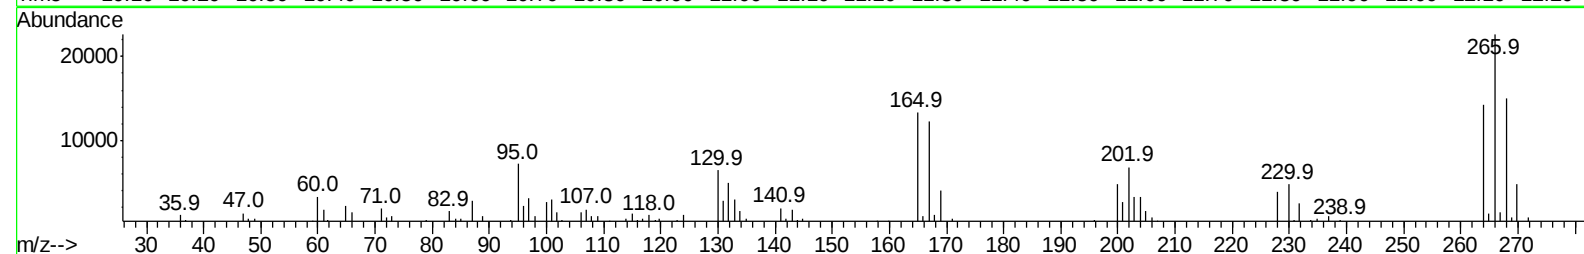


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF100819\
Data File : BF117338.D
Acq On : 8 Oct 2019 13:45
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 05:10:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 01:26:00 2019
Response via : Initial Calibration

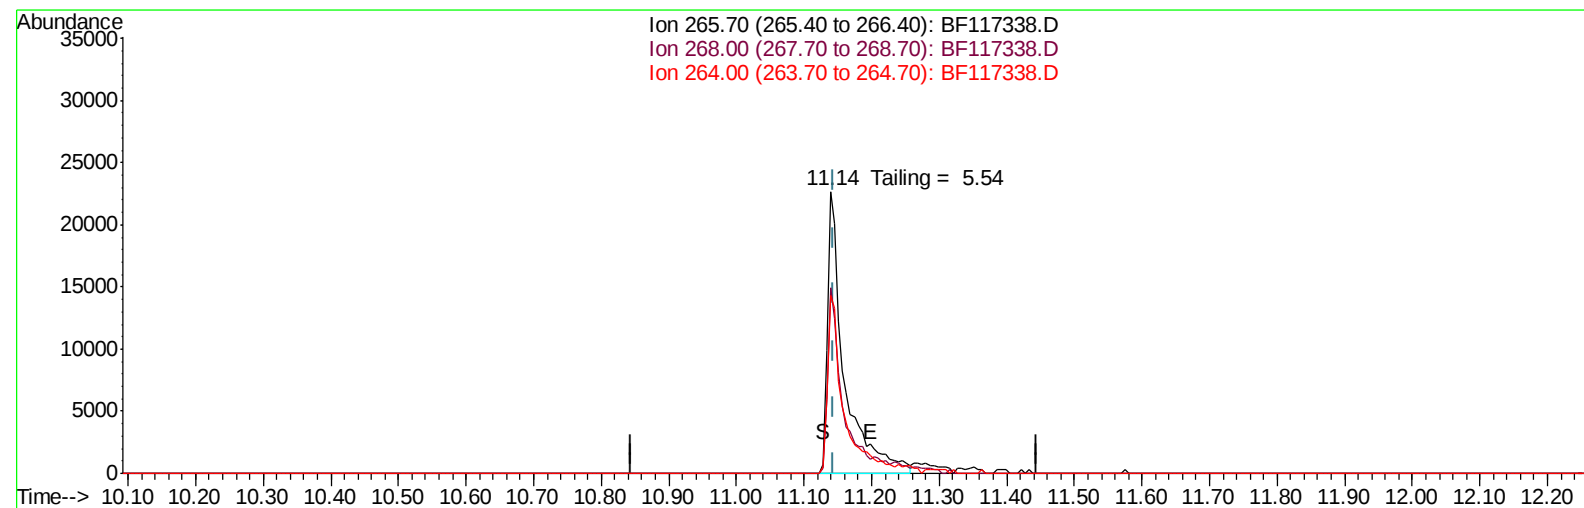

TIC: BF117338.D

(70) Pentachlorophenol (C)




11.139min (-0.006) 54646.48ng

response 40057

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	66.01
264.00	61.00	63.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF100819\
 Data File : BF117338.D
 Acq On : 8 Oct 2019 13:45
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 05:10:09 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 09 01:26:00 2019
 Response via : Initial Calibration

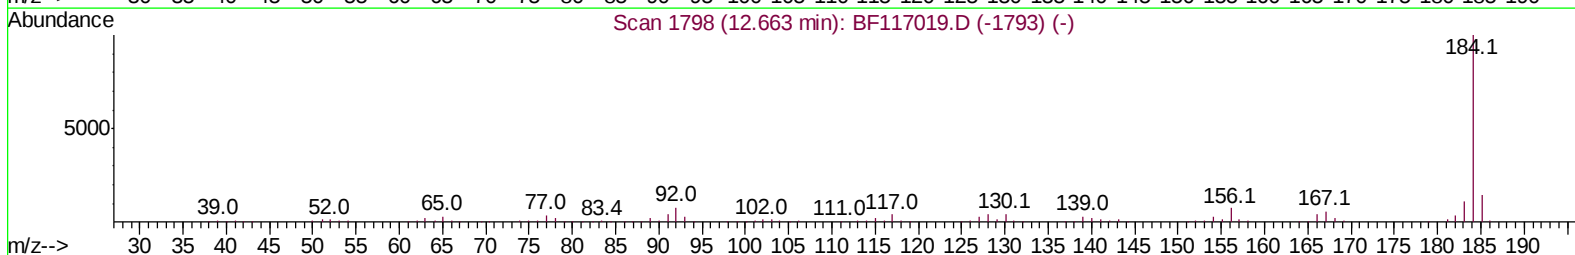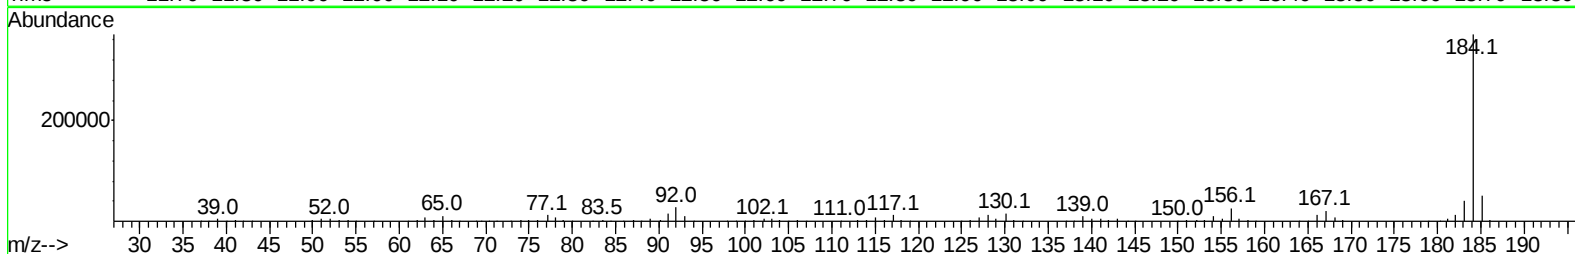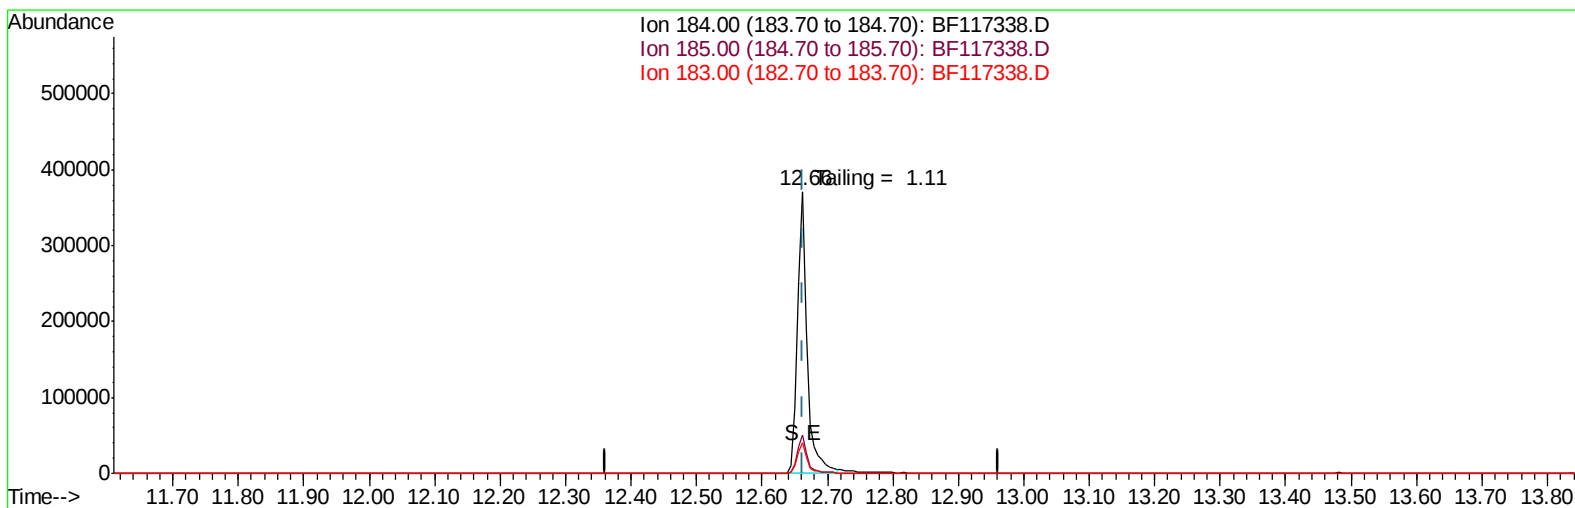

TIC: BF117338.D

(77) Benzidine

12.663min (+0.000) 0.00ng

response 395249

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	13.54
183.00	11.20	10.78
0.00	0.00	0.00