

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100819\
 Data File : BF117350.D
 Acq On : 8 Oct 2019 19:36
 Operator : JU
 Sample : K5146-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-100419

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.728	104	109	117	rVB	27091	41082	2.74%	0.349%
2	5.434	565	569	585	rBV	971660	1057504	70.54%	8.979%
3	6.445	737	741	759	rBV	970521	1137388	75.87%	9.657%
4	6.575	759	763	772	rVV	1274759	1179767	78.69%	10.017%
5	6.798	798	801	812	rBV	260353	238870	15.93%	2.028%
6	6.957	824	828	839	rBV	979370	875719	58.41%	7.435%
7	7.363	893	897	921	rBV	590980	719220	47.97%	6.106%
8	8.081	1016	1019	1036	rBV	227047	299068	19.95%	2.539%
9	9.151	1197	1201	1226	rBV	1256572	1400834	93.44%	11.894%
10	9.551	1265	1269	1282	rBV	167139	184703	12.32%	1.568%
11	9.834	1313	1317	1330	rBV	360057	362477	24.18%	3.078%
12	10.628	1448	1452	1468	rBV	685969	821572	54.80%	6.975%
13	11.322	1566	1570	1589	rBV	291591	354666	23.66%	3.011%
14	11.851	1656	1660	1668	rBV5	22494	48858	3.26%	0.415%
15	12.633	1791	1793	1801	rBV2	29800	41616	2.78%	0.353%
16	12.904	1835	1839	1842	rBV	1603750	1499220	100.00%	12.729%
17	13.469	1930	1935	1938	rBV2	52448	47497	3.17%	0.403%
18	13.798	1988	1991	2003	rVB3	69644	109405	7.30%	0.929%
19	13.963	2016	2019	2029	rBV	267111	321246	21.43%	2.727%
20	14.110	2039	2044	2048	rBV	82234	79398	5.30%	0.674%
21	14.416	2091	2096	2100	rBV	105618	97411	6.50%	0.827%
22	14.716	2143	2147	2151	rBV	109230	100774	6.72%	0.856%
23	14.786	2156	2159	2165	rBV	93633	92667	6.18%	0.787%
24	15.039	2198	2202	2207	rBV	93220	108789	7.26%	0.924%
25	15.415	2260	2266	2275	rBV2	217318	382903	25.54%	3.251%
26	15.827	2329	2336	2341	rBV	63341	94475	6.30%	0.802%
27	16.315	2412	2419	2424	rBV4	44096	80910	5.40%	0.687%


Sum of corrected areas: 11778039

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100819\
Data File : BF117350.D
Acq On : 8 Oct 2019 19:36
Operator : JU
Sample : K5146-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-100419

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

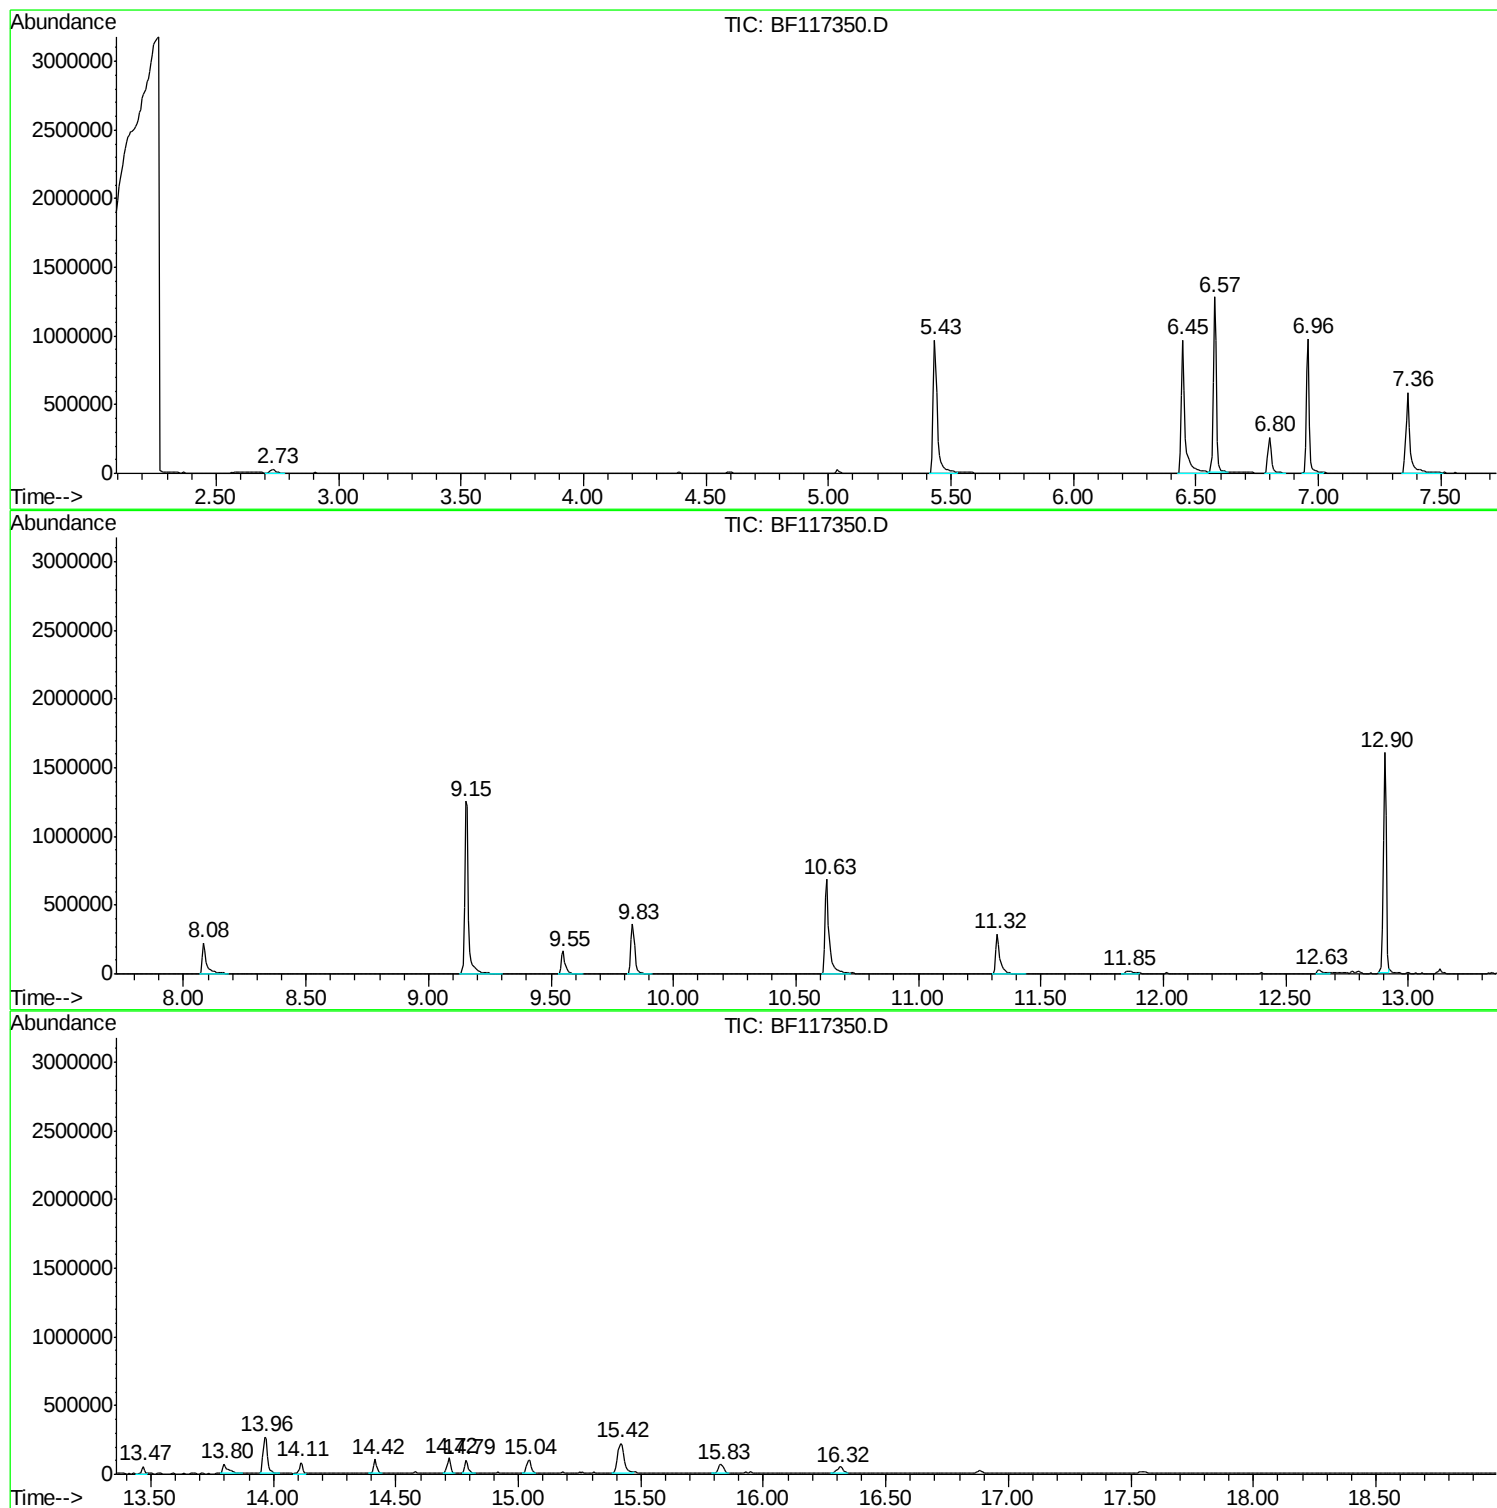

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100819\
Data_File : BF117350.D
Acq_On : 8_Oct_2019_ 19:366
Operator : JUJ
Sample : K5146-077
Misc :
ALS_Vial : 13 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
CL-01-100419

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
