


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100819\
 Data File : BF117338.D
 Acq On : 8 Oct 2019 13:45
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 09 01:26:00 2019

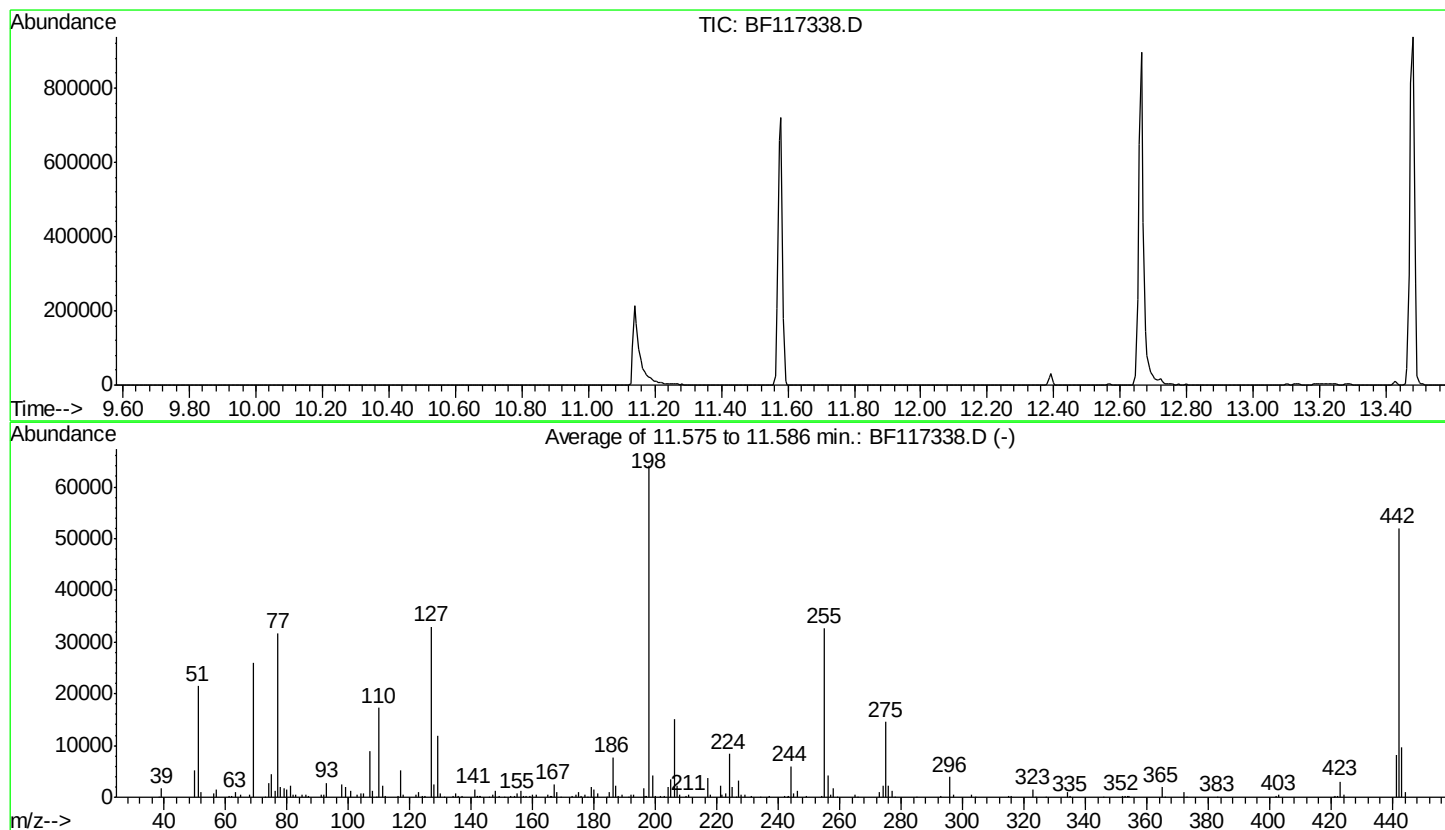

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	21528	PASS
68	69	0.00	2	1.7	447	PASS
69	198	0.00	100	40.7	26106	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.4	32929	PASS
197	198	0.00	2	0.3	173	PASS
198	198	100	100	100.0	64104	PASS
199	198	5	9	6.7	4295	PASS
275	198	10	60	22.7	14556	PASS
365	198	1	100	2.9	1875	PASS
441	198	0.01	100	12.9	8298	PASS
442	198	50	100	81.0	51920	PASS
443	442	15	24	18.7	9700	PASS