
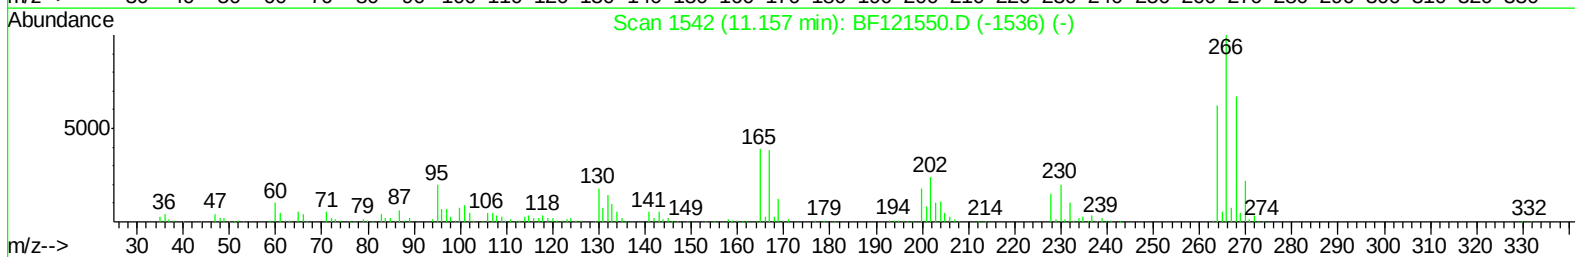
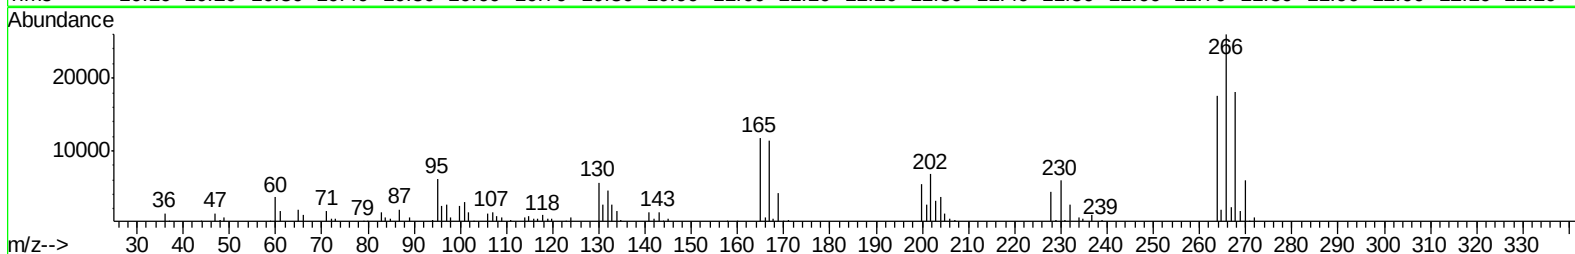


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100820\  
Data File : BF121883.D  
Acq On : 8 Oct 2020 11:52  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 05:27:08 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 01 14:29:14 2020  
Response via : Initial Calibration

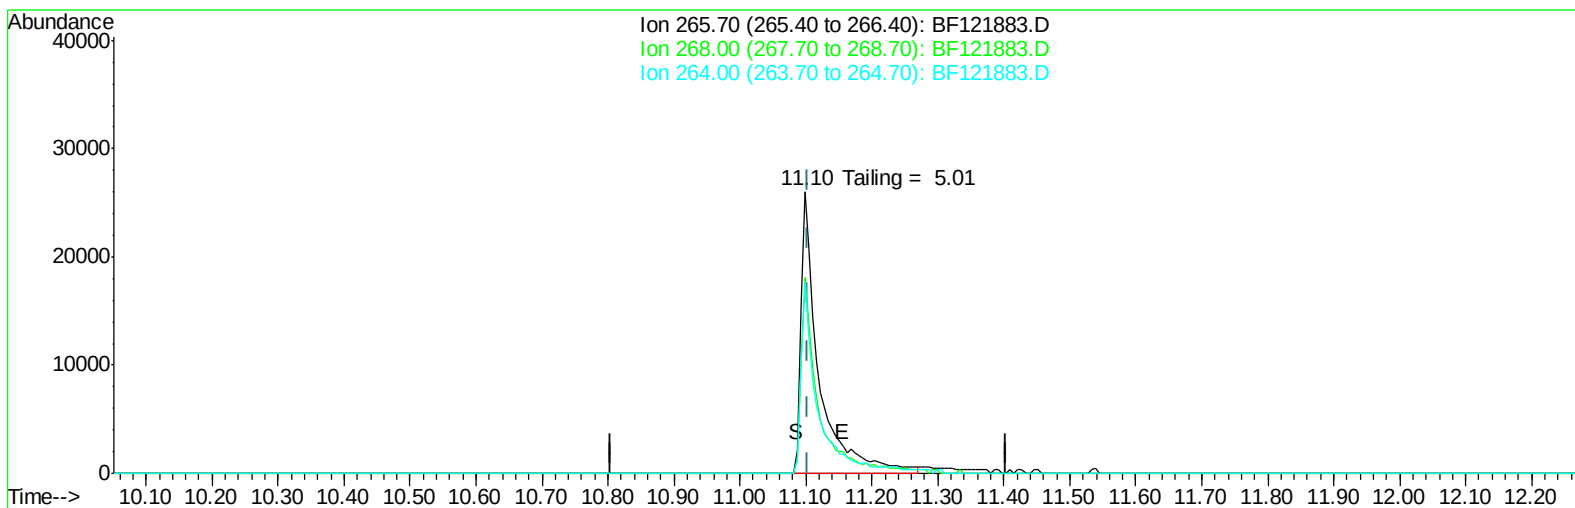

TIC: BF121883.D

(70) Pentachlorophenol (C)




11.098min (-0.006) 23659.83ng

response 49919

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.50 | 69.71 |
| 264.00 | 62.40 | 67.65 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100820\  
 Data File : BF121883.D  
 Acq On : 8 Oct 2020 11:52  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 05:27:08 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Oct 01 14:29:14 2020  
 Response via : Initial Calibration

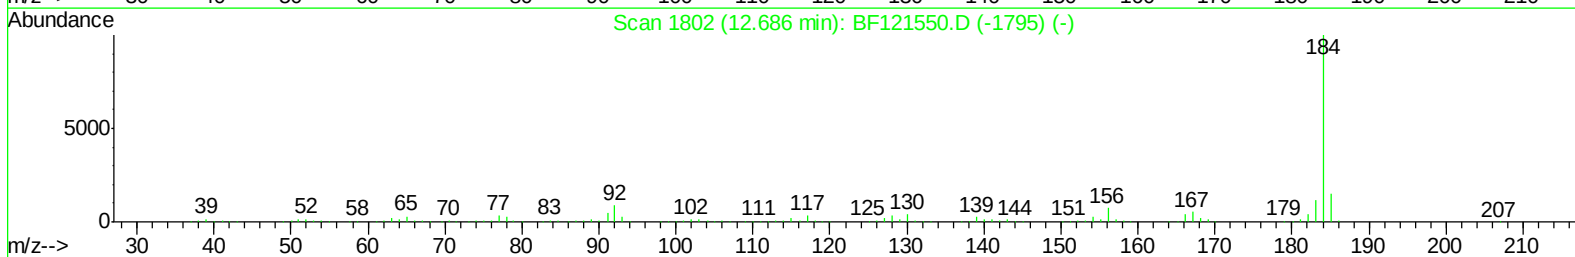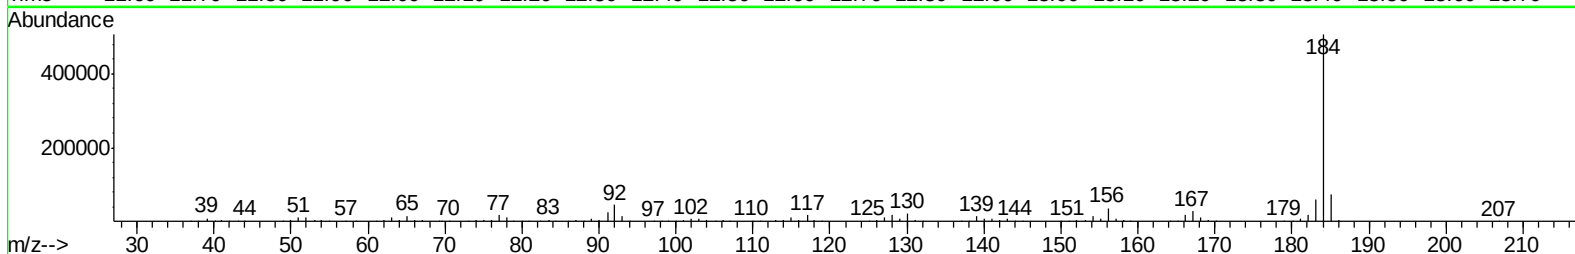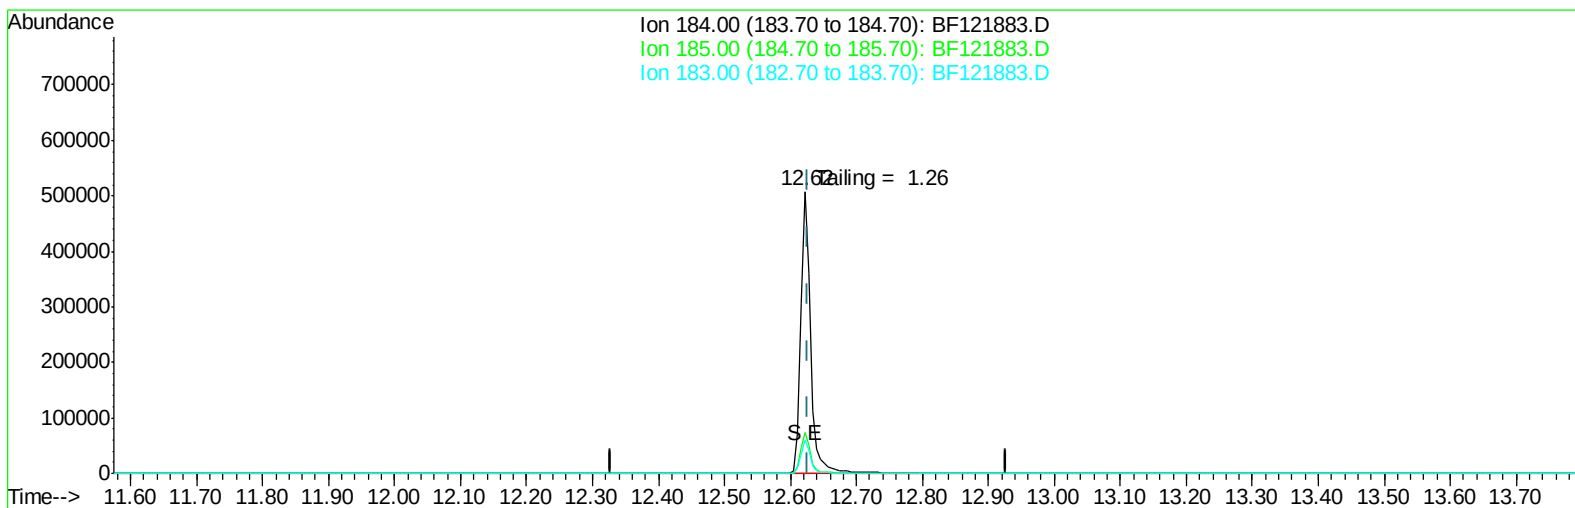

TIC: BF121883.D

(77) Benzidine

12.621min (-0.006) 0.00ng

response 534493

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.50 | 14.39 |
| 183.00 | 11.70 | 11.75 |
| 0.00   | 0.00  | 0.00  |