


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF100820\  
 Data File : BF121883.D  
 Acq On : 8 Oct 2020 11:52  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF091020.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Oct 01 14:29:14 2020

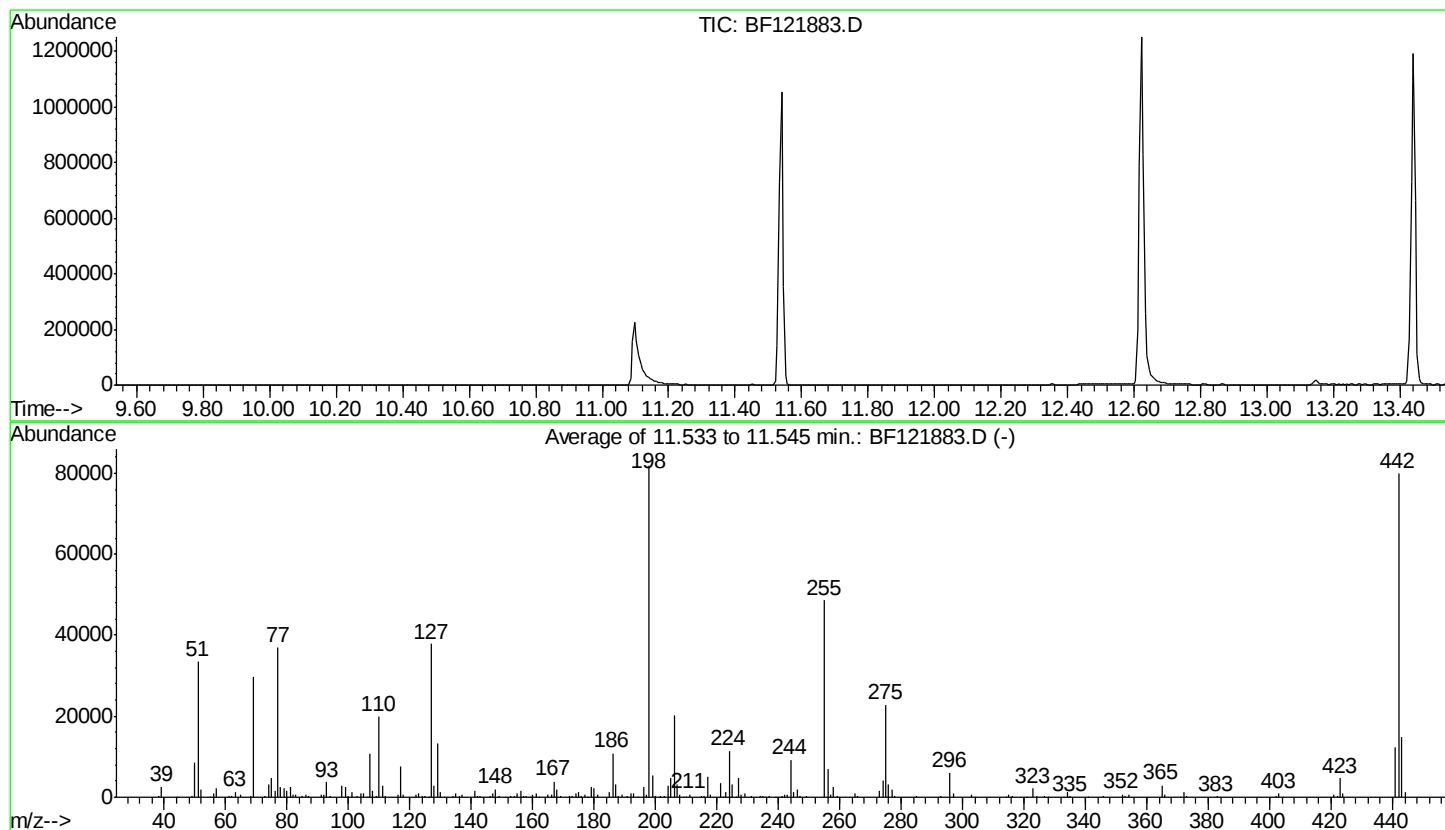

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1601

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 40.8      | 33434   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.6       | 459     | PASS             |
| 69          | 198          | 0.00         | 100          | 36.1      | 29596   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 46.3      | 37898   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.7       | 559     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 81882   | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 5434    | PASS             |
| 275         | 198          | 10           | 60           | 27.9      | 22866   | PASS             |
| 365         | 198          | 1            | 100          | 3.6       | 2941    | PASS             |
| 441         | 198          | 0.01         | 100          | 15.0      | 12244   | PASS             |
| 442         | 198          | 50           | 100          | 97.8      | 80096   | PASS             |
| 443         | 442          | 15           | 24           | 18.5      | 14854   | PASS             |