

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100821\
 Data File : BF125776.D
 Acq On : 8 Oct 2021 10:48
 Operator : JU/CG
 Sample : PB139688BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB139688BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125776.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.204	10	20	29	rVB	176165	240090	2.97%	0.498%
2	5.475	570	576	579	rBV	5727787	6370501	78.71%	13.202%
3	6.475	739	746	749	rBV	5095923	6379166	78.82%	13.220%
4	6.845	805	809	812	rBV	1815085	1453133	17.95%	3.011%
5	7.404	898	904	907	rBV	3786978	4314433	53.31%	8.941%
6	8.122	1021	1026	1030	rBV	2240842	2046196	25.28%	4.240%
7	9.204	1203	1210	1213	rBV	7649908	8093796	100.00%	16.773%
8	9.875	1319	1324	1328	rBV	2699778	2373979	29.33%	4.920%
9	10.663	1452	1458	1462	rBV	4568491	4793013	59.22%	9.933%
10	11.357	1572	1576	1580	rBV	2701907	2322127	28.69%	4.812%
11	12.951	1841	1847	1850	rBV	6857560	7376154	91.13%	15.286%
12	13.992	2020	2024	2027	rBV	1615069	1392883	17.21%	2.887%
13	15.445	2266	2271	2276	rBV	979067	1099180	13.58%	2.278%




Sum of corrected areas: 48254651

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100821\
Data File : BF125776.D
Acq On : 8 Oct 2021 10:48
Operator : JU/CG
Sample : PB139688BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139688BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

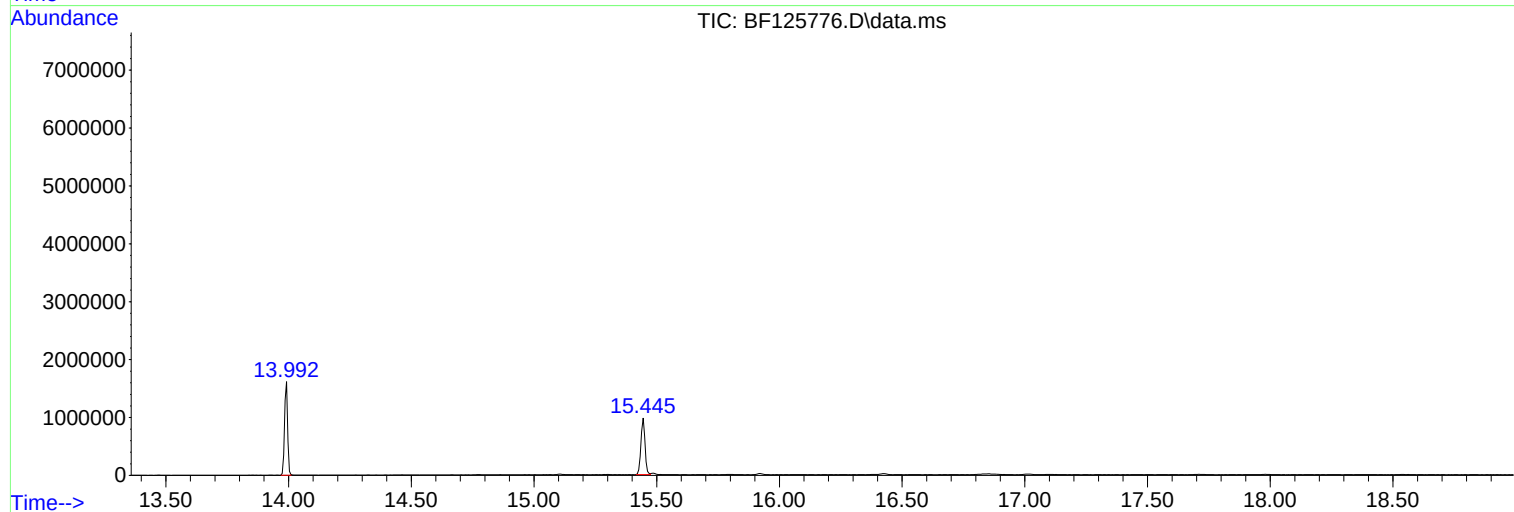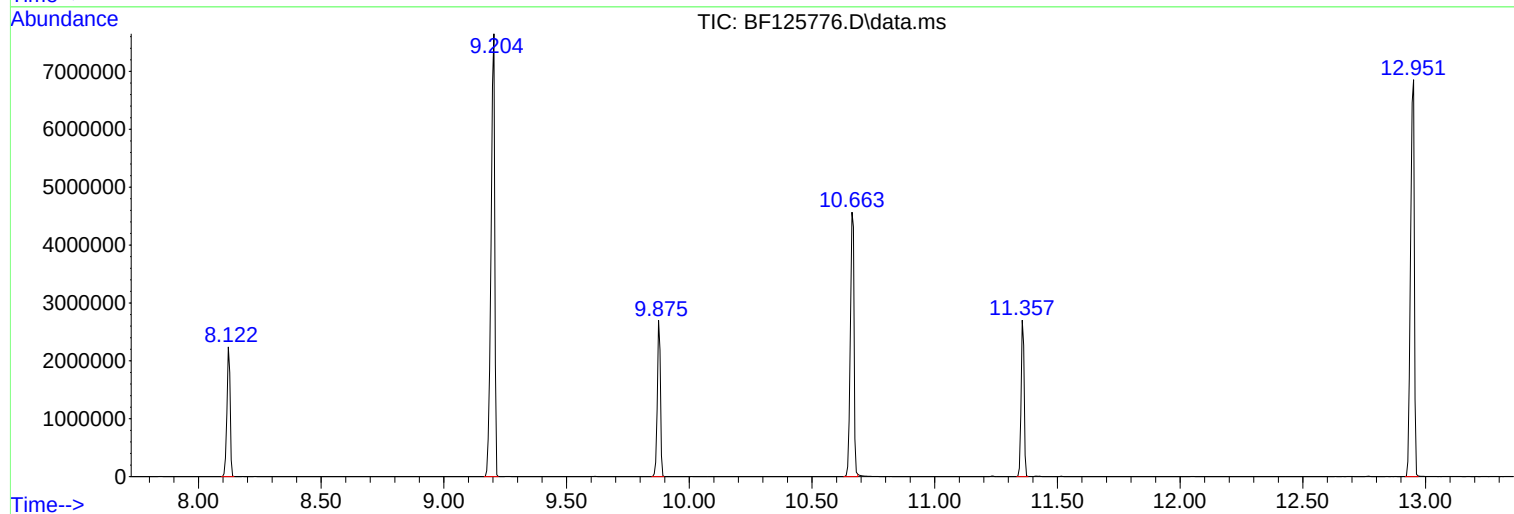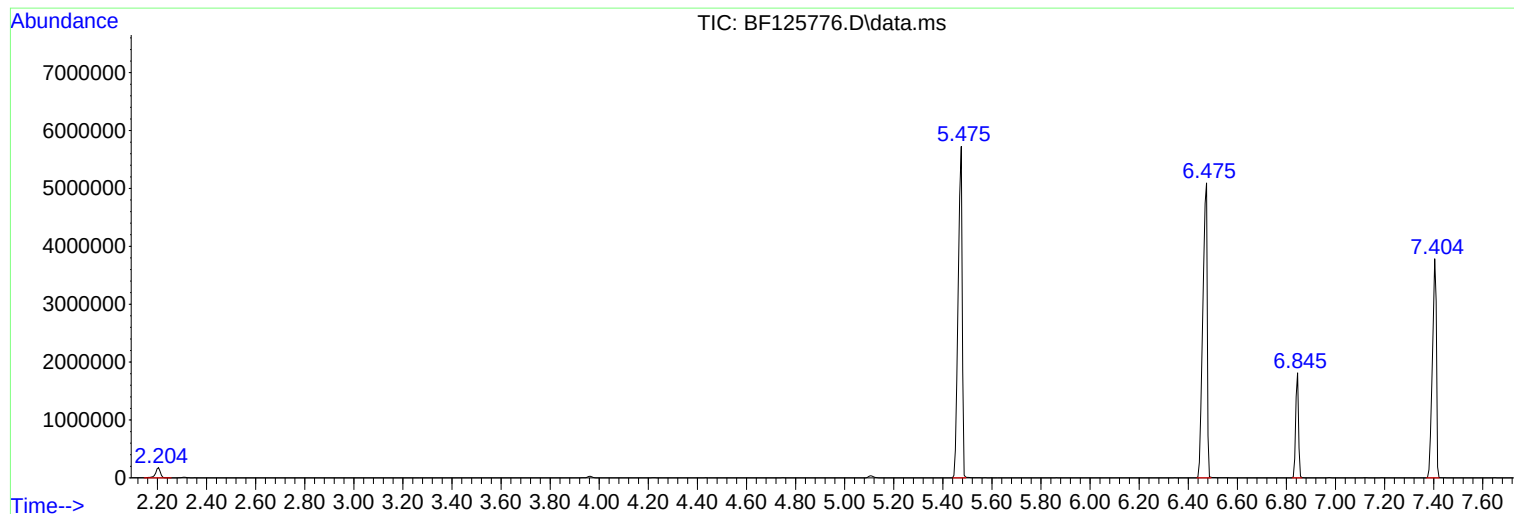

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100821\
Data File : BF125776.D
Acq On : 8 Oct 2021 10:48
Operator : JU/CG
Sample : PB139688BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139688BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.204	3.30 ng	240090	1,4-Dichlorobenzene-d4	6.845

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

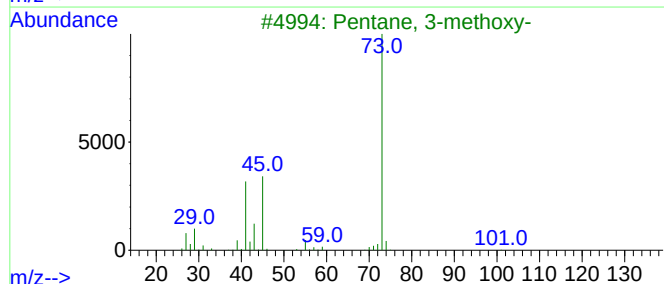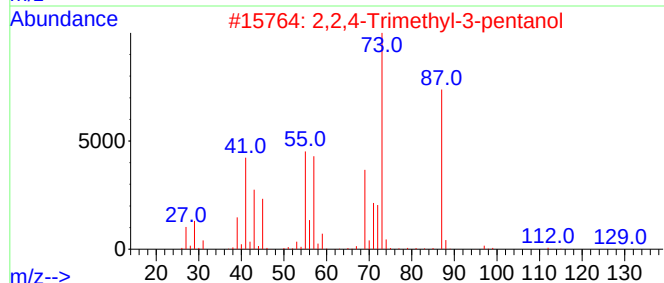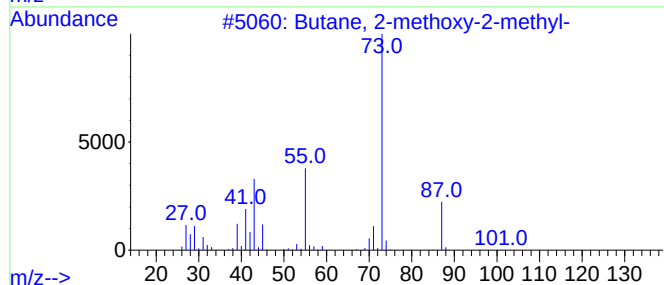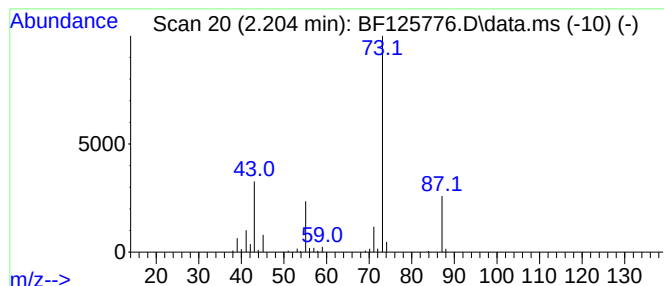

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100821\
Data File : BF125776.D
Acq On : 8 Oct 2021 10:48
Operator : JU/CG
Sample : PB139688BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139688BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.204	3.3	ng	240090	1	6.845	1453130	20.0