

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100821\
 Data File : BF125790.D
 Acq On : 8 Oct 2021 19:14
 Operator : JU/CG
 Sample : M4111-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GROWS-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125790.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.828	121	126	137	rVB	346967	474365	7.34%	1.172%
2	4.657	432	437	442	rBV	587424	585886	9.07%	1.448%
3	4.722	444	448	452	rBV	68342	70147	1.09%	0.173%
4	5.075	501	508	510	rBV	507888	672981	10.42%	1.663%
5	5.093	510	511	516	rVB	356345	305614	4.73%	0.755%
6	5.469	570	575	578	rBV	4733684	4918883	76.13%	12.153%
7	6.469	740	745	748	rBV	4296445	4446686	68.82%	10.986%
8	6.845	805	809	812	rBV	1309419	1171393	18.13%	2.894%
9	7.404	898	904	907	rBV	3620087	3394099	52.53%	8.386%
10	8.022	1006	1009	1022	rBV	920616	847588	13.12%	2.094%
11	8.122	1022	1026	1029	rBV	2048346	1628891	25.21%	4.024%
12	9.198	1204	1209	1212	rBV	7108531	6461494	100.00%	15.964%
13	9.875	1320	1324	1327	rBV	2350645	1850359	28.64%	4.572%
14	10.663	1453	1458	1461	rBV	4149007	3801143	58.83%	9.391%
15	11.357	1572	1576	1579	rBV	2145643	1713182	26.51%	4.233%
16	11.751	1640	1643	1646	rBV	119988	84921	1.31%	0.210%
17	12.457	1760	1763	1766	rVB	155410	111442	1.72%	0.275%
18	12.945	1841	1846	1849	rBV	5814893	5599021	86.65%	13.833%
19	13.986	2019	2023	2027	rBV	1328709	1110450	17.19%	2.744%
20	15.439	2265	2270	2276	rBV	975281	1226526	18.98%	3.030%




Sum of corrected areas: 40475071

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100821\
Data File : BF125790.D
Acq On : 8 Oct 2021 19:14
Operator : JU/CG
Sample : M4111-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GROWS-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

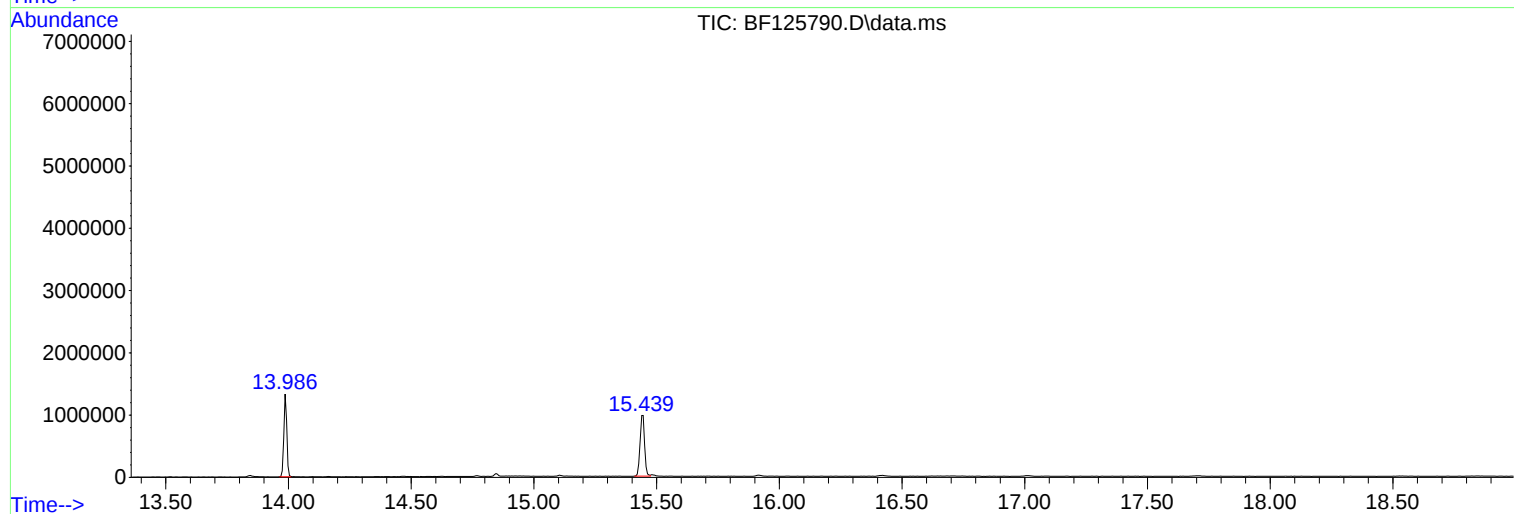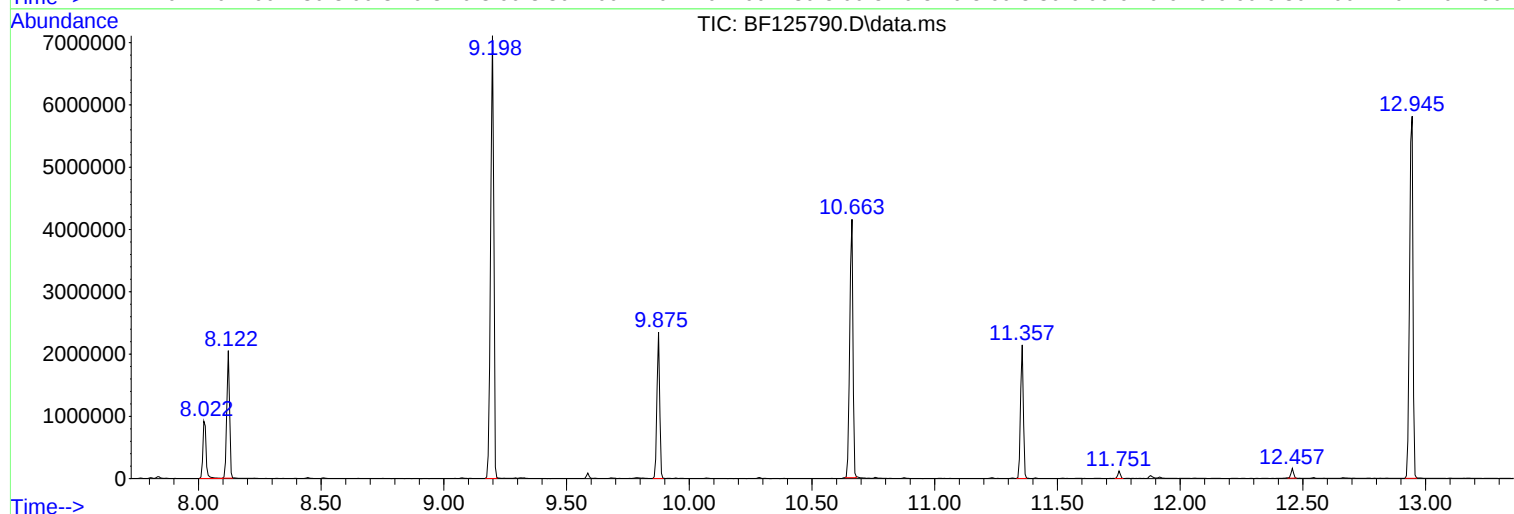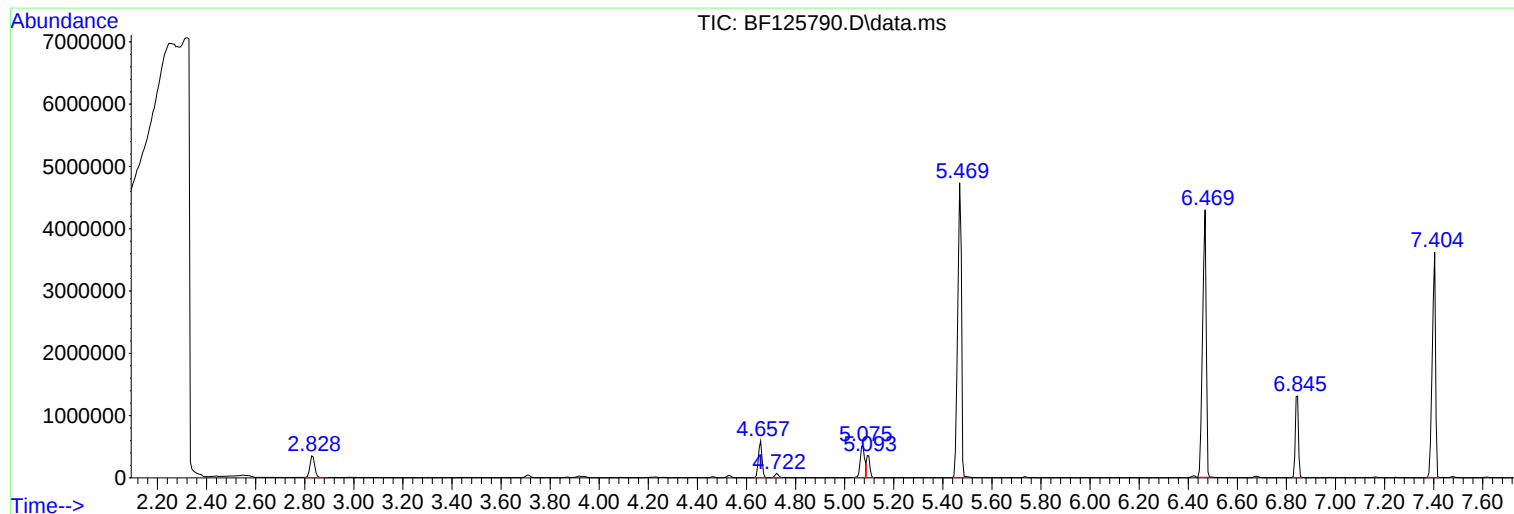

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100821\
Data File : BF125790.D
Acq On : 8 Oct 2021 19:14
Operator : JU/CG
Sample : M4111-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GROWS-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100821\
Data File : BF125790.D
Acq On : 8 Oct 2021 19:14
Operator : JU/CG
Sample : M4111-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GROWS-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
