


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100821\
 Data File : BF125774.D
 Acq On : 8 Oct 2021 9:46
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 07 17:16:23 2021

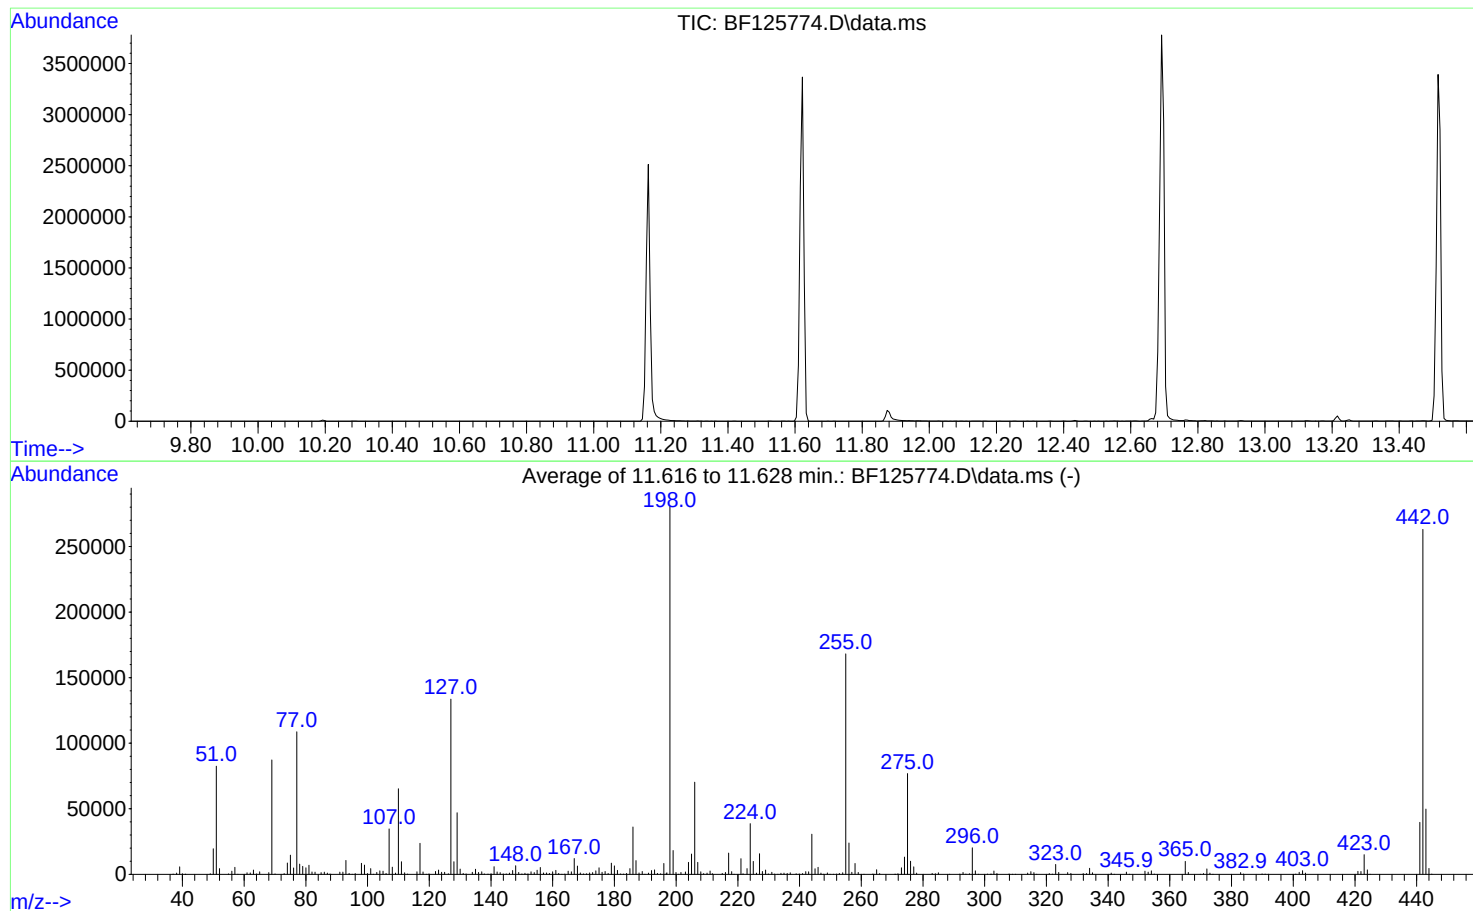




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	82515	PASS
68	69	0.00	2	1.5	1341	PASS
69	198	0.00	100	31.1	87232	PASS
70	69	0.00	2	0.4	367	PASS
127	198	10	80	47.6	133603	PASS
197	198	0.00	2	0.4	1195	PASS
198	198	100	100	100.0	280491	PASS
199	198	5	9	6.5	18245	PASS
275	198	10	60	27.4	76832	PASS
365	198	1	100	3.5	9895	PASS
441	198	0.01	100	14.1	39621	PASS
442	442	50	100	100.0	263061	PASS
443	442	15	24	18.9	49813	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100821\
 Data File : BF125774.D
 Acq On : 8 Oct 2021 9:46
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 08 11:57:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 07 17:16:23 2021
 Response via : Initial Calibration

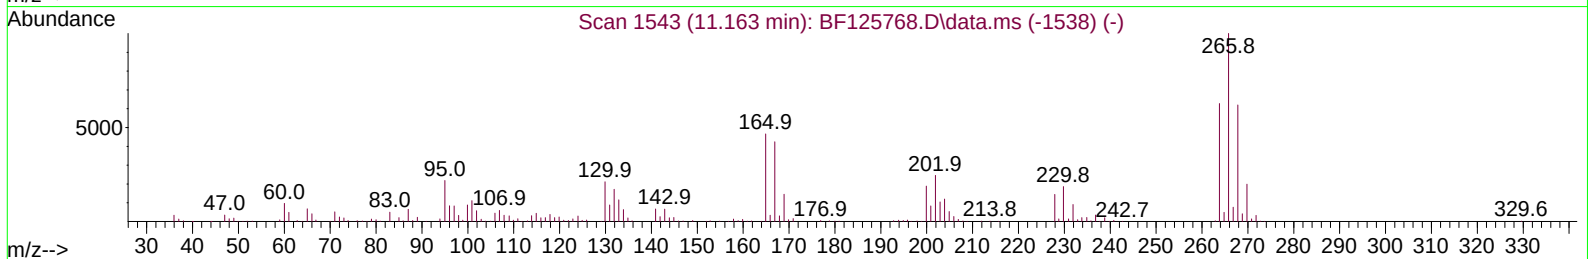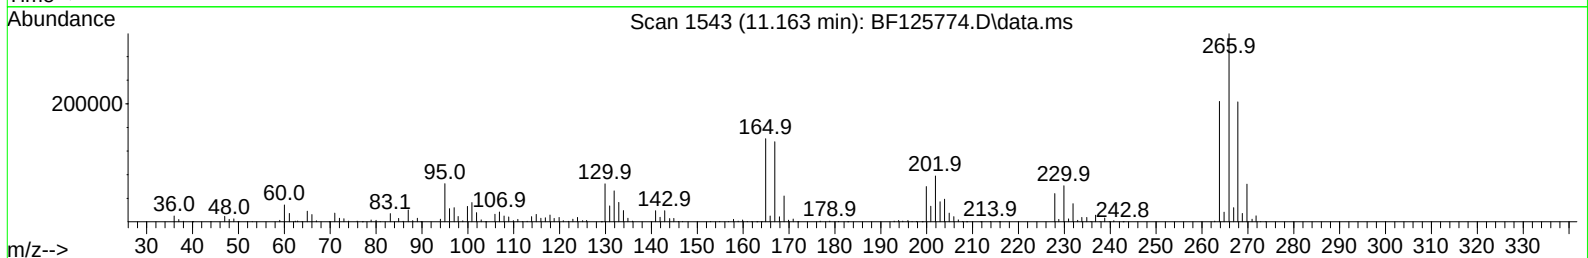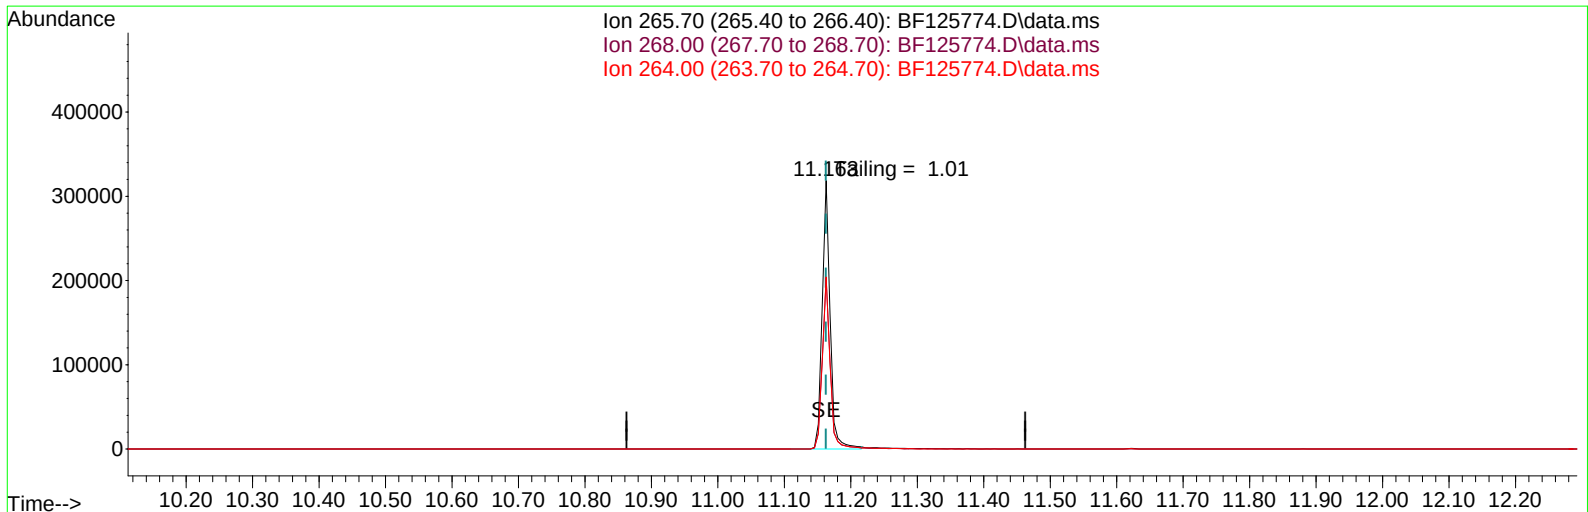

TIC: BF125774.D\data.ms

(70) Pentachlorophenol (C)

11.163min (+ 0.000) 34515.25 ng




response 271625

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.78
264.00	69.90	64.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100821\
Data File : BF125774.D
Acq On : 8 Oct 2021 9:46
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 08 11:57:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 07 17:16:23 2021
Response via : Initial Calibration

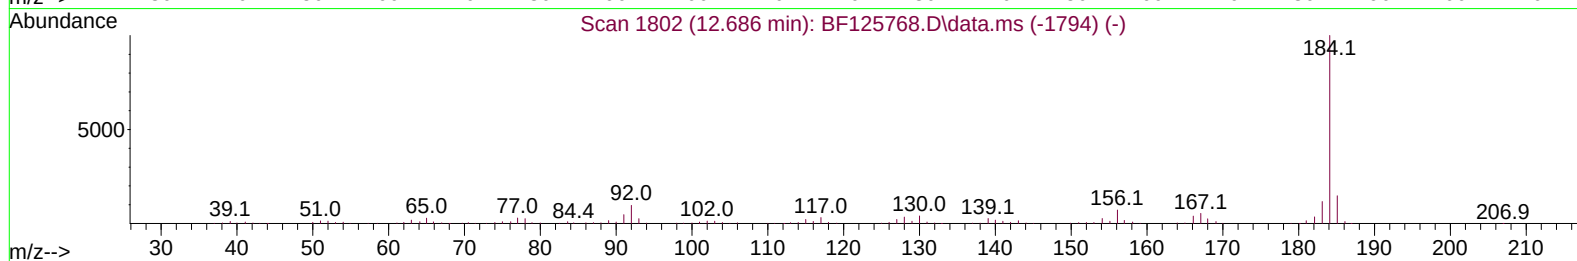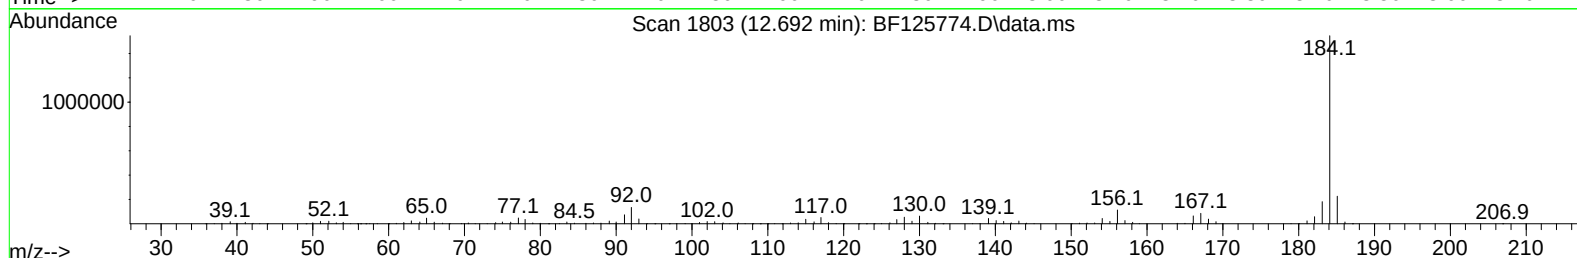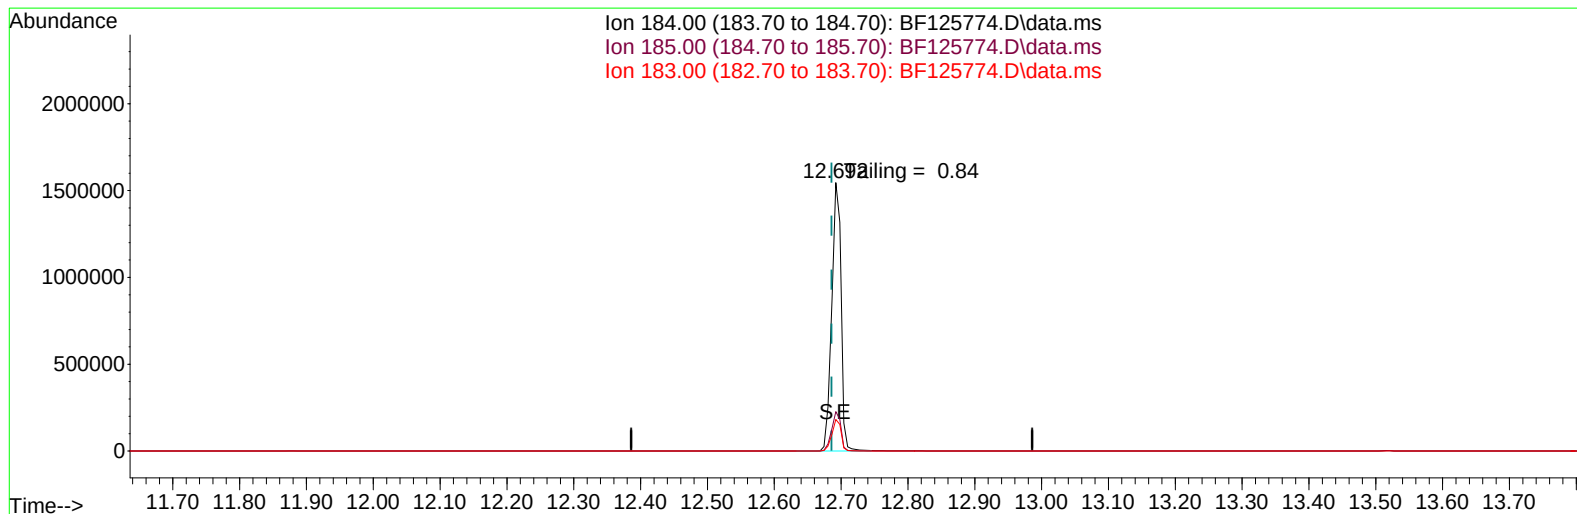

TIC: BF125774.D\data.ms

(77) Benzidine

12.692min (+ 0.006) 0.00 ng

response 1500240

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.70
183.00	10.10	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/8/2021	BNA_F	<u>BF125774.D</u>
Compound Name	Response	Retention Time
DDT	603509	13.51
DDD	9482	13.21
DDE	276	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9758	613267	1.59

Instrument :
BNA_F
ClientSampleId :
DFTPP