

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100824\
 Data File : BF139710.D
 Acq On : 08 Oct 2024 14:05
 Operator : RC/JU
 Sample : P4328-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CONCRETE-RO

Quant Time: Oct 08 14:30:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 02 04:58:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.863	152	76585	20.000	ng	0.00
21) Naphthalene-d8	8.145	136	277164	20.000	ng	0.00
39) Acenaphthene-d10	9.898	164	140632	20.000	ng	-0.01
64) Phenanthrene-d10	11.386	188	232617	20.000	ng	0.00
76) Chrysene-d12	14.027	240	174990	20.000	ng	0.00
86) Perylene-d12	15.498	264	143610	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.487	112	373162	84.453	ng	0.00
7) Phenol-d6	6.498	99	500573	84.242	ng	0.00
23) Nitrobenzene-d5	7.428	82	334029	61.018	ng	0.00
42) 2,4,6-Tribromophenol	10.692	330	96172	70.841	ng	0.00
45) 2-Fluorobiphenyl	9.222	172	616404	67.289	ng	0.00
79) Terphenyl-d14	12.974	244	577053	54.109	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100824\
Data File : BF139710.D
Acq On : 08 Oct 2024 14:05
Operator : RC/JU
Sample : P4328-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONCRETE-RO

Quant Time: Oct 08 14:30:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration



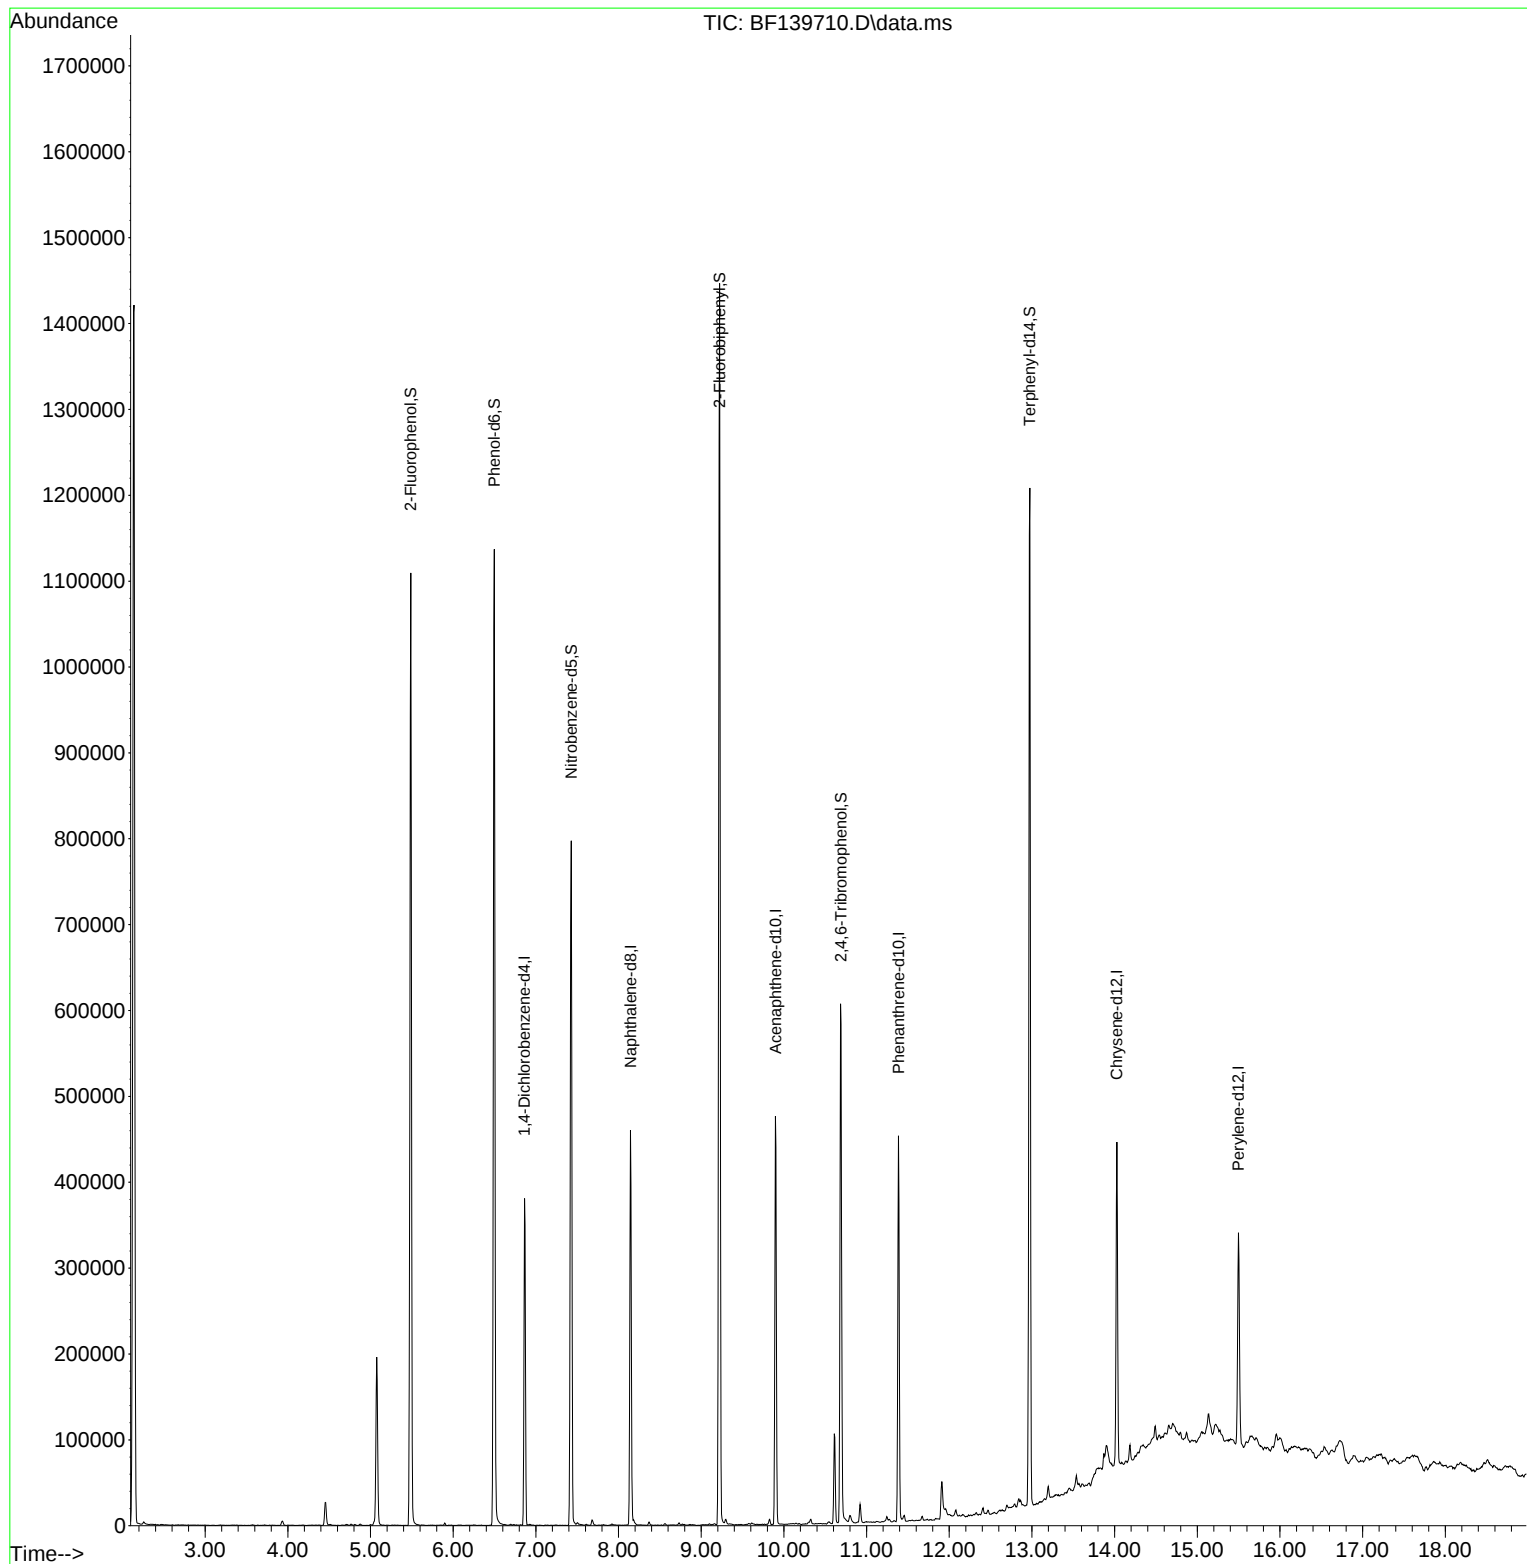




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.863 min Scan# 812
Delta R.T. -0.006 min
Lab File: BF139710.D
Acq: 08 Oct 2024 14:05




Instrument :
BNA_F
ClientSampleId :
CONCRETE-RO


Tgt Ion:152 Resp: 76585
Ion Ratio Lower Upper
152 100
150 156.3 127.2 190.8
115 59.9 49.0 73.4

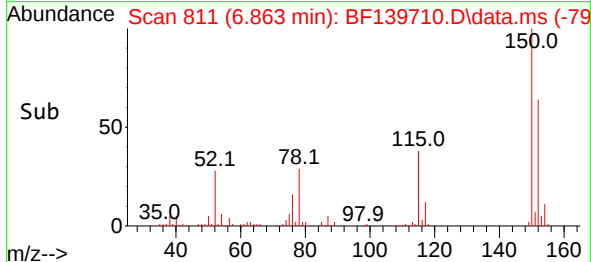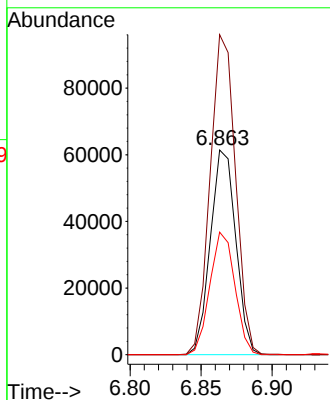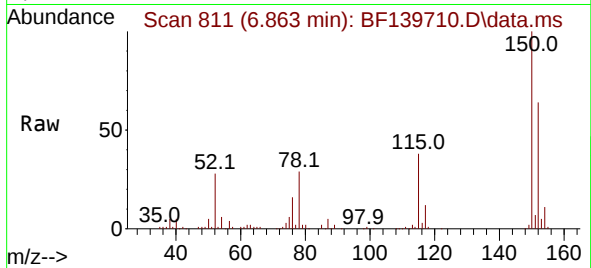

#5
2-Fluorophenol
Concen: 84.453 ng
RT: 5.487 min Scan# 577
Delta R.T. -0.000 min
Lab File: BF139710.D
Acq: 08 Oct 2024 14:05

Tgt Ion:112 Resp: 373162
Ion Ratio Lower Upper
112 100
64 67.3 54.2 81.4
63 36.3 29.4 44.2

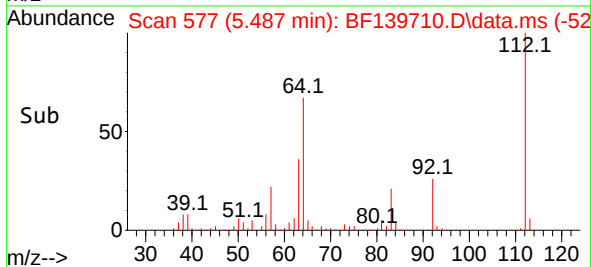
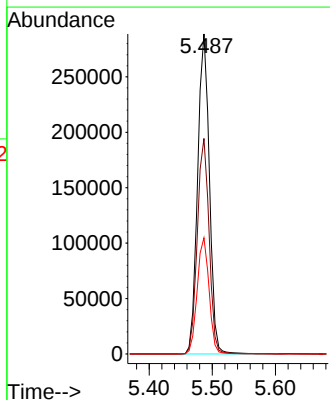
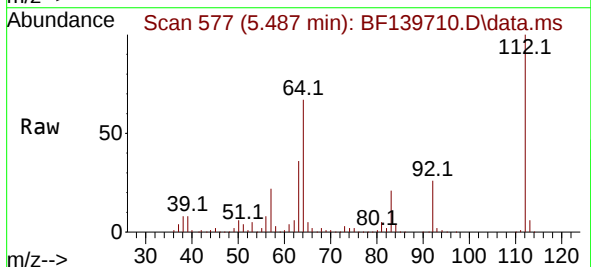


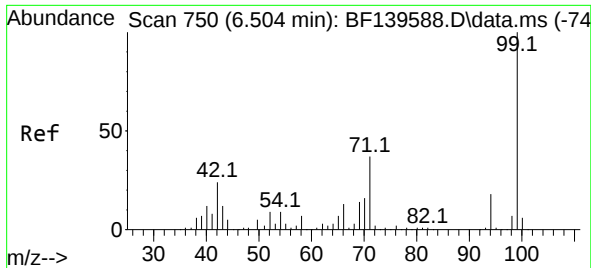

#7
Phenol-d6
Concen: 84.242 ng
RT: 6.498 min Scan# 74
Delta R.T. -0.006 min
Lab File: BF139710.D
Acq: 08 Oct 2024 14:05




Instrument :
BNA_F
ClientSampleId :
CONCRETE-RO


Tgt Ion: 99 Resp: 500573
Ion Ratio Lower Upper
99 100
42 22.7 19.1 28.7
71 36.0 29.7 44.5

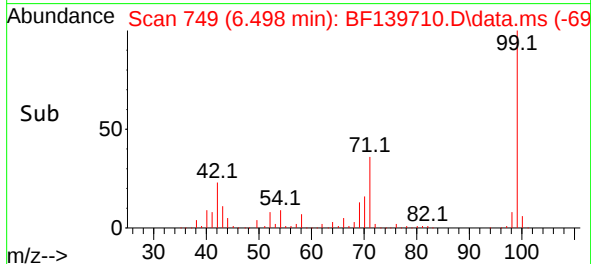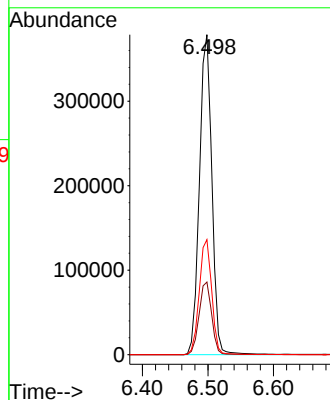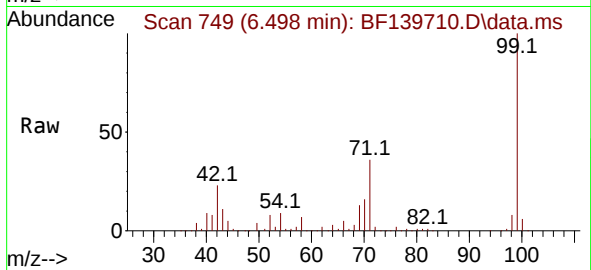

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.145 min Scan# 1029
Delta R.T. -0.006 min
Lab File: BF139710.D
Acq: 08 Oct 2024 14:05

Tgt Ion: 136 Resp: 277164
Ion Ratio Lower Upper
136 100
137 10.4 8.6 13.0
54 10.0 8.3 12.5
68 6.1 4.6 7.0


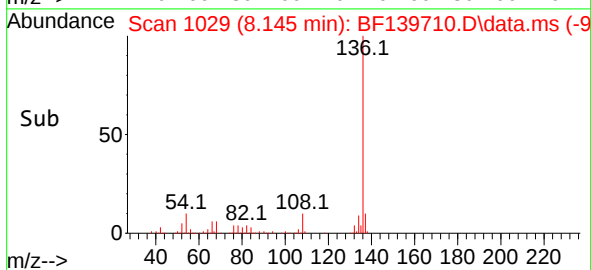
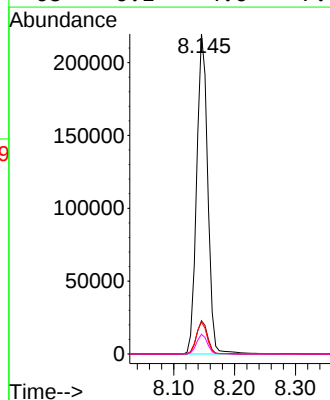
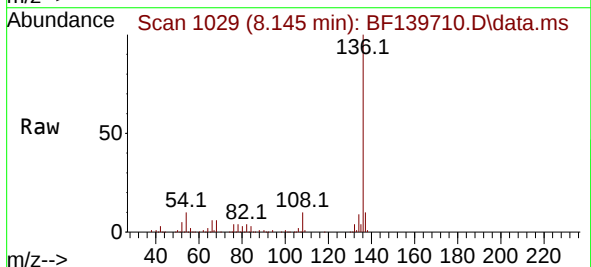


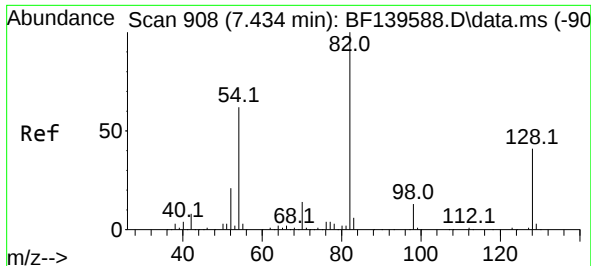

#23
Nitrobenzene-d5
Concen: 61.018 ng
RT: 7.428 min Scan# 908
Delta R.T. -0.006 min
Lab File: BF139710.D
Acq: 08 Oct 2024 14:05




Instrument :
BNA_F
ClientSampleId :
CONCRETE-RO


Tgt Ion: 82 Resp: 334029
Ion Ratio Lower Upper
82 100
128 42.2 32.4 48.6
54 59.6 49.1 73.7

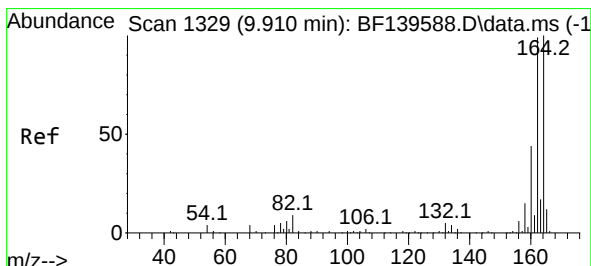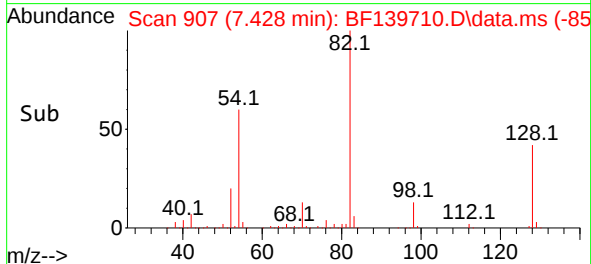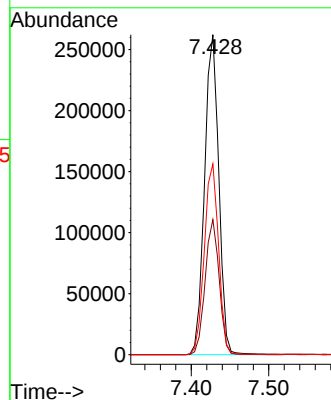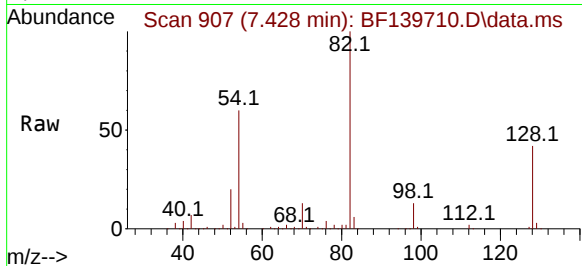

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.898 min Scan# 1327
Delta R.T. -0.012 min
Lab File: BF139710.D
Acq: 08 Oct 2024 14:05


Tgt Ion:164 Resp: 140632
Ion Ratio Lower Upper
164 100
162 99.0 79.4 119.0
160 42.7 35.1 52.7

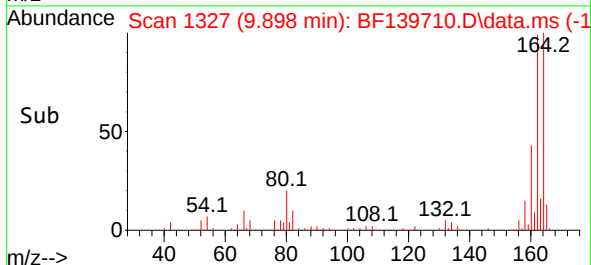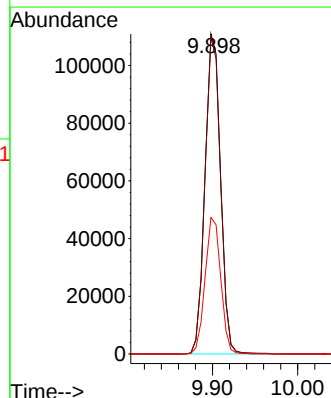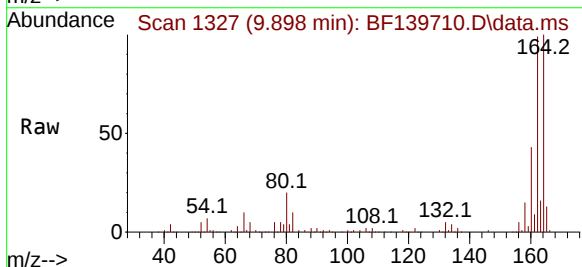



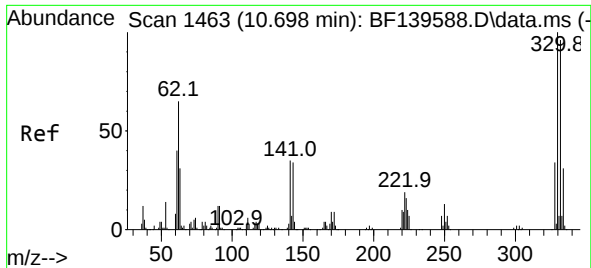


#42
2,4,6-Tribromophenol
Concen: 70.841 ng
RT: 10.692 min Scan# 1462
Delta R.T. -0.006 min
Lab File: BF139710.D
Acq: 08 Oct 2024 14:05

Instrument :
BNA_F
ClientSampleId :
CONCRETE-RO



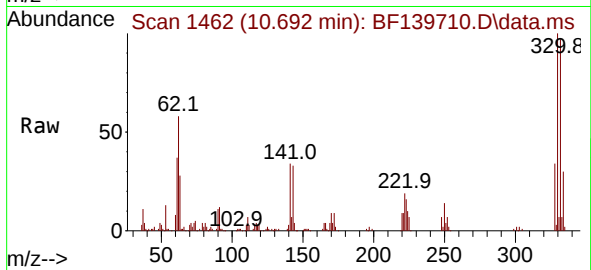



Tgt Ion:330 Resp: 96172
Ion Ratio Lower Upper
330 100
332 96.2 76.5 114.7
141 36.5 29.3 43.9

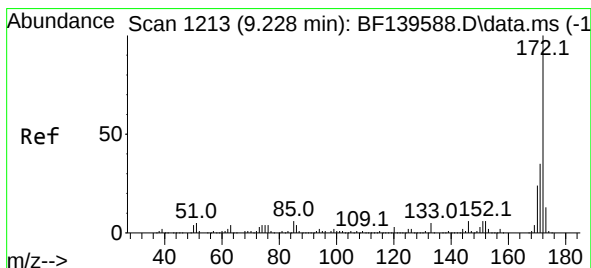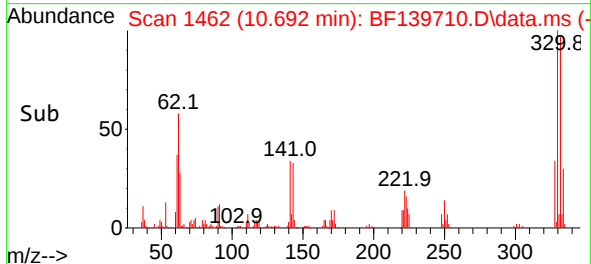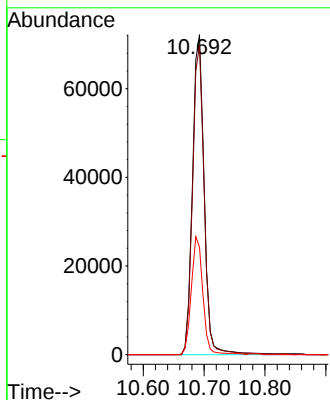

#45
2-Fluorobiphenyl
Concen: 67.289 ng
RT: 9.222 min Scan# 1212
Delta R.T. -0.006 min
Lab File: BF139710.D
Acq: 08 Oct 2024 14:05

Tgt Ion:172 Resp: 616404
Ion Ratio Lower Upper
172 100
171 35.2 28.2 42.4
170 23.5 18.8 28.2

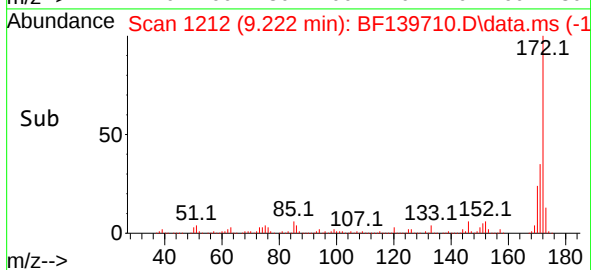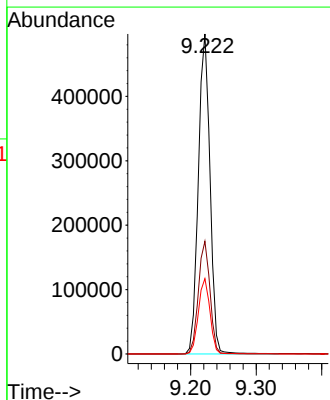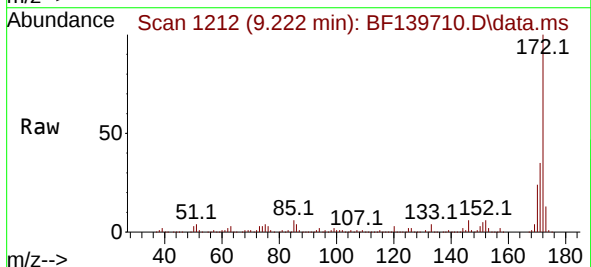

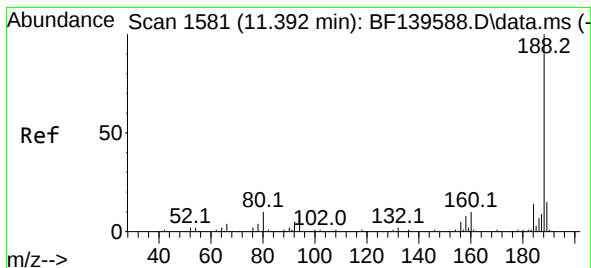

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.386 min Scan# 11

Delta R.T. -0.006 min

Lab File: BF139710.D

Acq: 08 Oct 2024 14:05

Instrument :

BNA_F

ClientSampleId :

CONCRETE-RO





Tgt Ion:188 Resp: 232617

Ion Ratio Lower Upper

188 100

94 9.5 7.4 11.2

80 10.0 8.2 12.2

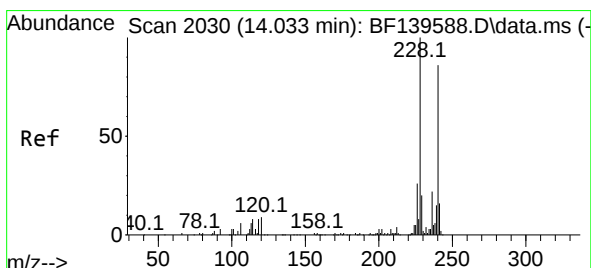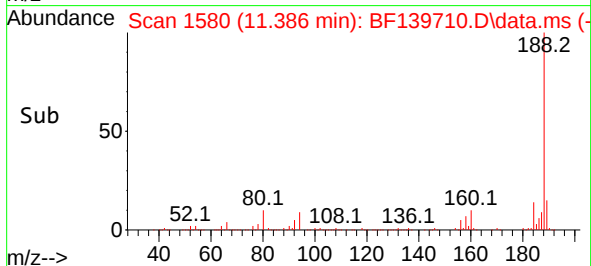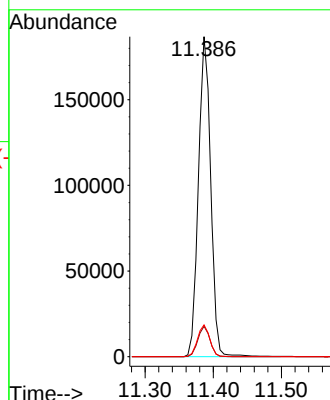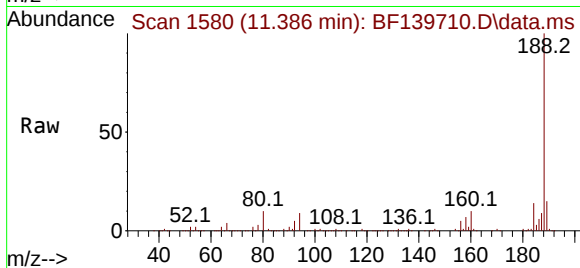

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.027 min Scan# 2029

Delta R.T. -0.006 min

Lab File: BF139710.D

Acq: 08 Oct 2024 14:05




Tgt Ion:240 Resp: 174990


Ion Ratio Lower Upper

240 100

120 10.1 8.4 12.6

236 25.7 20.3 30.5


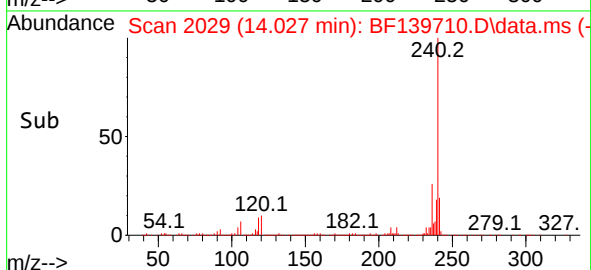
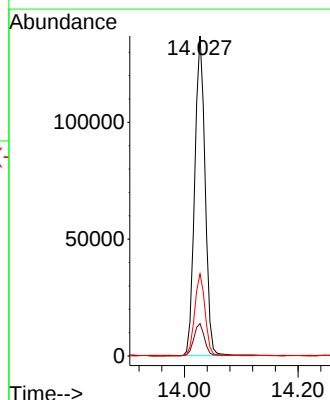
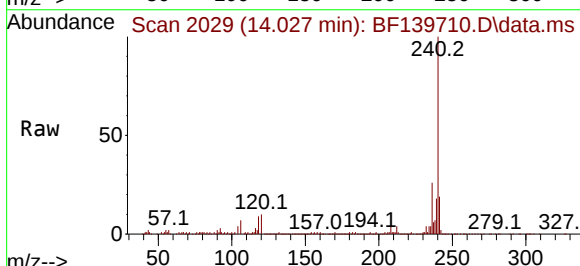


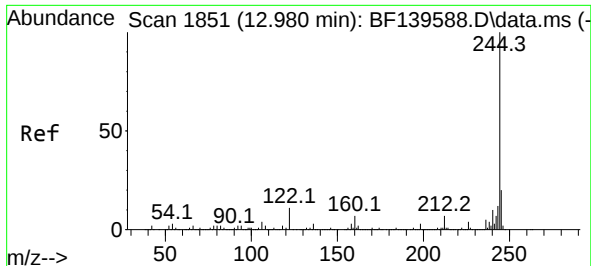

#79
 Terphenyl-d14
 Concen: 54.109 ng
 RT: 12.974 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF139710.D
 Acq: 08 Oct 2024 14:05

Instrument :
 BNA_F
 ClientSampleId :
 CONCRETE-RO

Tgt Ion:244 Resp: 577053
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.8 8.6
 122 10.3 8.6 12.8

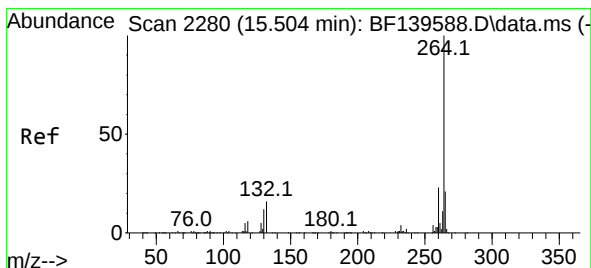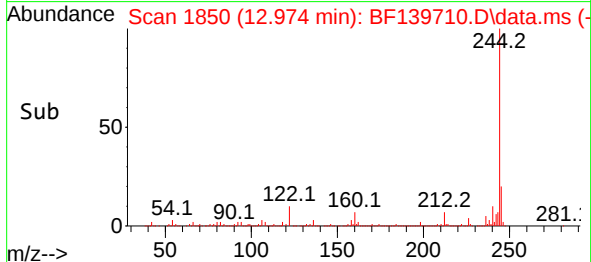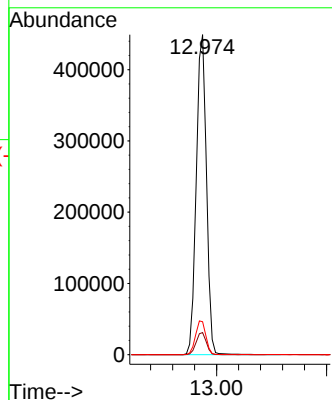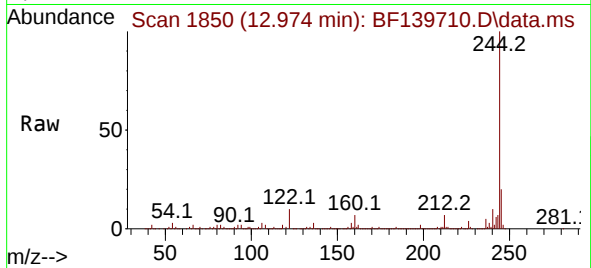

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.498 min Scan# 2279
 Delta R.T. -0.006 min
 Lab File: BF139710.D
 Acq: 08 Oct 2024 14:05

Tgt Ion:264 Resp: 143610
 Ion Ratio Lower Upper
 264 100
 260 23.6 18.7 28.1
 265 21.2 16.9 25.3

