


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100824\
Data File : BF139700.D
Acq On : 08 Oct 2024 09:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 02 04:58:47 2024

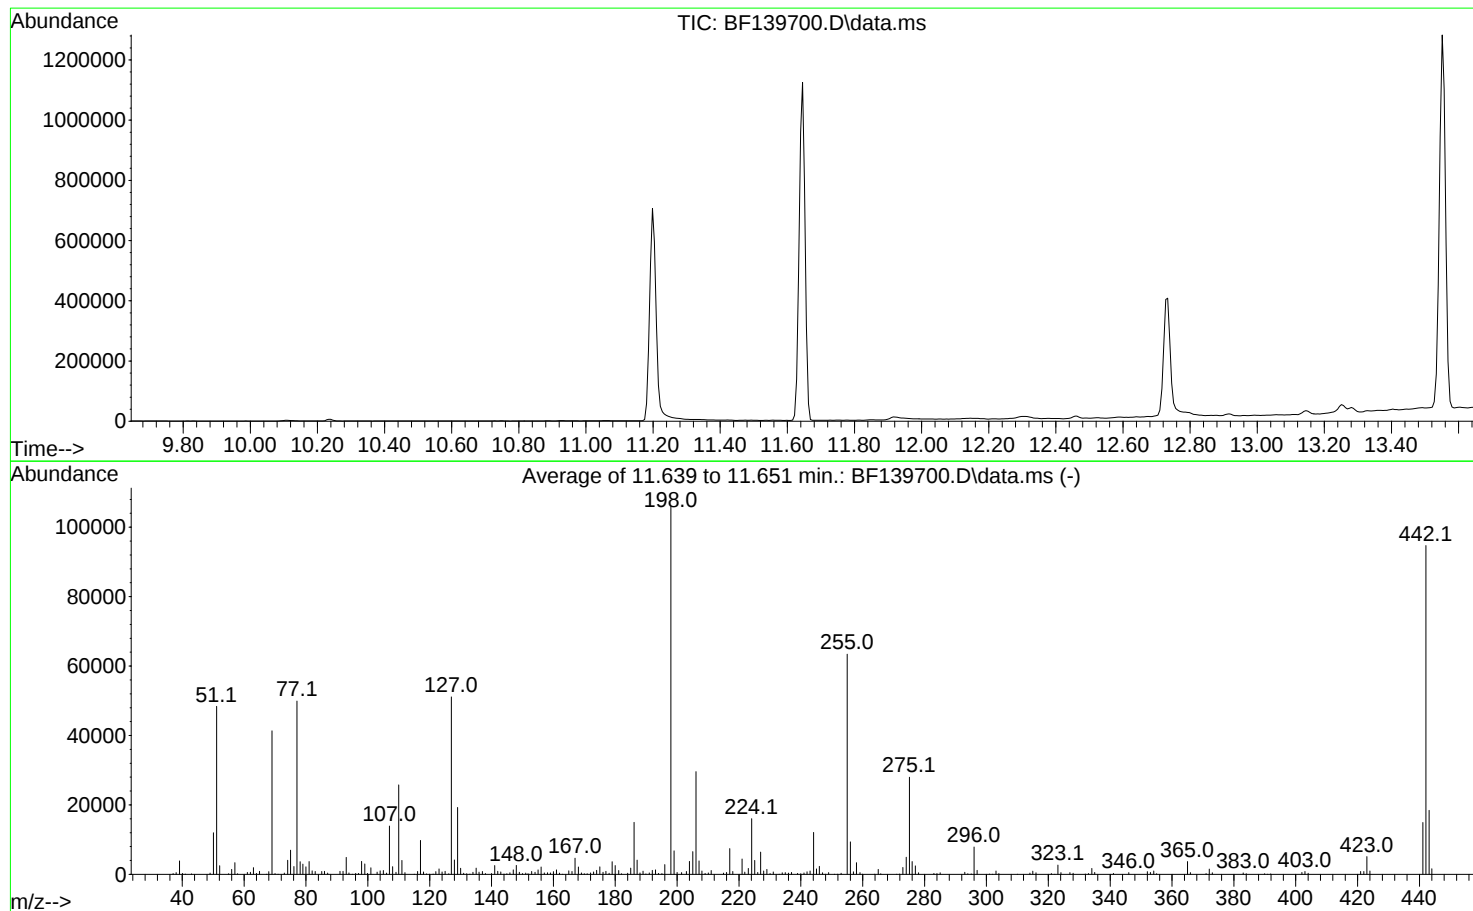




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	48395	PASS
68	69	0.00	2	1.9	785	PASS
69	198	0.00	100	39.0	41328	PASS
70	69	0.00	2	0.6	241	PASS
127	198	10	80	48.2	51115	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	105960	PASS
199	198	5	9	6.4	6770	PASS
275	198	10	60	26.4	27992	PASS
365	198	1	100	3.5	3681	PASS
441	198	0.01	100	14.1	14946	PASS
442	442	50	100	100.0	94704	PASS
443	442	15	24	19.4	18417	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100824\
Data File : BF139700.D
Acq On : 08 Oct 2024 09:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 08 11:36:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

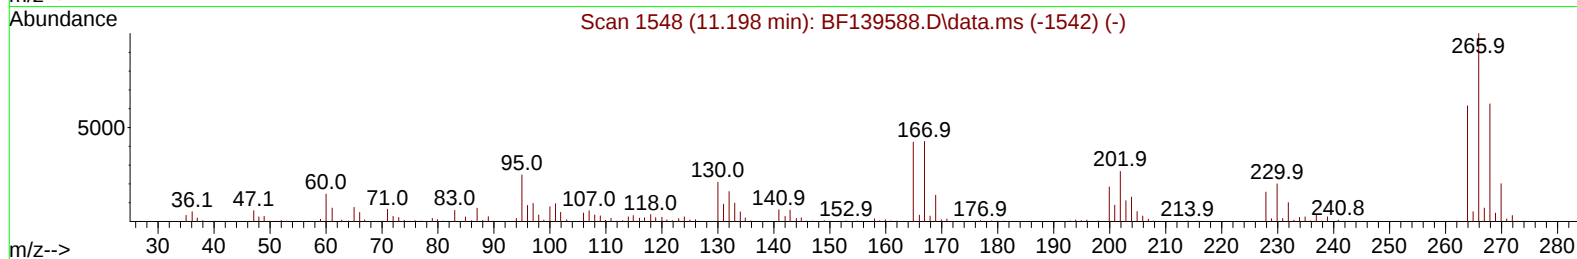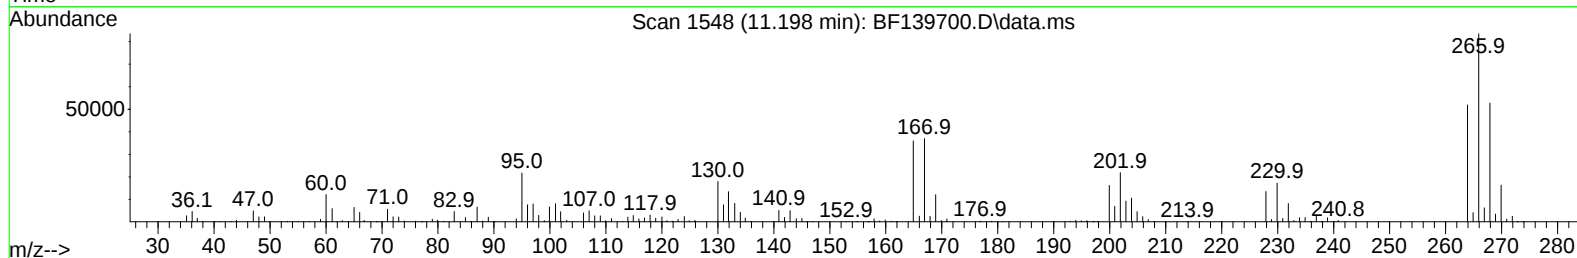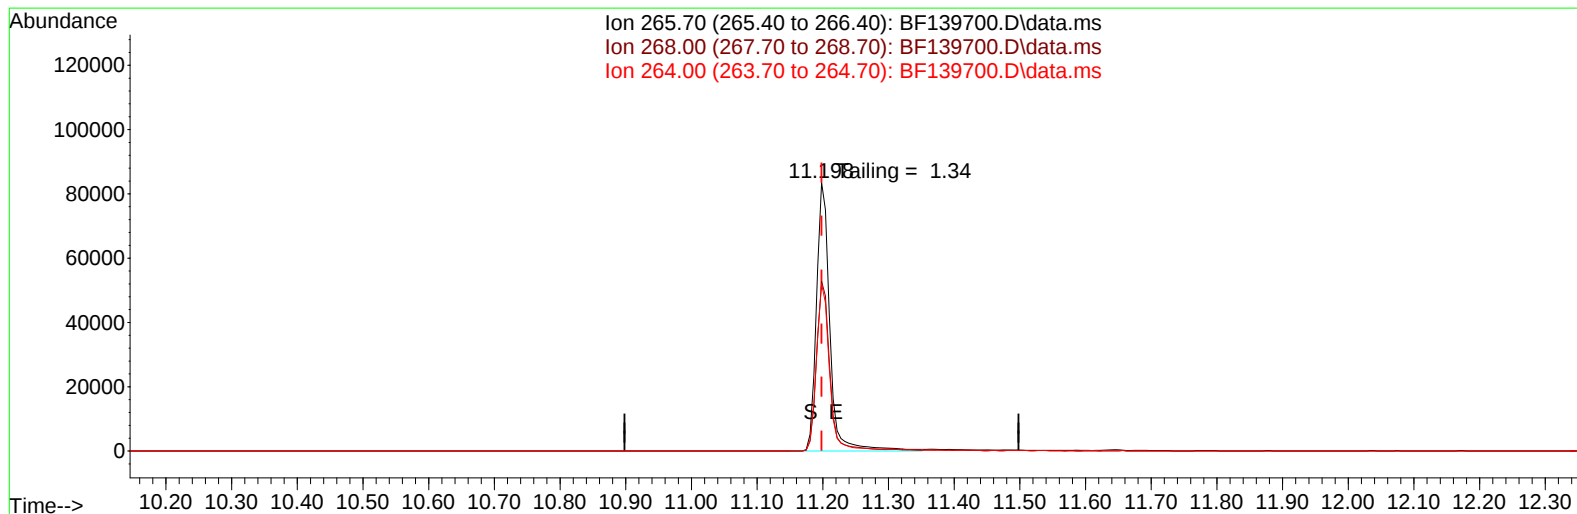

TIC: BF139700.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 34412.57 ng




response 119596

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	63.21
264.00	61.60	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100824\
Data File : BF139700.D
Acq On : 08 Oct 2024 09:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 08 11:36:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

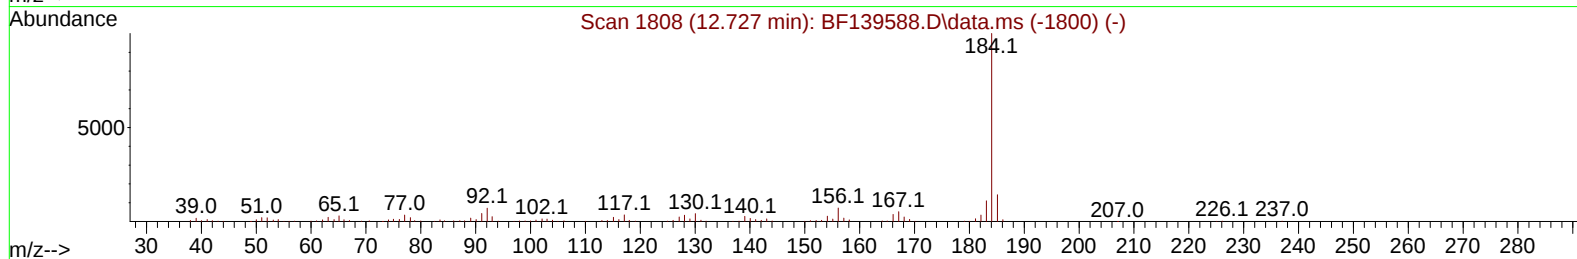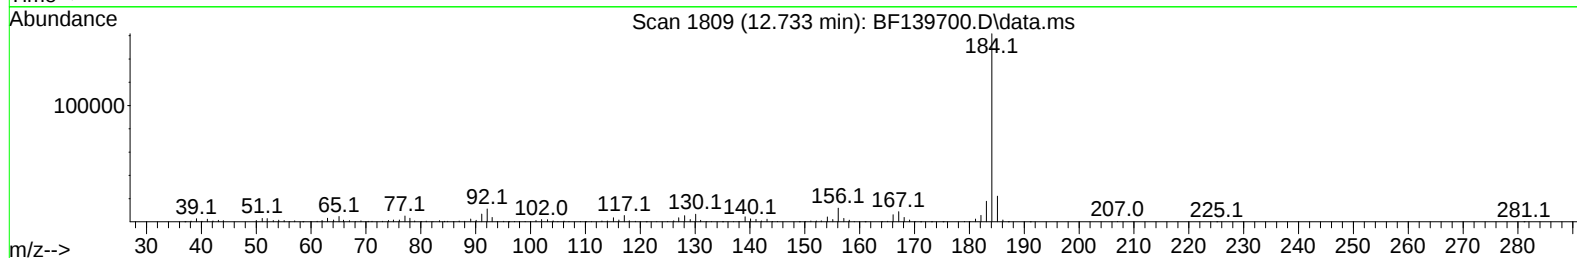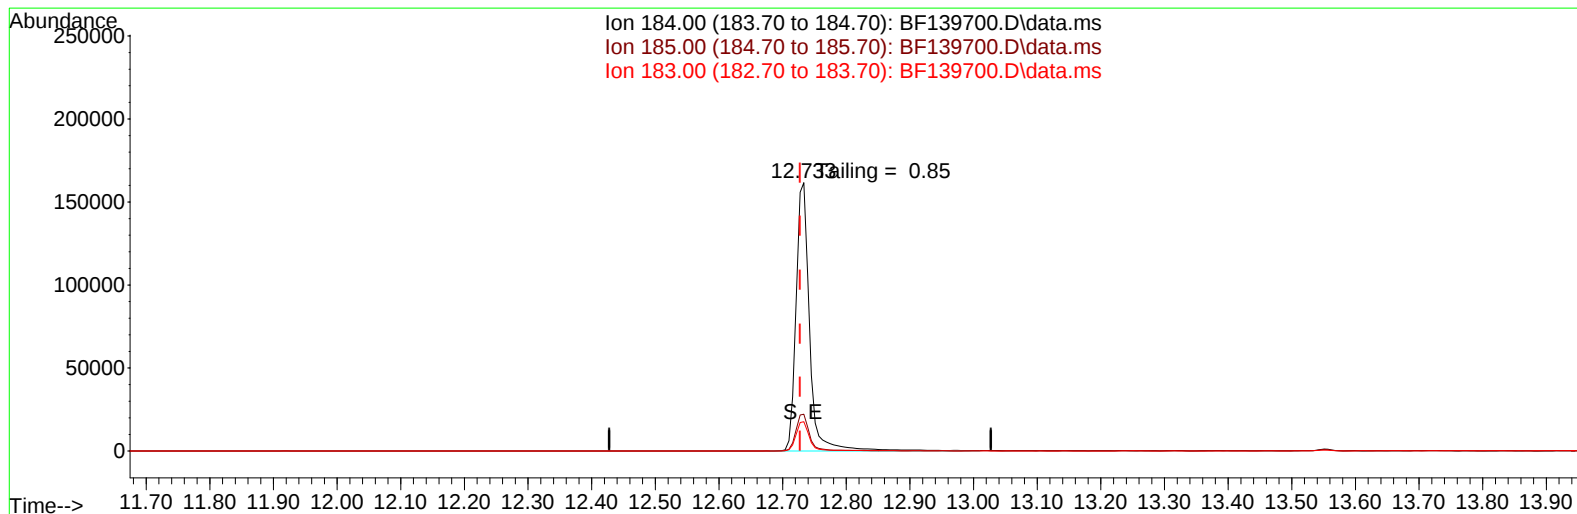

TIC: BF139700.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 113702.93 ng

response 236659

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.72
183.00	11.00	10.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/8/2024	BNA_F	<u>BF139700.D</u>
Compound Name	Response	Retention Time
DDT	303953	13.551
DDD	4867	13.251
DDE	1216	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6083	310036	1.96

Instrument :
BNA_F
ClientSampleId :
DFTPP