
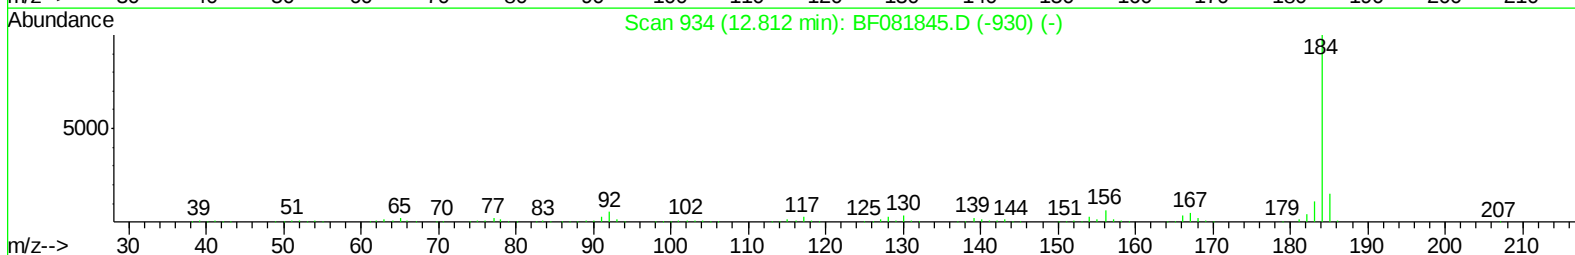
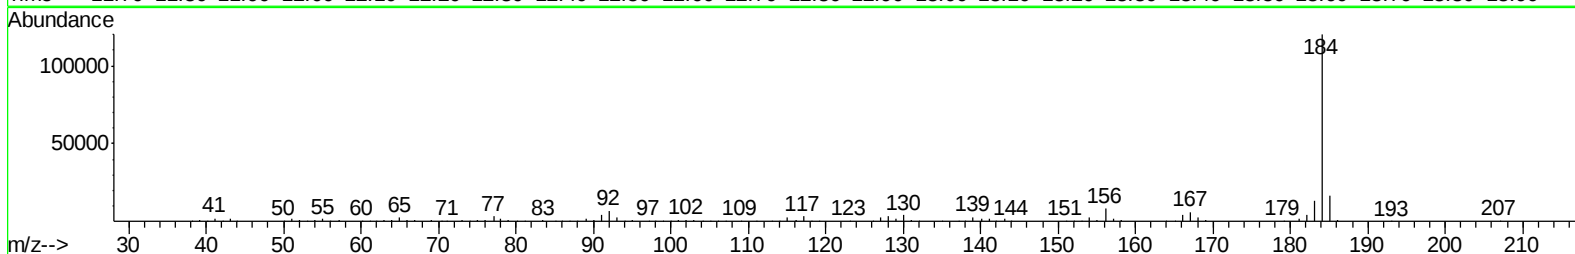


Data Path : Z:\HPCHEM1\BNA F\Data\BF100915\
Data File : BF082142.D
Acq On : 9 Oct 2015 13:16
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 08:15:25 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 08 02:46:05 2015
Response via : Initial Calibration

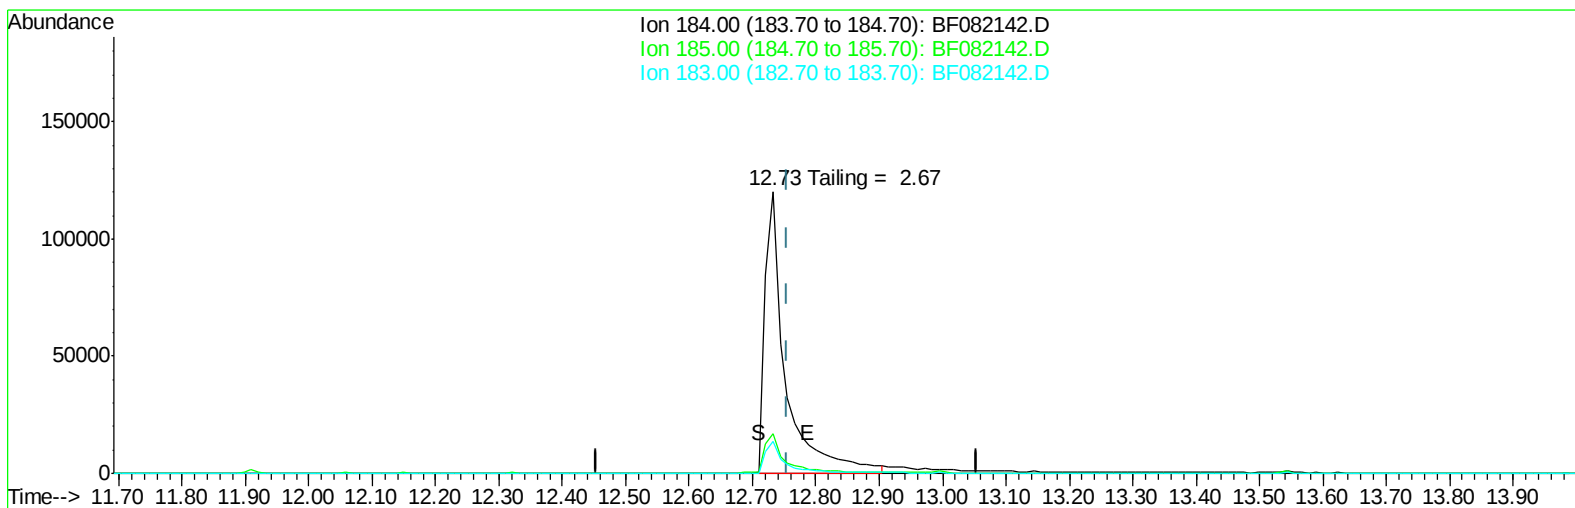

TIC: BF082142.D

(76) Benzidine




12.732min (-0.023) 0.00ng m

response 272092

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.10
183.00	9.50	11.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF100915\
Data File : BF082142.D
Acq On : 9 Oct 2015 13:16
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 08:15:25 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 08 02:46:05 2015
Response via : Initial Calibration

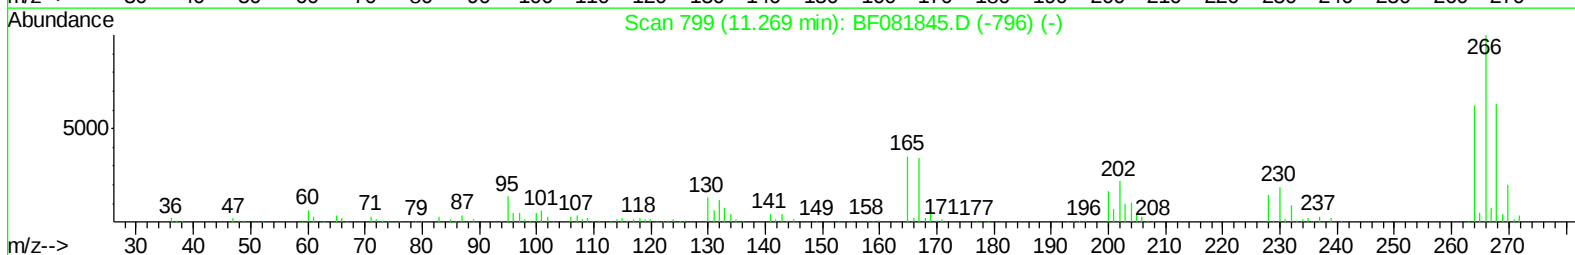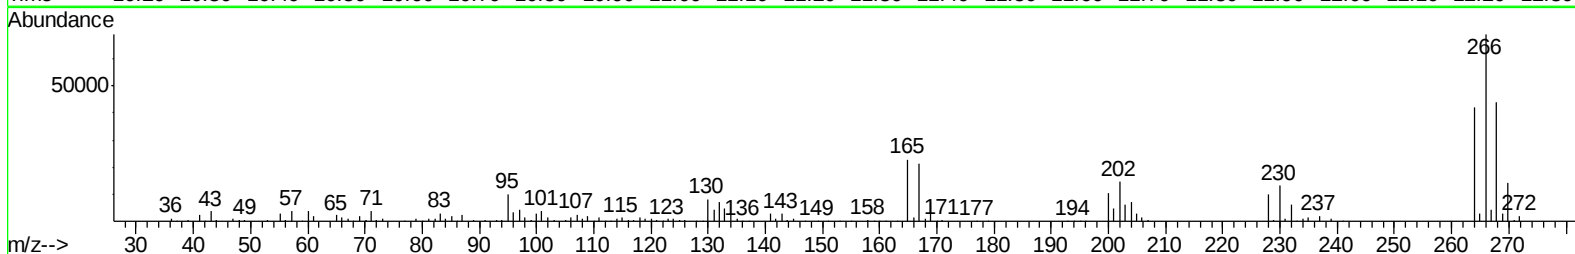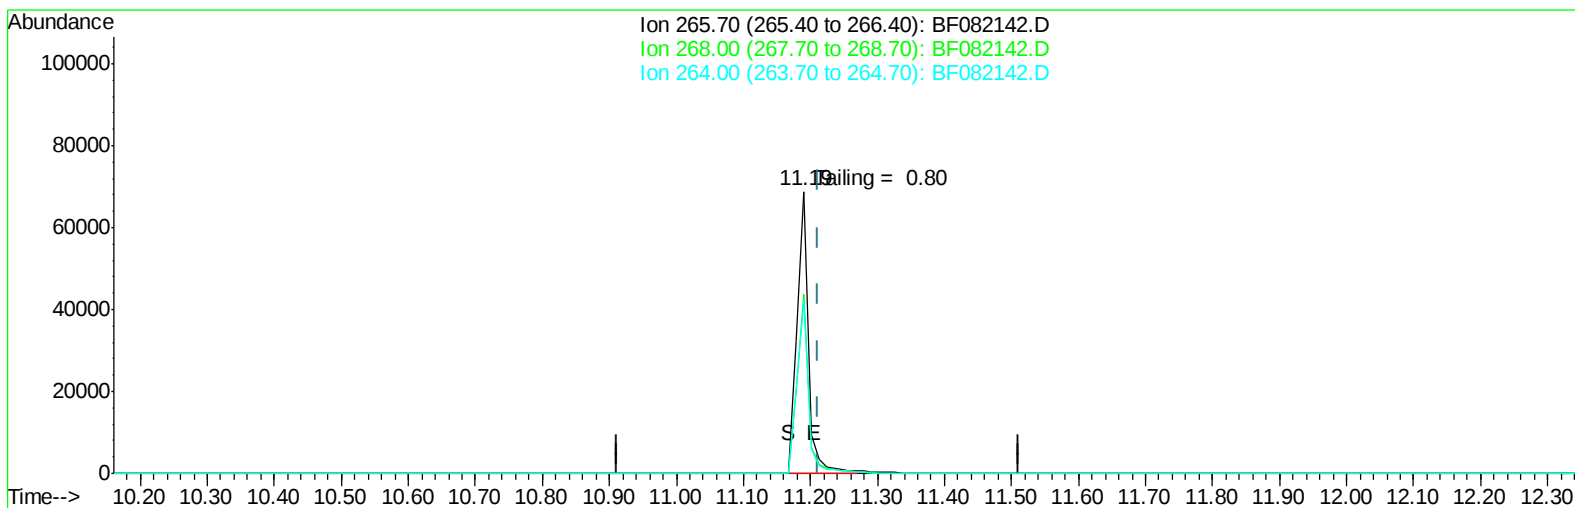

TIC: BF082142.D

(69) Pentachlorophenol (C)

11.189min (-0.023) 35134.59ng

response 82920

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.76
264.00	62.70	61.42
0.00	0.00	0.00