

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100915\
 Data File : BF082152.D
 Acq On : 9 Oct 2015 18:41
 Operator : UM/IZ
 Sample : G3963-02DL 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PROPOSED-FILL(BESM)DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.017	250	252	260	rVB	425722	586454	31.82%	1.778%
2	5.440	287	289	292	rBV	1078454	1027150	55.73%	3.114%
3	6.480	378	380	387	rBV	1099625	1120322	60.79%	3.397%
4	6.617	389	392	394	rVV	1056096	1195758	64.88%	3.626%
5	6.674	394	397	400	rVB	67794	80069	4.34%	0.243%
6	6.846	410	412	416	rBV	621963	633438	34.37%	1.921%
7	7.006	423	426	428	rBV	965791	980239	53.19%	2.972%
8	7.417	460	462	464	rBV	702216	723419	39.25%	2.193%
9	8.137	521	525	529	rBV2	907240	1088134	59.04%	3.299%
10	8.720	574	576	579	rVB	80336	96699	5.25%	0.293%
11	8.846	586	587	590	rBV2	47823	57982	3.15%	0.176%
12	8.949	594	596	598	rBV2	58714	66721	3.62%	0.202%
13	9.212	617	619	622	rBV	1358710	1381510	74.96%	4.189%
14	9.292	624	626	627	rVV	141369	119706	6.50%	0.363%
15	9.555	645	649	652	rVV3	44576	109083	5.92%	0.331%
16	9.612	652	654	656	rVV	329570	309134	16.77%	0.937%
17	9.749	664	666	669	rBV	100421	125466	6.81%	0.380%
18	9.818	671	672	674	rVB	130961	114629	6.22%	0.348%
19	9.898	676	679	680	rVV	757743	855222	46.40%	2.593%
20	9.921	680	681	684	rVV	118373	140481	7.62%	0.426%
21	10.092	694	696	698	rBV	71180	103249	5.60%	0.313%
22	10.138	698	700	702	rVB2	39077	47517	2.58%	0.144%
23	10.298	712	714	715	rBV	41106	63718	3.46%	0.193%
24	10.321	715	716	718	rVB	166934	117253	6.36%	0.356%
25	10.435	725	726	729	rBV	114709	157865	8.57%	0.479%
26	10.538	733	735	739	rBV3	44768	76018	4.12%	0.230%
27	10.686	745	748	750	rBV	606618	762394	41.37%	2.312%
28	10.789	756	757	762	rVB	156021	254958	13.83%	0.773%
29	10.983	771	774	776	rBV3	48820	87933	4.77%	0.267%
30	11.132	783	787	790	rBV3	30023	80053	4.34%	0.243%
31	11.189	790	792	794	rBV	51380	56218	3.05%	0.170%
32	11.235	794	796	798	rBV2	99766	170068	9.23%	0.516%
33	11.269	798	799	802	rVB2	83745	114683	6.22%	0.348%
34	11.384	806	809	810	rBV	724545	898679	48.76%	2.725%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100915\
 Data File : BF082152.D
 Acq On : 9 Oct 2015 18:41
 Operator : UM/IZ
 Sample : G3963-02DL 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PROPOSED-FILL(BESM)DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.406	810	811	814	rVV	1517990	1246080	67.61%	3.778%
36	11.452	814	815	817	rVB	208513	212659	11.54%	0.645%
37	11.612	826	829	832	rVV2	123146	216398	11.74%	0.656%
38	11.669	832	834	837	rVV2	156558	175358	9.51%	0.532%
39	11.875	850	852	854	rBV	111443	197042	10.69%	0.597%
40	11.909	854	855	857	rVV	268528	232686	12.63%	0.706%
41	11.955	857	859	861	rVV2	48906	75823	4.11%	0.230%
42	11.989	861	862	867	rVB	269353	407452	22.11%	1.235%
43	12.081	867	870	871	rBV	82518	130404	7.08%	0.395%
44	12.115	871	873	875	rVB	41879	59188	3.21%	0.179%
45	12.172	877	878	880	rBV	70343	129020	7.00%	0.391%
46	12.206	880	881	883	rVB	125129	92286	5.01%	0.280%
47	12.435	898	901	902	rBV	71855	113981	6.18%	0.346%
48	12.469	902	904	907	rVB	110353	153869	8.35%	0.467%
49	12.515	907	908	912	rVB	80053	93697	5.08%	0.284%
50	12.595	912	915	918	rBV	1839779	1843019	100.00%	5.588%
51	12.686	922	923	925	rVB	96344	79099	4.29%	0.240%
52	12.744	925	928	930	rBV2	59218	92336	5.01%	0.280%
53	12.824	930	935	938	rBV	1358105	1729157	93.82%	5.243%
54	12.869	938	939	941	rVB2	76423	78979	4.29%	0.239%
55	12.961	945	947	951	rVB	767289	1208481	65.57%	3.664%
56	13.041	951	954	956	rBV2	107405	175269	9.51%	0.531%
57	13.155	960	964	966	rBV2	180557	325398	17.66%	0.987%
58	13.212	966	969	971	rBV2	113837	232423	12.61%	0.705%
59	13.258	971	973	976	rVB	118304	189179	10.26%	0.574%
60	13.349	979	981	982	rVB	50415	54027	2.93%	0.164%
61	13.372	982	983	987	rVB2	48030	81741	4.44%	0.248%
62	13.498	992	994	995	rVB2	35041	47570	2.58%	0.144%
63	13.532	995	997	1004	rBV4	82995	216630	11.75%	0.657%
64	13.658	1004	1008	1012	rBV	123749	201885	10.95%	0.612%
65	13.772	1015	1018	1019	rBV2	137392	188721	10.24%	0.572%
66	13.864	1024	1026	1029	rVB	229150	299276	16.24%	0.907%
67	14.024	1036	1040	1041	rBV2	958161	1644389	89.22%	4.986%
68	14.184	1050	1054	1056	rBV3	88234	175500	9.52%	0.532%
69	14.230	1056	1058	1059	rVV2	34794	58456	3.17%	0.177%
70	14.412	1066	1074	1075	rBV2	122279	319508	17.34%	0.969%
71	14.447	1075	1077	1079	rVB3	65322	80083	4.35%	0.243%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100915\
 Data File : BF082152.D
 Acq On : 9 Oct 2015 18:41
 Operator : UM/IZ
 Sample : G3963-02DL 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PROPOSED-FILL(BESM)DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	14.492	1079	1081	1083	rBV2	88320	158185	8.58%	0.480%
73	14.550	1083	1086	1088	rVB4	70288	149374	8.10%	0.453%
74	14.721	1098	1101	1102	rBV2	29586	58192	3.16%	0.176%
75	14.790	1105	1107	1109	rVV2	78870	103872	5.64%	0.315%
76	14.892	1114	1116	1118	rVV2	55086	87112	4.73%	0.264%
77	15.052	1127	1130	1134	rBV	673148	1452118	78.79%	4.403%
78	15.110	1134	1135	1137	rVV2	71349	121264	6.58%	0.368%
79	15.155	1137	1139	1141	rVV	131537	171628	9.31%	0.520%
80	15.247	1145	1147	1150	rBV3	35501	98226	5.33%	0.298%
81	15.338	1153	1155	1158	rVV	281181	469688	25.48%	1.424%
82	15.407	1158	1161	1164	rVV	509704	641119	34.79%	1.944%
83	15.464	1164	1166	1173	rVB2	401066	777791	42.20%	2.358%
84	15.681	1183	1185	1188	rVB2	40111	67141	3.64%	0.204%
85	15.898	1200	1204	1206	rBV2	52582	109144	5.92%	0.331%
86	15.944	1206	1208	1211	rVV4	29051	79110	4.29%	0.240%
87	16.001	1211	1213	1219	rVV	38354	90445	4.91%	0.274%
88	16.138	1223	1225	1232	rVB	16592	53375	2.90%	0.162%
89	16.550	1255	1261	1269	rVB9	25657	115191	6.25%	0.349%
90	16.721	1269	1276	1283	rVB3	36765	157963	8.57%	0.479%
91	16.881	1286	1290	1294	rBV2	184575	394628	21.41%	1.197%
92	16.961	1294	1297	1301	rVB2	26546	64653	3.51%	0.196%
93	17.053	1301	1305	1307	rBV	39310	88559	4.81%	0.269%
94	17.110	1307	1310	1313	rBV	24582	52332	2.84%	0.159%
95	17.304	1323	1327	1334	rBV	137188	313286	17.00%	0.950%
96	17.533	1344	1347	1356	rVB2	31500	92726	5.03%	0.281%
97	18.424	1421	1425	1433	rVB8	12525	56587	3.07%	0.172%
98	19.476	1511	1517	1526	rVB2	31126	134104	7.28%	0.407%
99	19.659	1528	1533	1537	rBV	21777	86930	4.72%	0.264%
100	20.653	1616	1620	1629	rVB3	18204	76826	4.17%	0.233%


Sum of corrected areas: 32980860

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100915\
Data File : BF082152.D
Acq On : 9 Oct 2015 18:41
Operator : UM/IZ
Sample : G3963-02DL 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PROPOSED-FILL(BESM)DL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

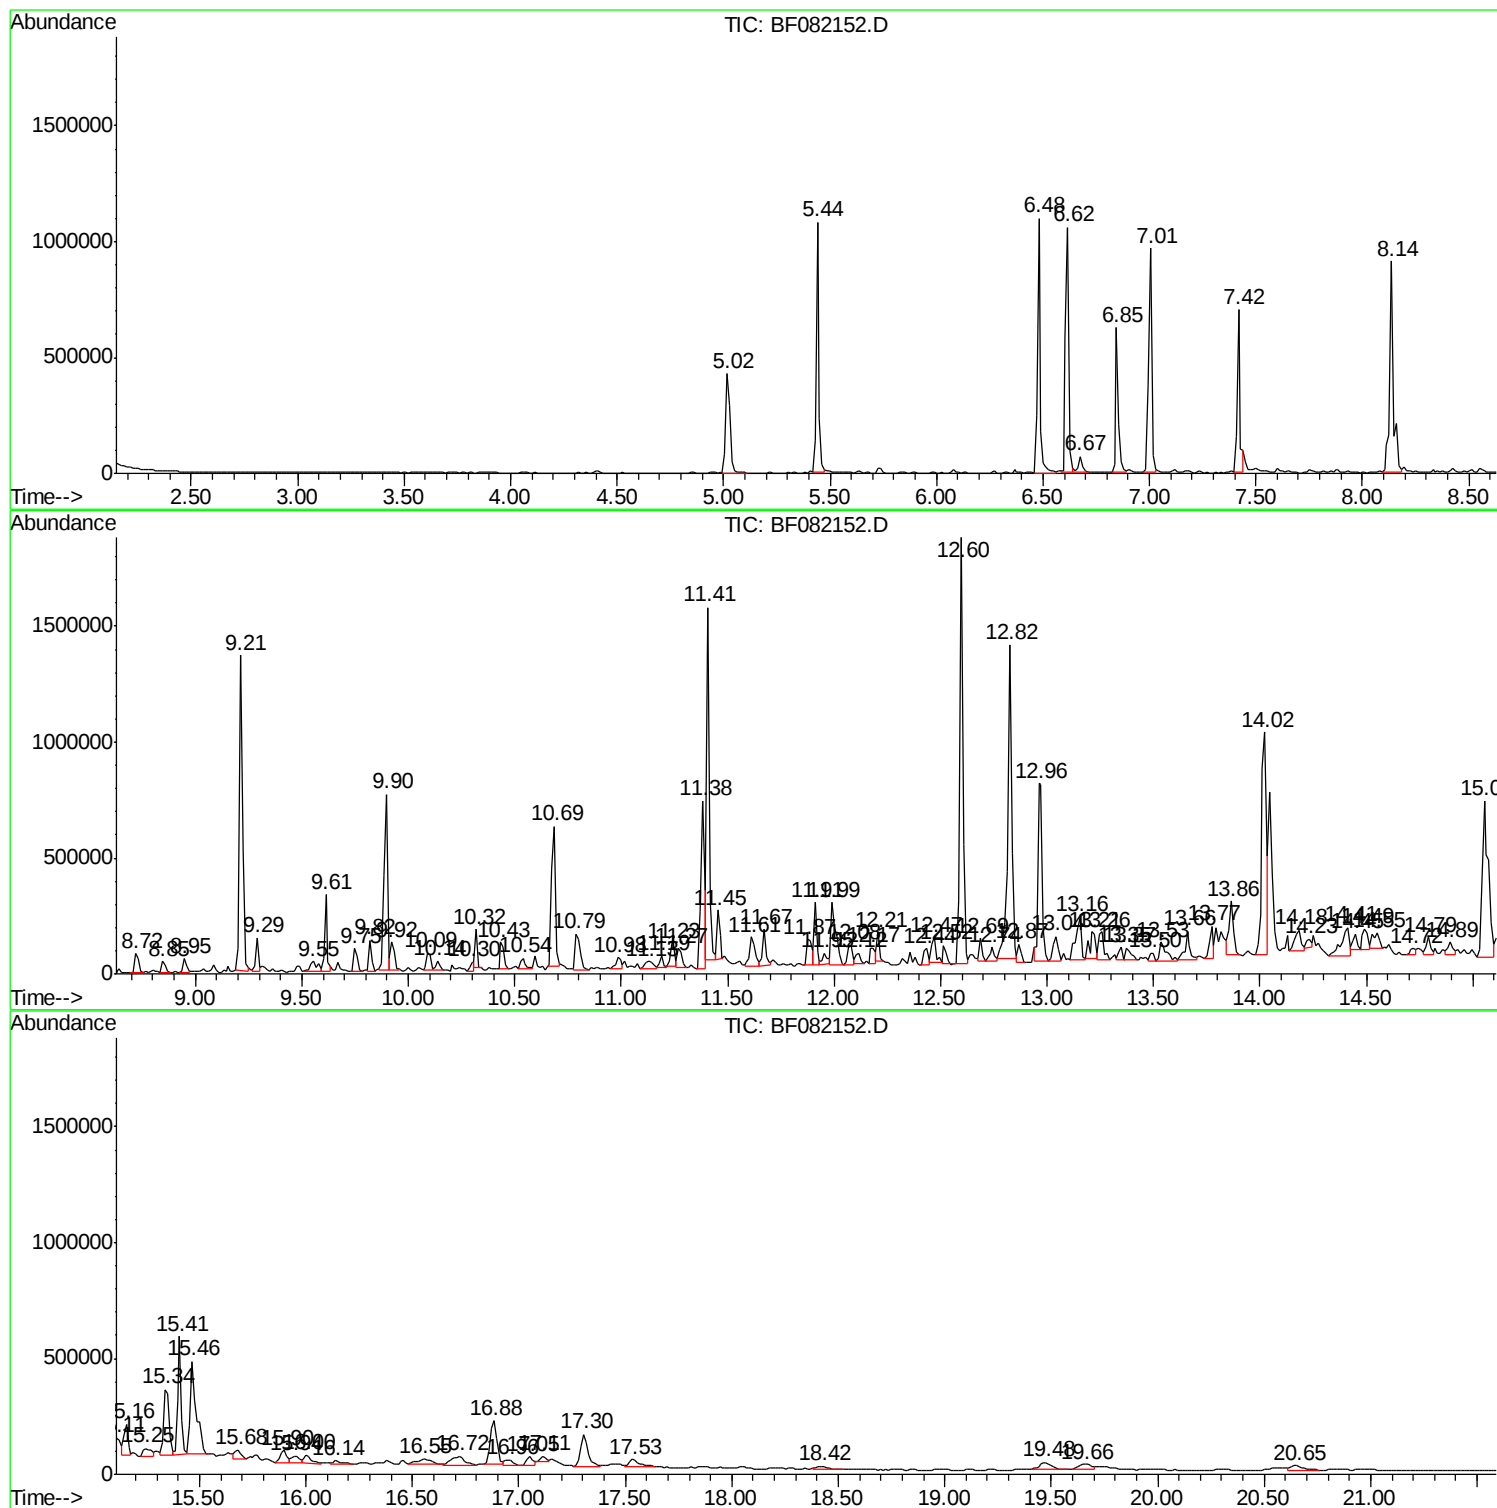

DbaaaPathh::ZZ\NRPBEMM1BBAFNDAAABBE000955\
 DbaaaFile::BB0022522DD
 Aeqq00n :: 9900tt20055 188441
 Oppaaaor ::UMMIZZ
 Saaapbe ::G09063000DL2XX
 MMsC ::
 AASSVaal ::111 SaaapbeMMuipbeer:11

Instrument :
 BNA_F
 ClientSampleId :
 PROPOSED-FILL(BESM)DL

QQaantMebbdd::ZZ\NRPBEMM1BBAFMEEMH00S88200BB002285MM
 QQaantTife ::ASBPBNASSAN0ABBSF00R55P000NTCAILBRATION

TICCLibbaay ::CC\DAABASSEN0SS002LL
 TICInteggaionPaaameess:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
