


Data Path : Z:\HPCHEM1\BNA_F\Data\BF100915\
 Data File : BF082142.D
 Acq On : 9 Oct 2015 13:16
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 08 02:46:05 2015

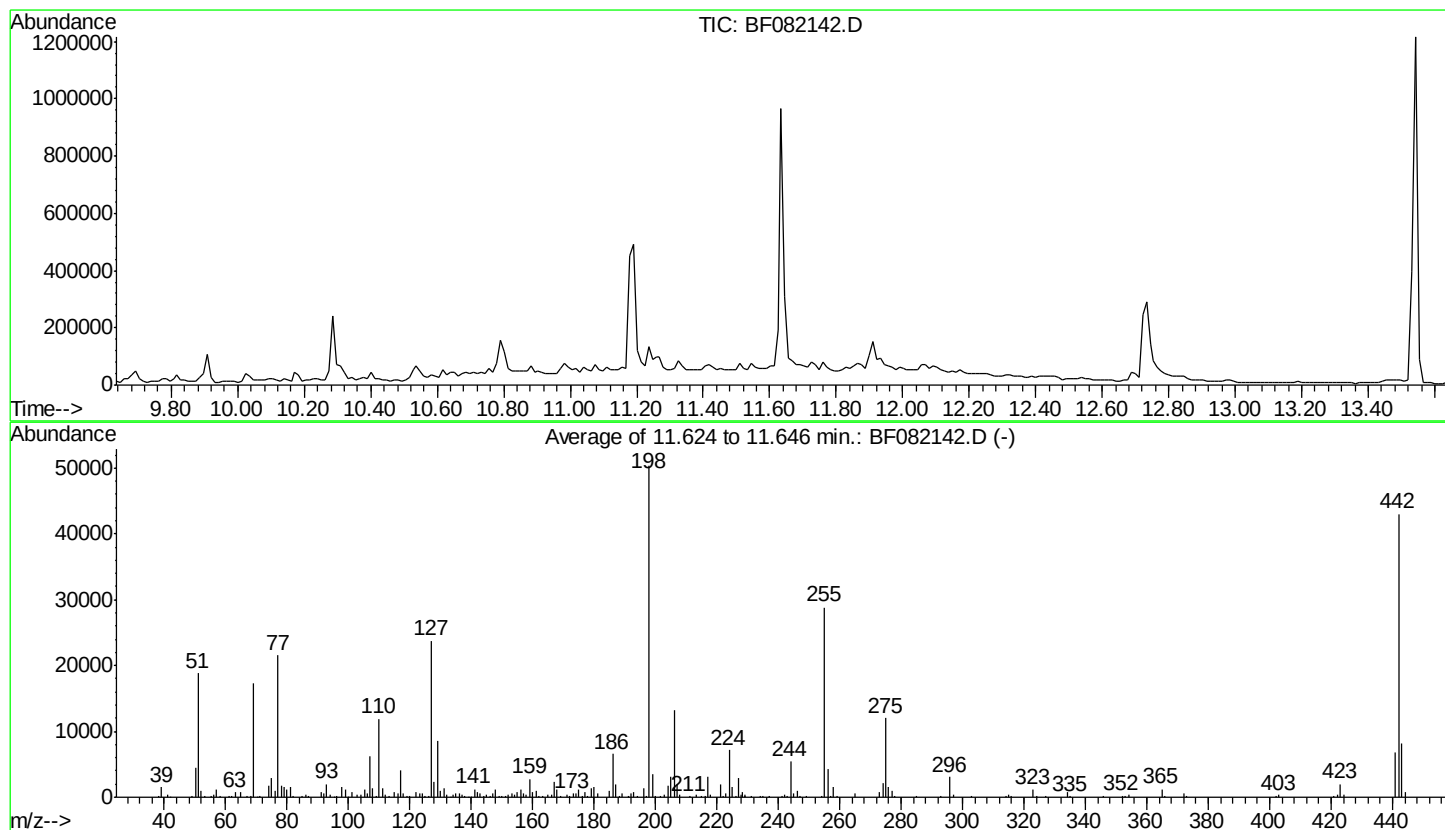

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	18843	PASS
68	69	0.00	2	1.3	227	PASS
69	198	0.00	100	34.6	17400	PASS
70	69	0.00	2	0.4	77	PASS
127	198	10	80	47.1	23736	PASS
197	198	0.00	2	0.4	210	PASS
198	198	100	100	100.0	50353	PASS
199	198	5	9	6.8	3416	PASS
275	198	10	60	23.9	12027	PASS
365	198	1	100	2.4	1229	PASS
441	442	0.01	24	15.8	6780	PASS
442	198	50	100	85.5	43041	PASS
443	442	15	24	18.9	8134	PASS