
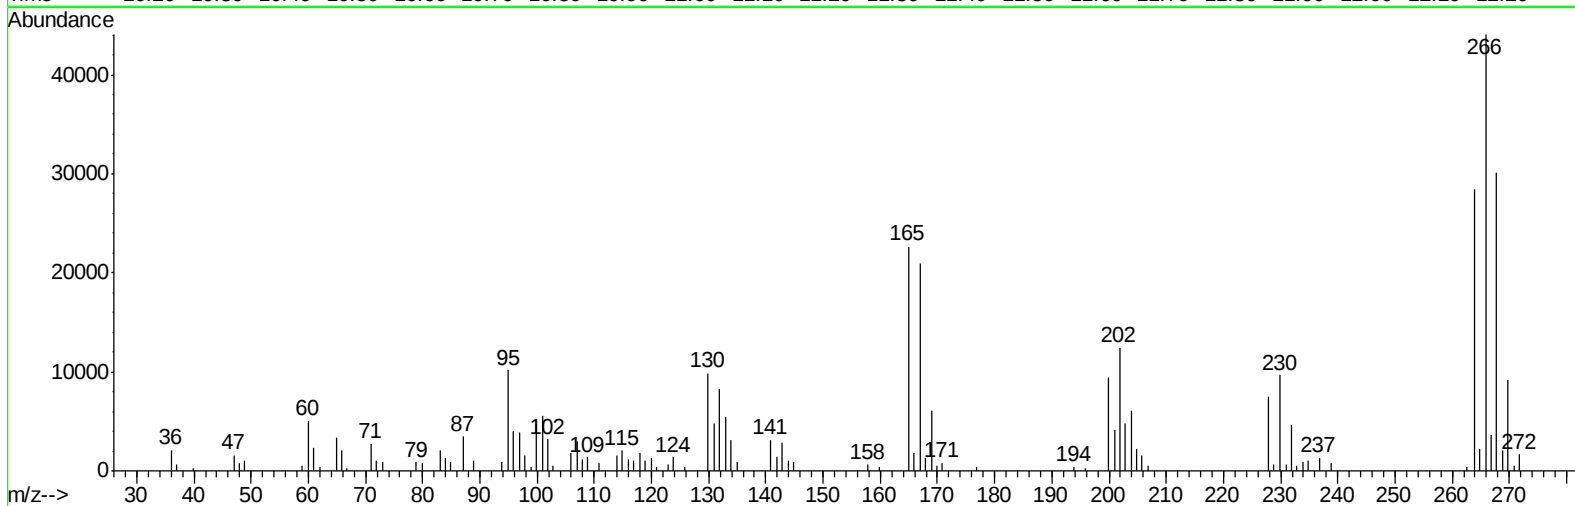


Data Path : Z:\HPCHEM1\BNA F\DATA\BF100917\
Data File : BF099258.D
Acq On : 9 Oct 2017 13:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 10 07:26:32 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

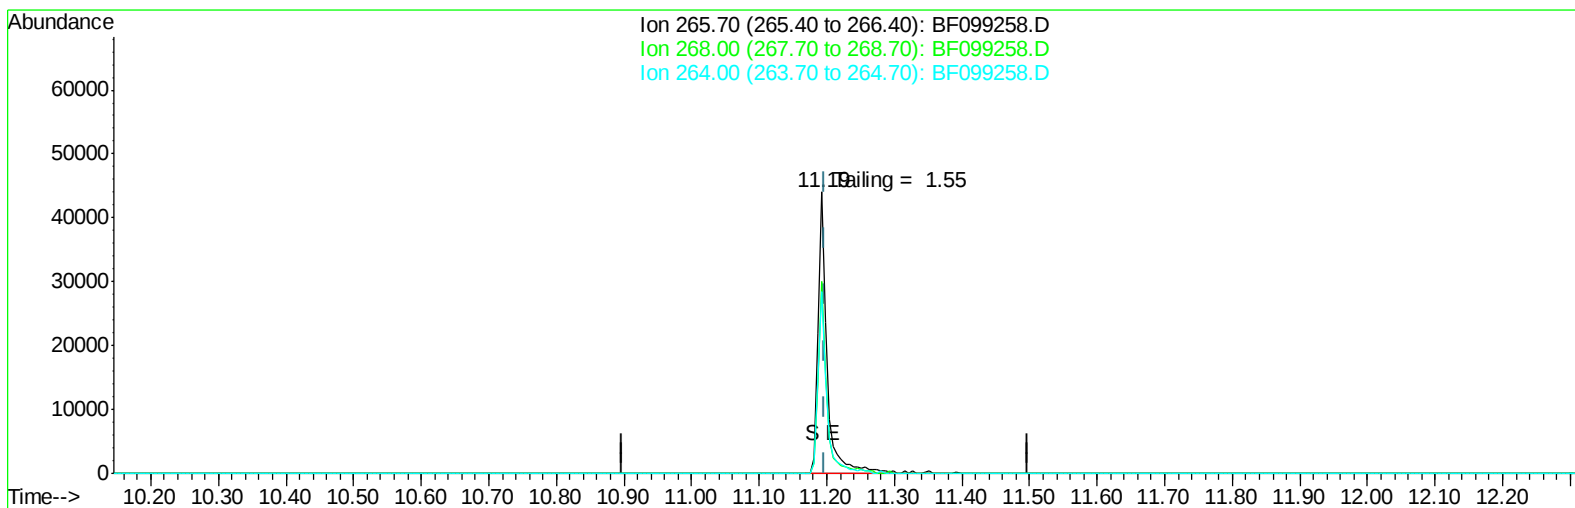

TIC: BF099258.D

(69) Pentachlorophenol (C)



11.192min (-0.006) 19377.03ng

response 42361

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.23
264.00	61.90	64.55
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100917\
Data File : BF099258.D
Acq On : 9 Oct 2017 13:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 10 07:26:32 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

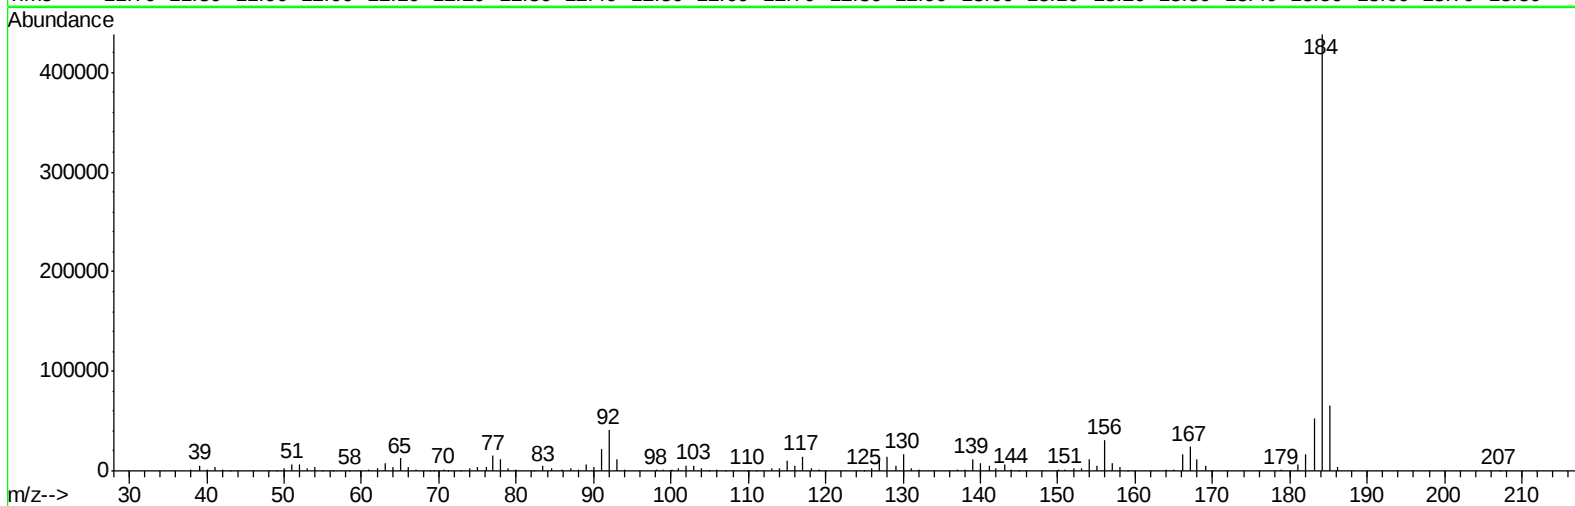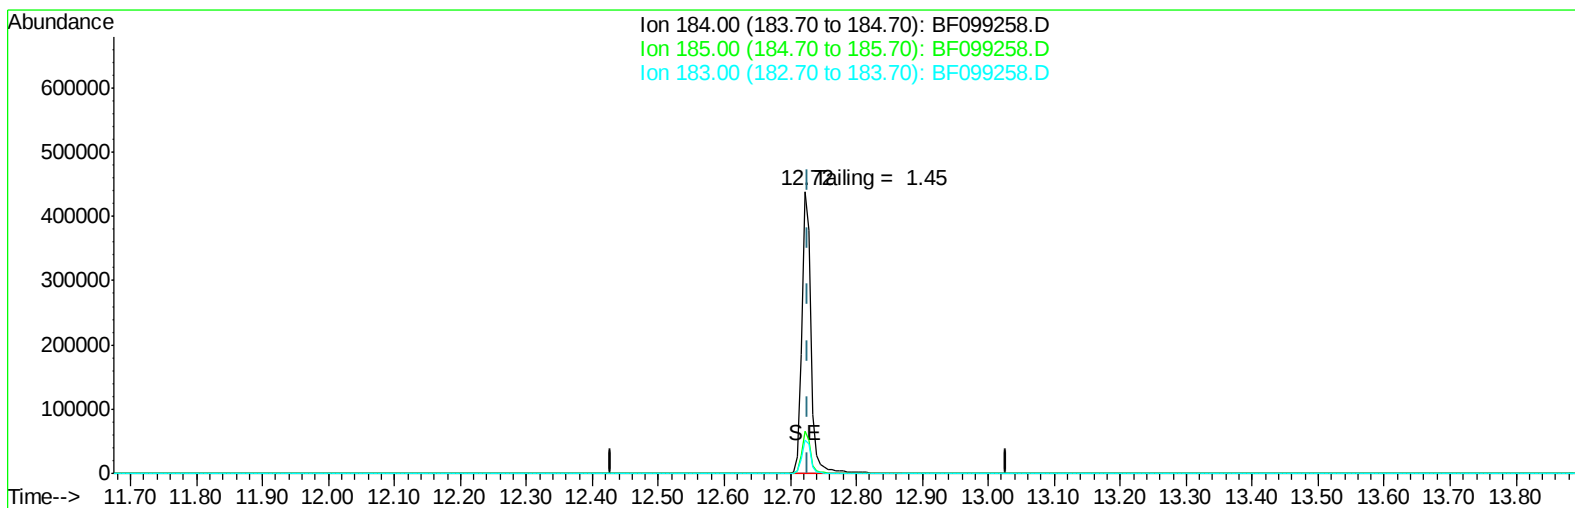

TIC: BF099258.D

(76) Benzidine

12.722min (-0.006) 0.00ng

response 429579

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.90
183.00	11.60	12.02
0.00	0.00	0.00