


Data Path : Z:\HPCHEM1\BNA F\Data\BF100917\
 Data File : BF099258.D
 Acq On : 9 Oct 2017 13:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 05 17:20:48 2017

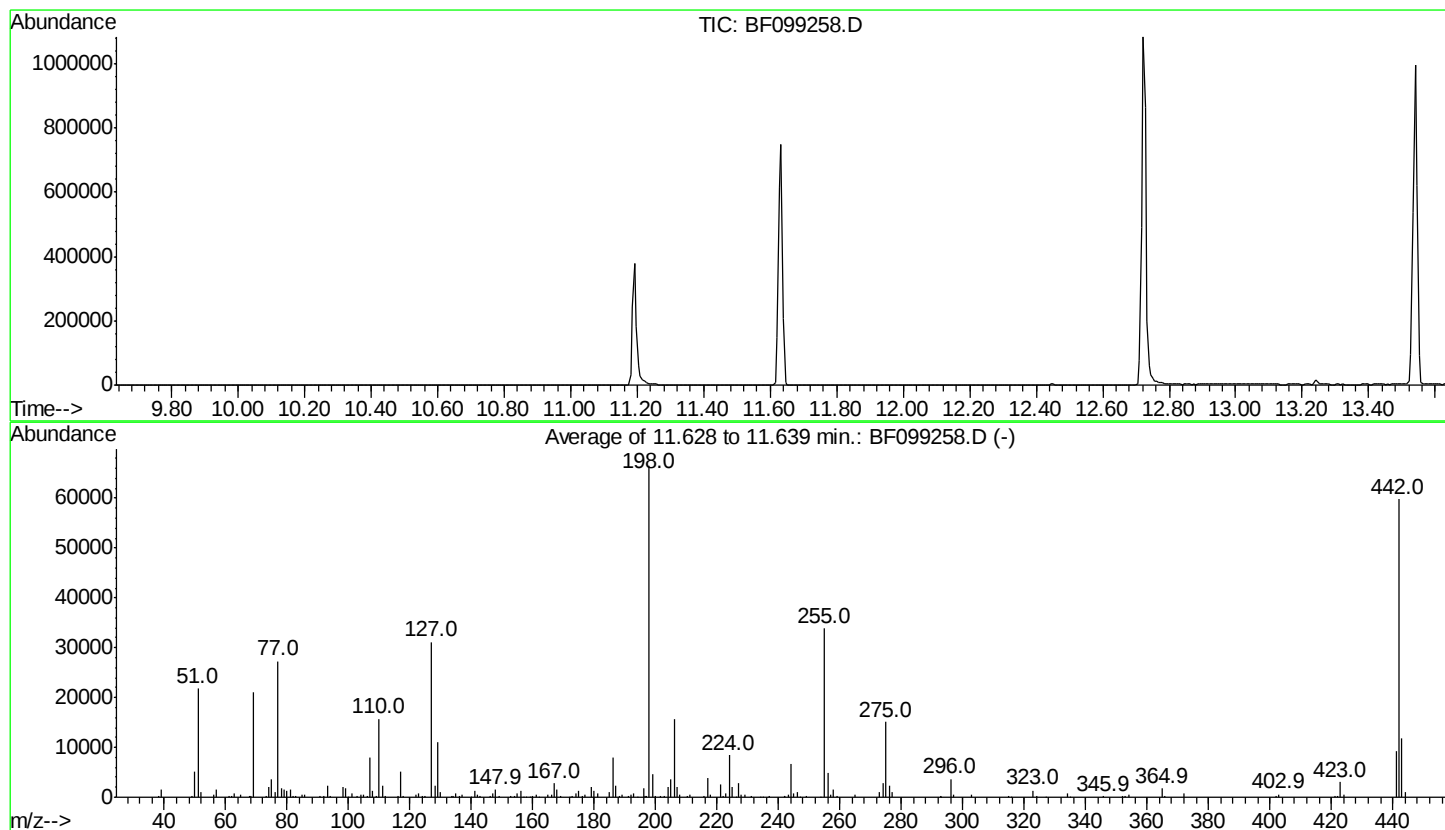

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	21825	PASS
68	69	0.00	2	0.9	194	PASS
69	198	0.00	100	31.8	21167	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.9	31200	PASS
197	198	0.00	2	0.5	312	PASS
198	198	100	100	100.0	66554	PASS
199	198	5	9	6.8	4526	PASS
275	198	10	60	22.7	15115	PASS
365	198	1	100	2.6	1735	PASS
441	442	0.01	24	15.5	9268	PASS
442	198	50	100	89.8	59794	PASS
443	442	15	24	19.8	11829	PASS