
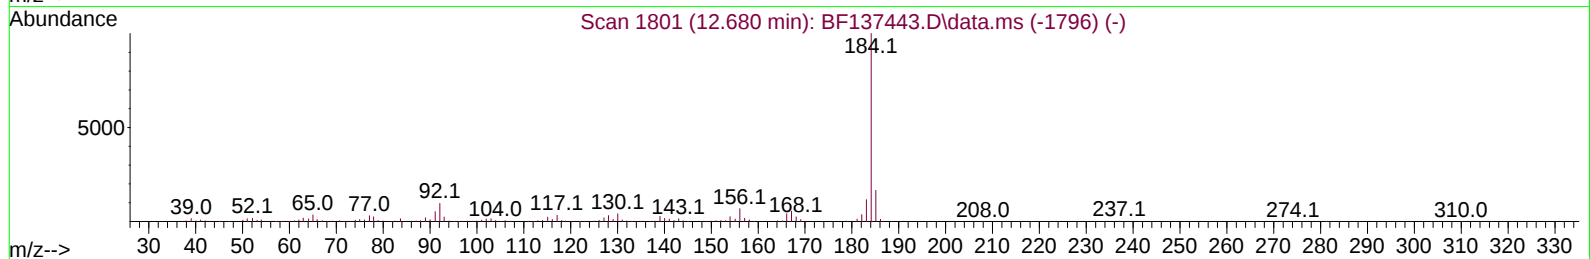
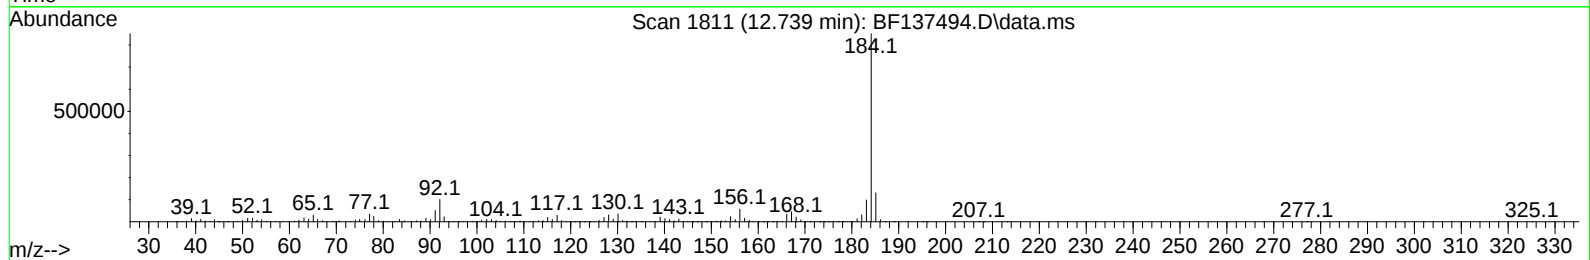


Data Path : C:\Users\euser\Desktop\krishna\BF030524\
Data File : BF137494.D
Acq On : 05 Mar 2024 11:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 10 05:38:51 2024
Quant Method : C:\Users\euser\Desktop\krishna\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 08:01:15 2024
Response via : Initial Calibration

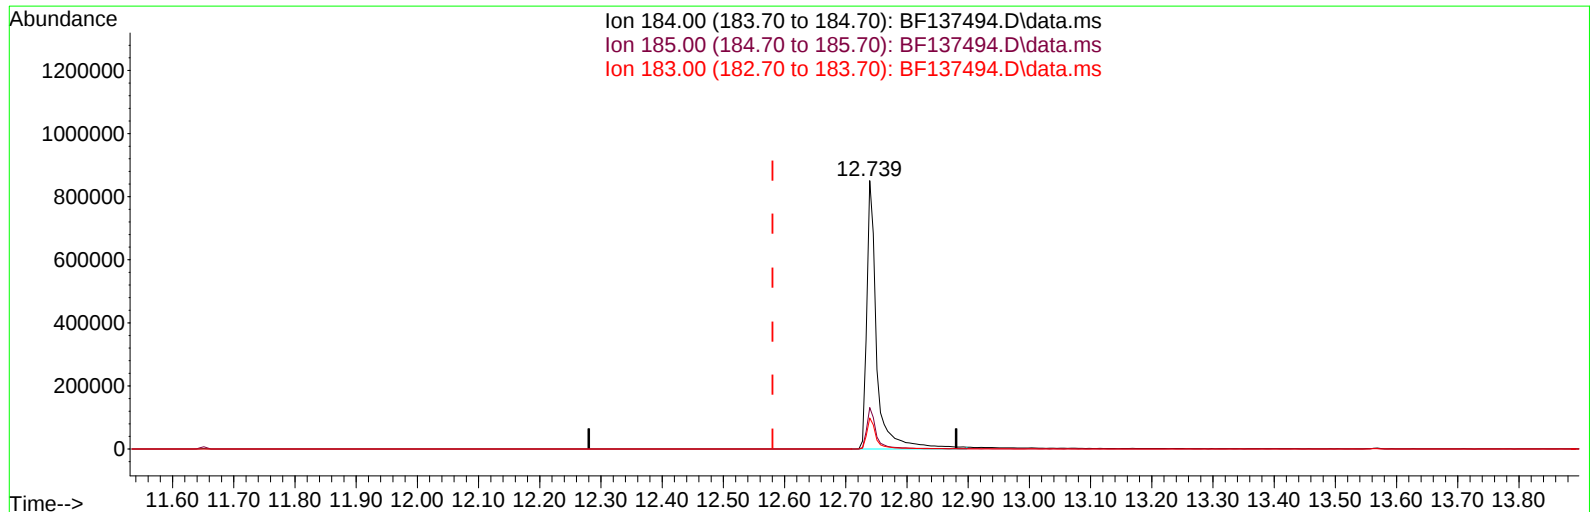

TIC: BF137494.D\data.ms

(77) Benzidine

12.739min (+ 0.159) 343498.15 ng

response 966710

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	15.44
183.00	11.60	11.58
0.00	0.00	0.00