
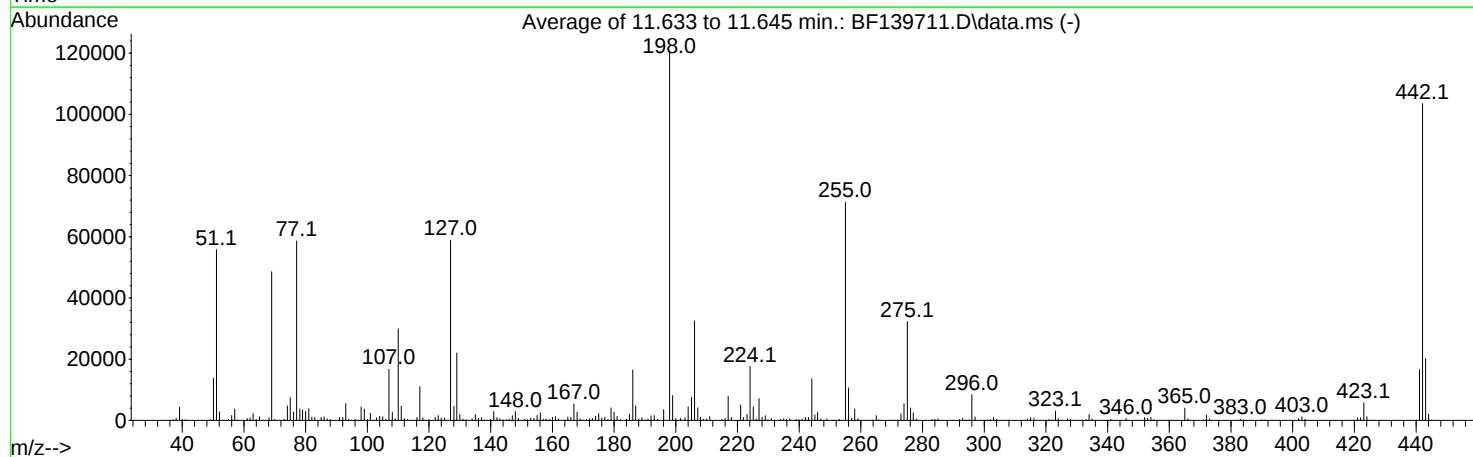


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100924\
Data File : BF139711.D
Acq On : 09 Oct 2024 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 02 04:58:47 2024

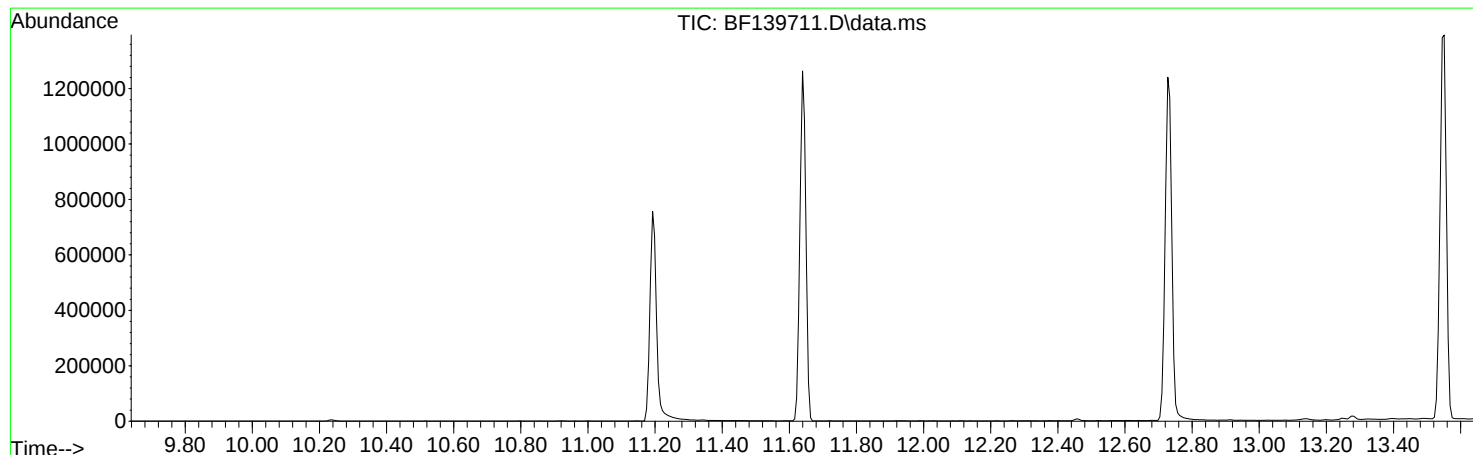




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	55813	PASS
68	69	0.00	2	1.7	846	PASS
69	198	0.00	100	40.4	48555	PASS
70	69	0.00	2	0.6	314	PASS
127	198	10	80	49.0	58861	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	120213	PASS
199	198	5	9	6.7	8086	PASS
275	198	10	60	26.9	32304	PASS
365	198	1	100	3.3	4003	PASS
441	198	0.01	100	13.8	16582	PASS
442	442	50	100	100.0	103544	PASS
443	442	15	24	19.5	20189	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100924\
Data File : BF139711.D
Acq On : 09 Oct 2024 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 09 12:41:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

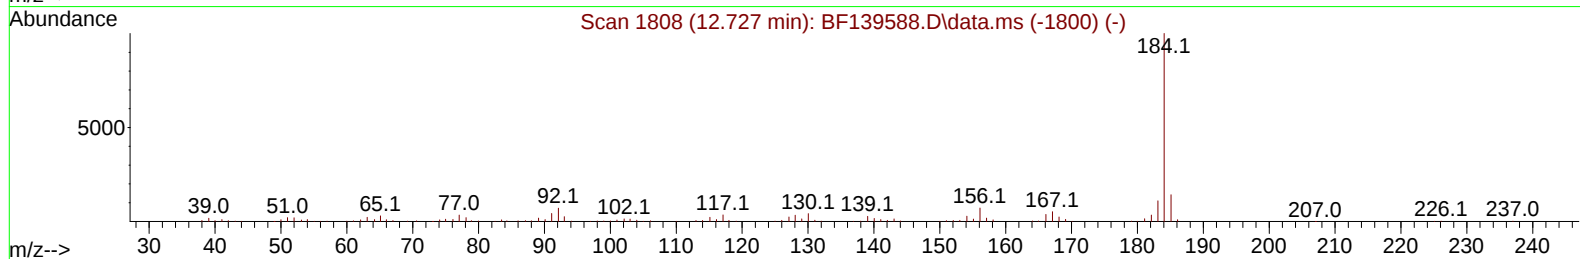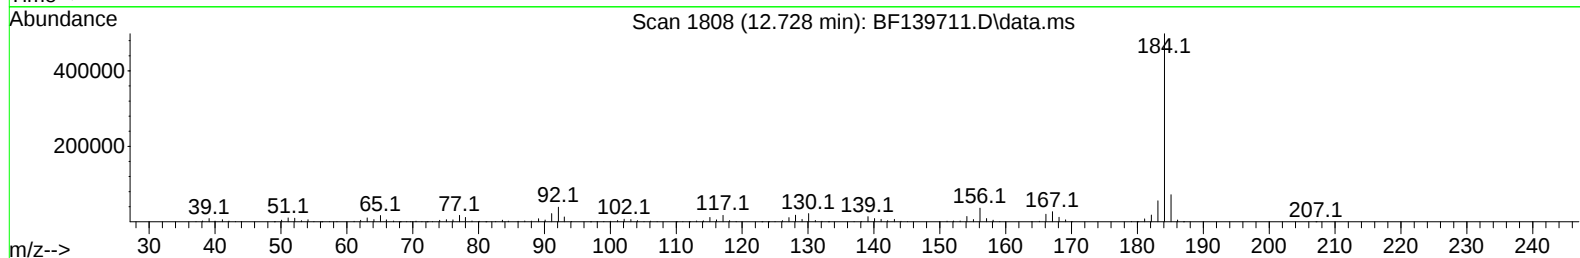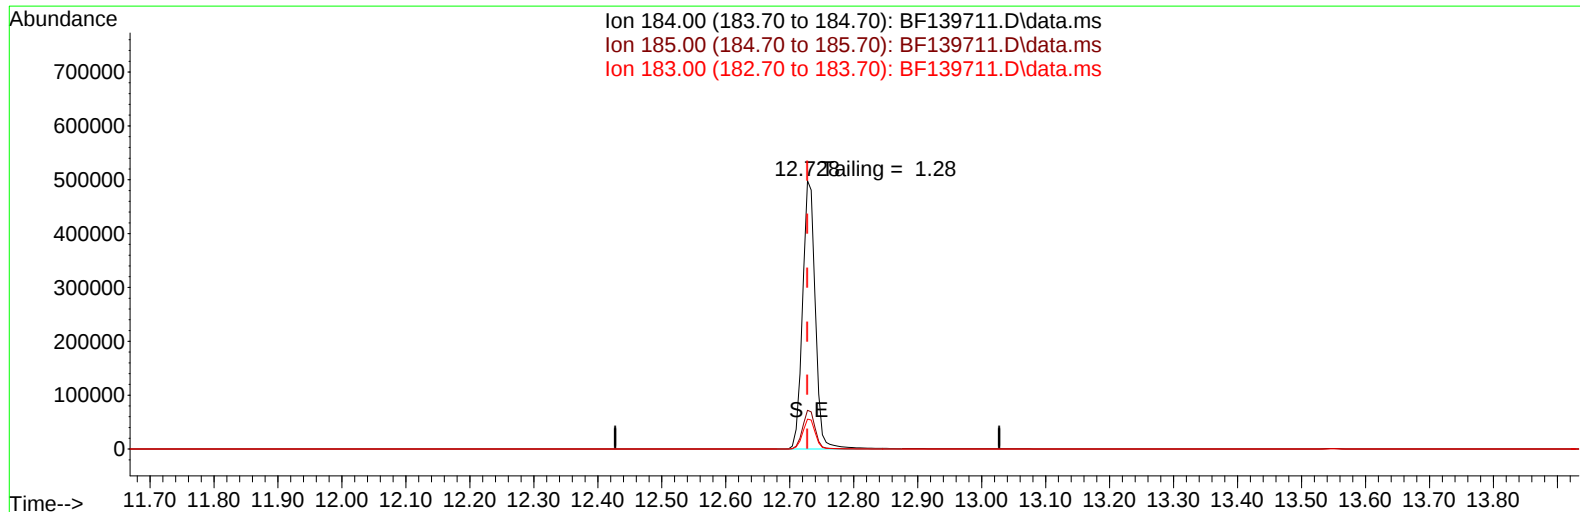

TIC: BF139711.D\data.ms

(77) Benzidine

12.728min (+ 0.000) 0.00 ng

response 698048

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.43
183.00	11.00	11.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/9/2024	BNA_F	<u>BF139711.D</u>
Compound Name	Response	Retention Time
DDT	358567	13.551
DDD	6605	13.28
DDE	665	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7270	365837	1.99

Instrument :
BNA_F
ClientSampleId :
DFTPP