

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100925\
 Data File : BF143918.D
 Acq On : 09 Oct 2025 19:41
 Operator : RC/JU
 Sample : Q3319-01 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-01-100825

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143918.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.946	293	298	304	rVB	6818	11098	1.34%	0.163%
2	5.487	555	560	572	rBV	273756	370535	44.74%	5.437%
3	6.498	727	732	747	rBV	257655	362144	43.73%	5.314%
4	6.881	792	797	802	rBV	492835	601797	72.67%	8.831%
5	7.439	887	892	902	rBV	150982	205496	24.81%	3.015%
6	8.163	1010	1015	1023	rBV	588178	729083	88.04%	10.698%
7	9.233	1192	1197	1207	rBV	251363	342018	41.30%	5.019%
8	9.780	1286	1290	1296	rVB	7979	10688	1.29%	0.157%
9	9.922	1308	1314	1324	rBV	588459	756627	91.37%	11.102%
10	10.333	1380	1384	1390	rBV2	7571	14977	1.81%	0.220%
11	10.469	1405	1407	1416	rVB8	4391	10215	1.23%	0.150%
12	10.569	1416	1424	1429	rBV7	5483	12937	1.56%	0.190%
13	10.633	1430	1435	1442	rVV	37867	51672	6.24%	0.758%
14	10.710	1442	1448	1456	rVV	135283	193565	23.37%	2.840%
15	10.827	1464	1468	1475	rVB3	10724	17354	2.10%	0.255%
16	11.274	1540	1544	1546	rBV4	9473	12666	1.53%	0.186%
17	11.304	1547	1549	1553	rVB2	8749	9580	1.16%	0.141%
18	11.410	1562	1567	1574	rBV	582428	773448	93.40%	11.349%
19	11.651	1604	1608	1611	rBV6	5563	8544	1.03%	0.125%
20	11.704	1612	1617	1621	rBV2	10048	16483	1.99%	0.242%
21	11.933	1649	1656	1666	rBV4	49938	116650	14.09%	1.712%
22	12.021	1668	1671	1674	rBV2	11040	16467	1.99%	0.242%
23	12.110	1683	1686	1689	rBV2	10514	12734	1.54%	0.187%
24	12.463	1743	1746	1749	rBV	15093	20340	2.46%	0.298%
25	12.498	1749	1752	1758	rVB4	20200	27564	3.33%	0.404%
26	12.551	1758	1761	1765	rBV5	8622	13973	1.69%	0.205%
27	12.627	1770	1774	1778	rBV	39746	52469	6.34%	0.770%
28	12.721	1787	1790	1794	rBV4	17222	25901	3.13%	0.380%
29	12.857	1809	1813	1819	rBV	53062	81642	9.86%	1.198%
30	12.998	1832	1837	1846	rVB	257675	344092	41.55%	5.049%
31	14.057	2012	2017	2028	rBV	596932	828120	100.00%	12.152%
32	15.539	2264	2269	2280	rVB	418912	764065	92.27%	11.212%




Sum of corrected areas: 6814944

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100925\
Data File : BF143918.D
Acq On : 09 Oct 2025 19:41
Operator : RC/JU
Sample : Q3319-01 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-100825

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

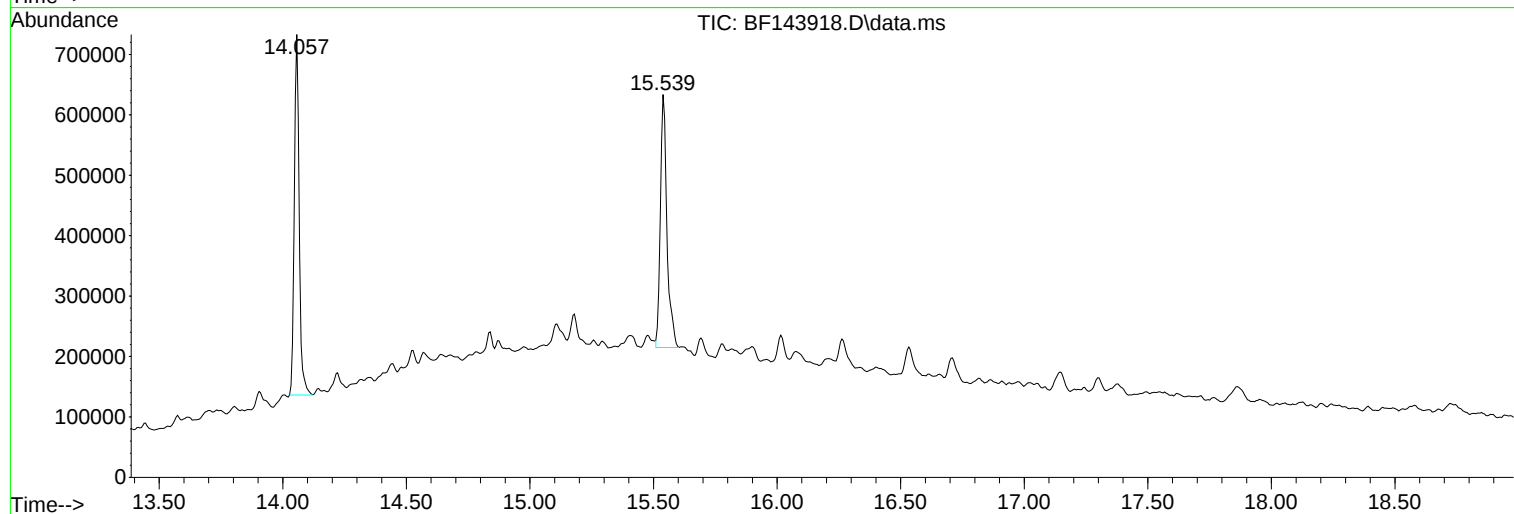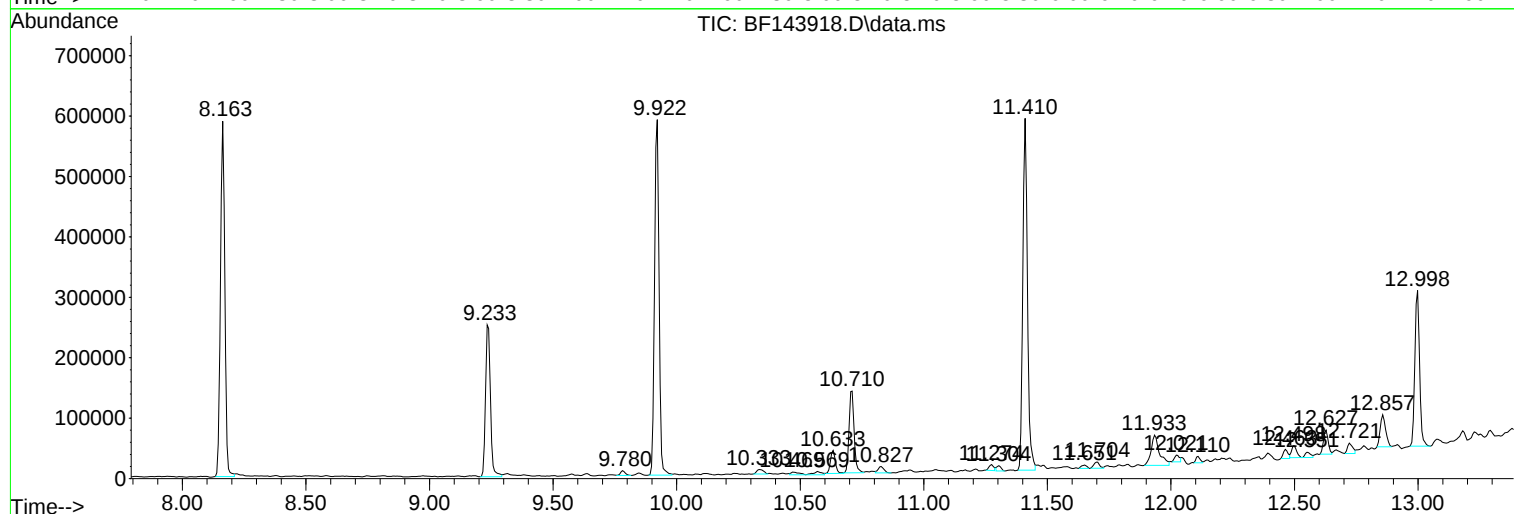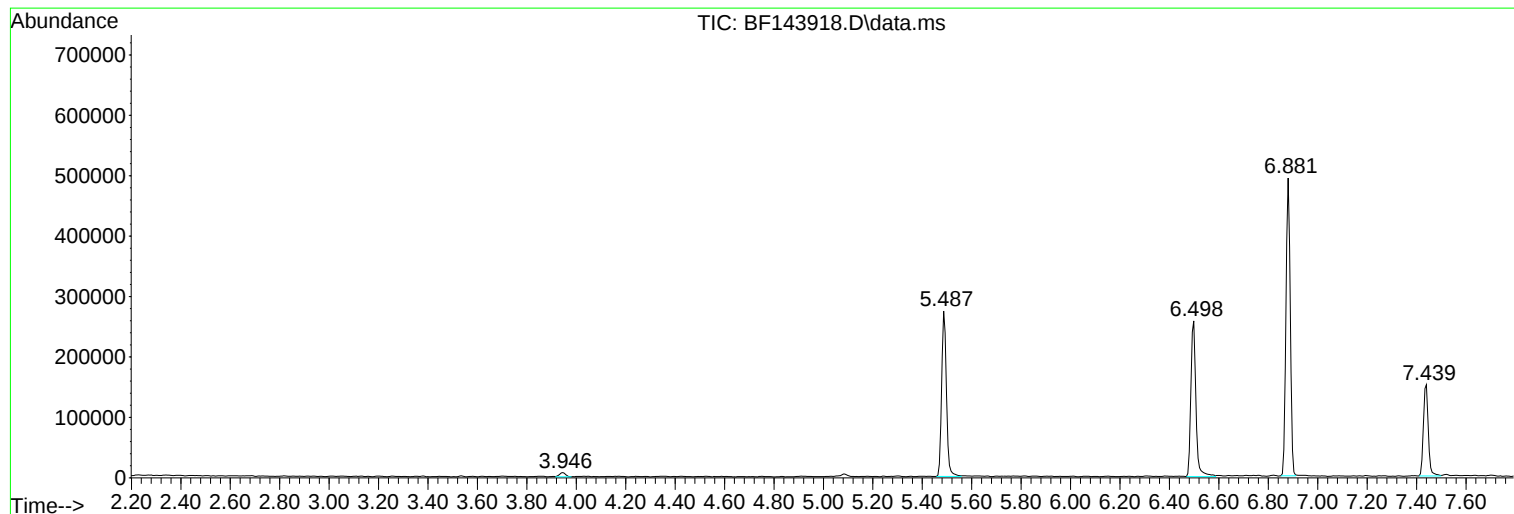

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100925\
Data File : BF143918.D
Acq On : 09 Oct 2025 19:41
Operator : RC/JU
Sample : Q3319-01 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-100825

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100925\
Data File : BF143918.D
Acq On : 09 Oct 2025 19:41
Operator : RC/JU
Sample : Q3319-01 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-100825

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------