
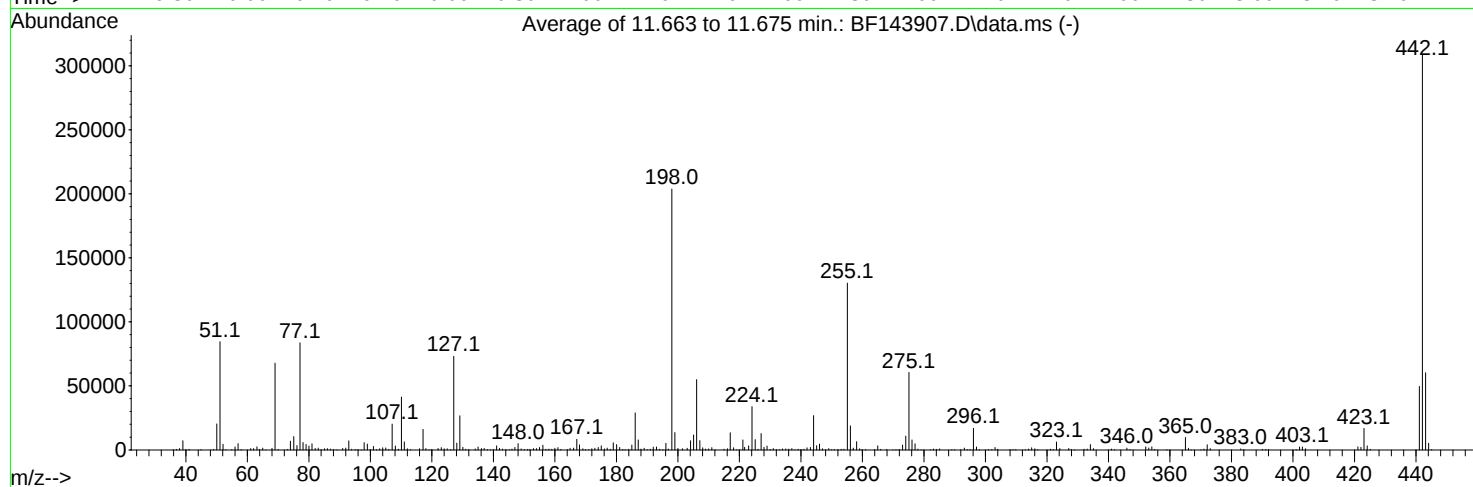


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100925\
Data File : BF143907.D
Acq On : 09 Oct 2025 13:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 06 15:29:47 2025

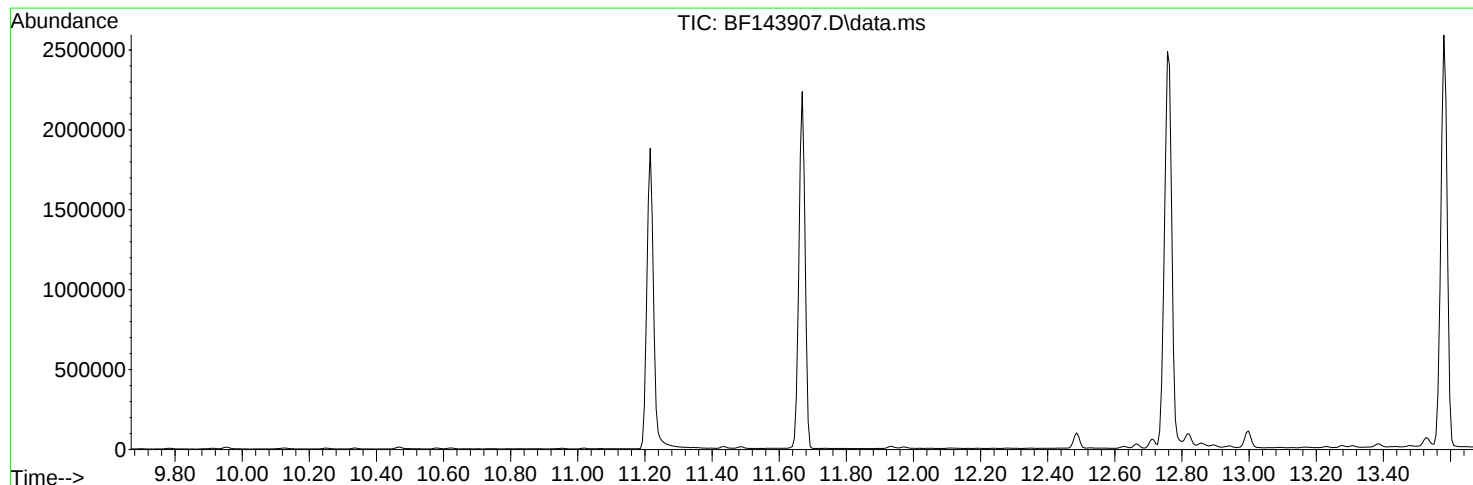




AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	1318	PASS
69	69	100	100	100.0	67867	PASS
70	69	0.00	2	0.7	497	PASS
197	198	0.00	2	0.4	767	PASS
198	198	100	100	100.0	203797	PASS
199	198	5	9	6.6	13530	PASS
365	198	1	100	4.7	9644	PASS
441	443	0.01	150	82.1	49552	PASS
442	442	100	100	100.0	308395	PASS
443	442	15	24	19.6	60331	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100925\
Data File : BF143907.D
Acq On : 09 Oct 2025 13:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 09 14:41:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

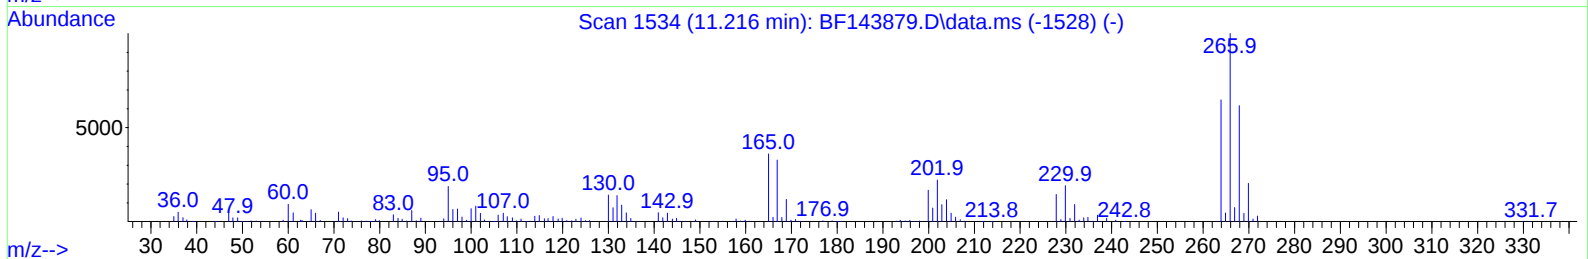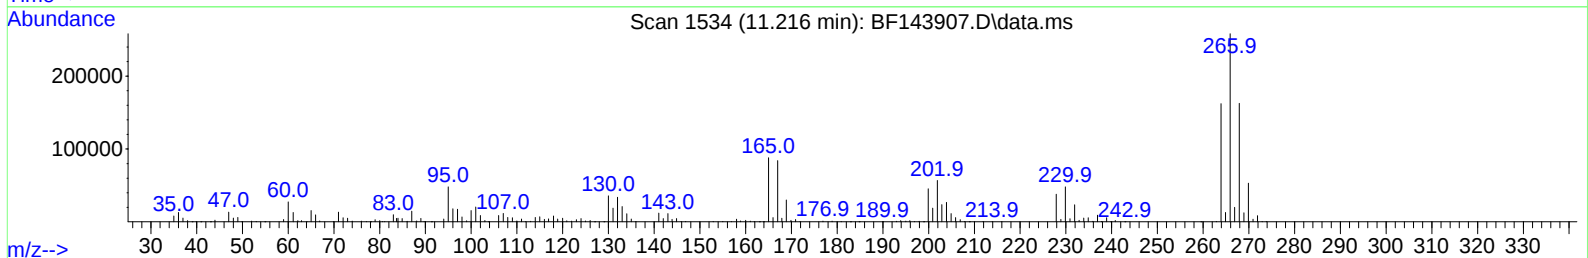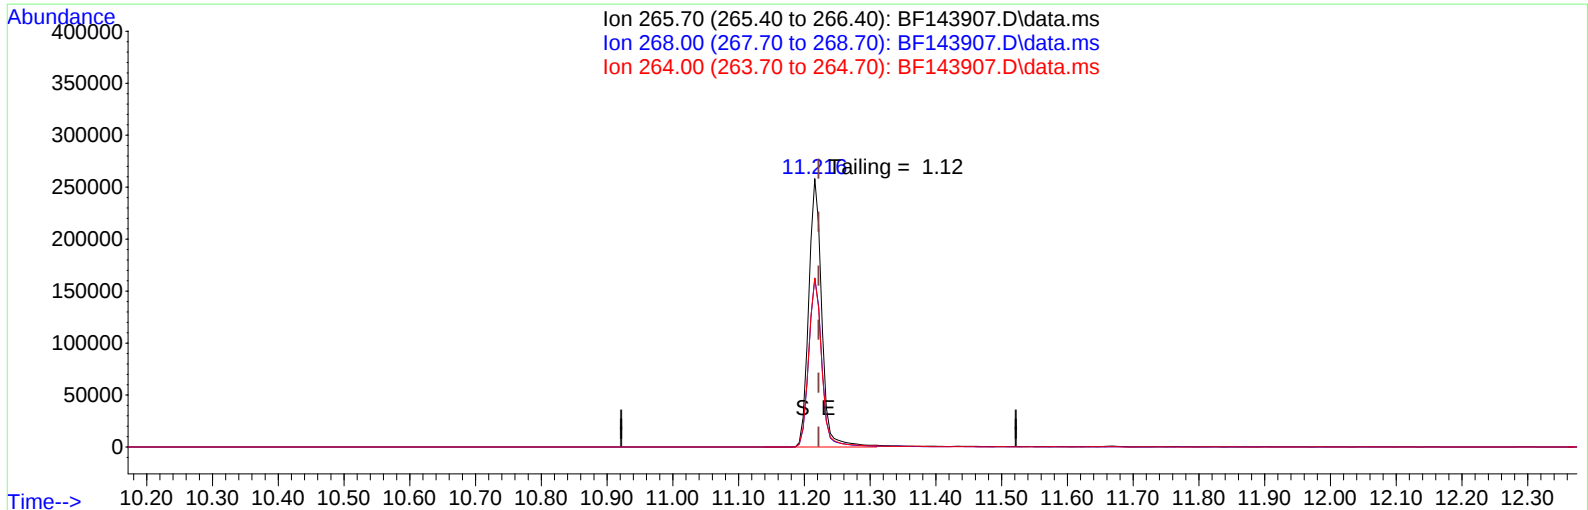

TIC: BF143907.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.006) 52666.13 ng m




response 355269

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	62.97
264.00	64.70	62.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100925\
Data File : BF143907.D
Acq On : 09 Oct 2025 13:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 09 14:41:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

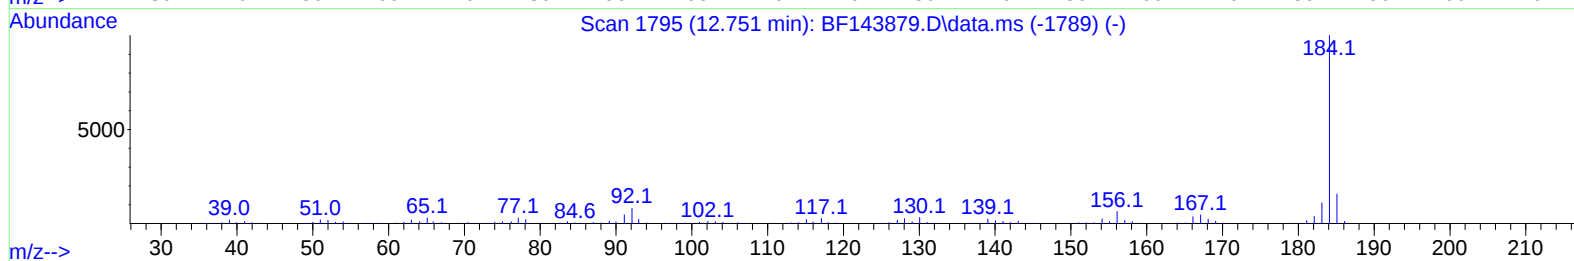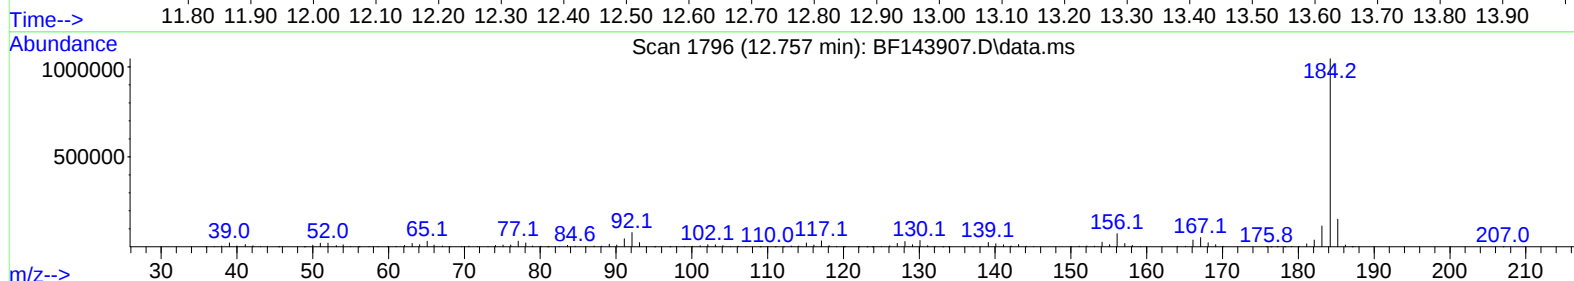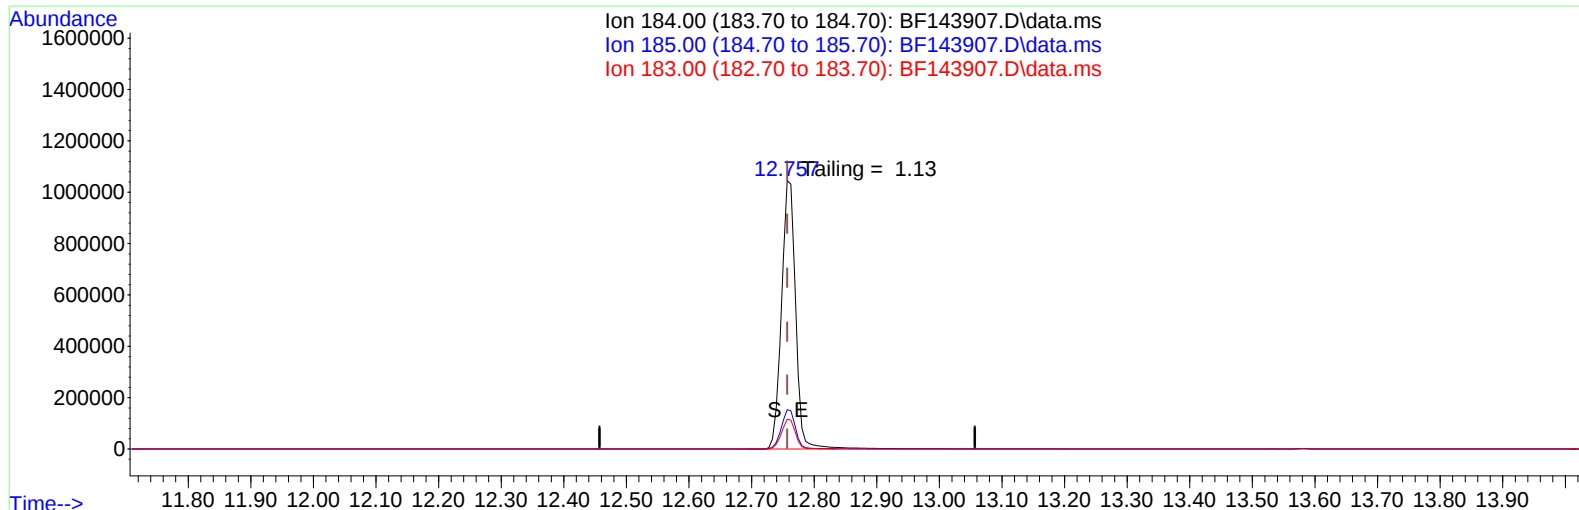

TIC: BF143907.D\data.ms

(77) Benzidine

12.757min (-0.000) 0.00 ng

response 1653284

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.69
183.00	11.00	11.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/9/2025	BNA_F	<u>BF143907.D</u>
Compound Name	Response	Retention Time
DDT	699042	13.58
DDD	7830	13.274
DDE	0	12.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7830	706872	1.11

Instrument :
BNA_F
ClientSampleId :
DFTPP