
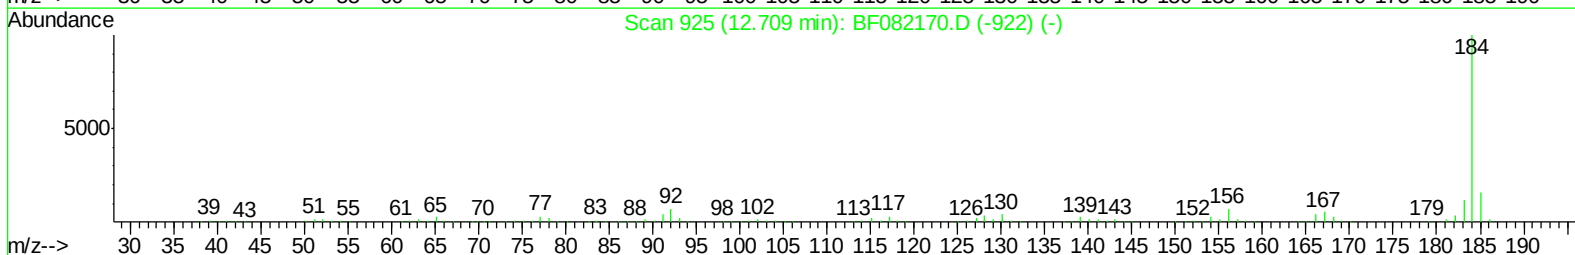
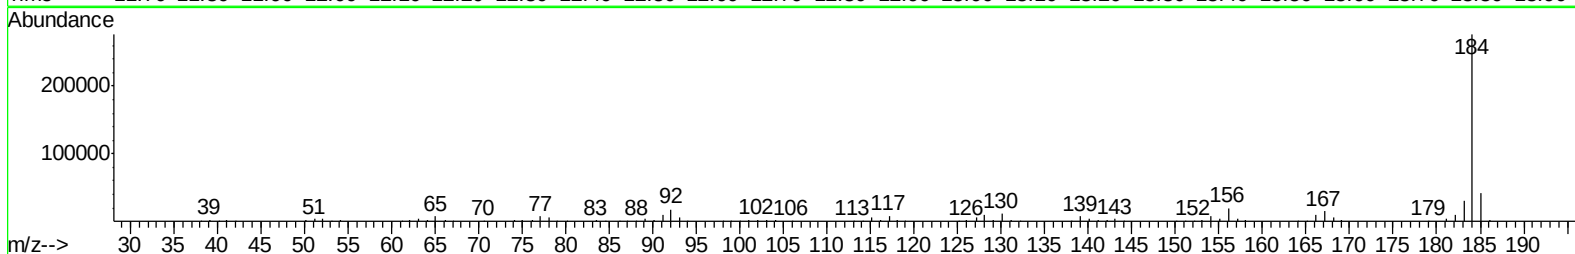


Data Path : Z:\HPCHEM1\BNA F\Data\BF101015\
Data File : BF082189.D
Acq On : 10 Oct 2015 21:41
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 08:19:14 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 01:46:21 2015
Response via : Initial Calibration

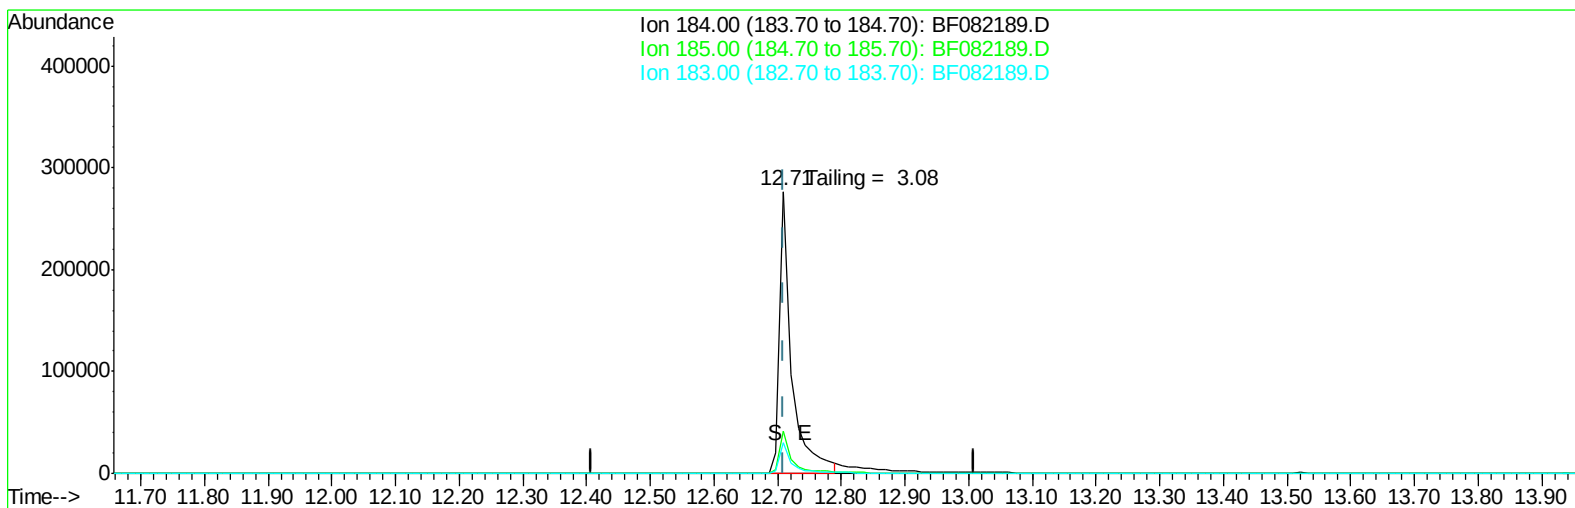

TIC: BF082189.D

(76) Benzidine




12.709min (-0.000) 0.00ng

response 395644

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	15.07
183.00	11.40	11.03
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF101015\
Data File : BF082189.D
Acq On : 10 Oct 2015 21:41
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 08:19:14 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 01:46:21 2015
Response via : Initial Calibration

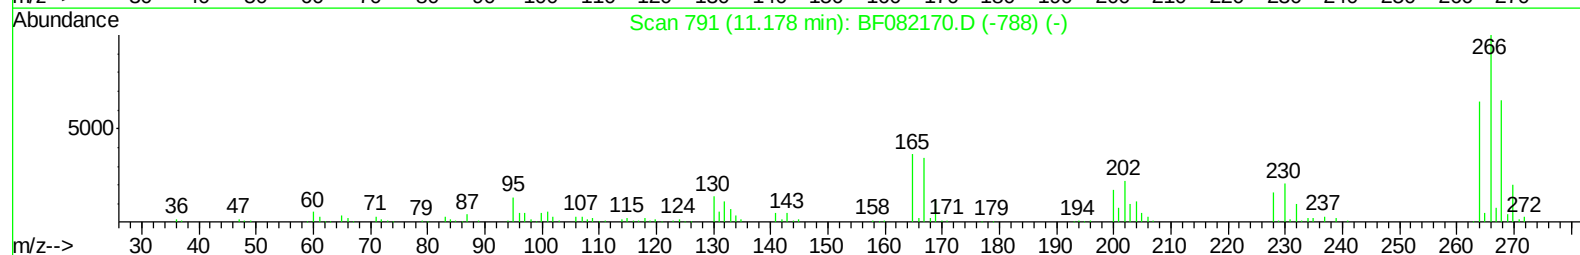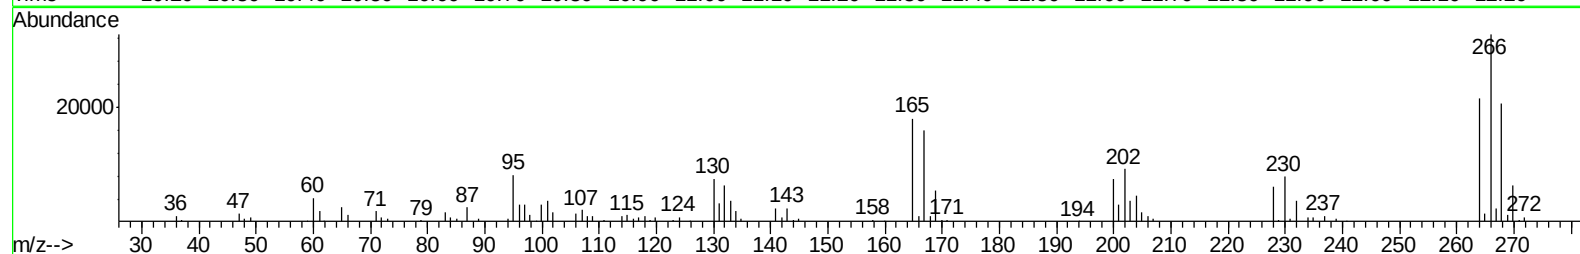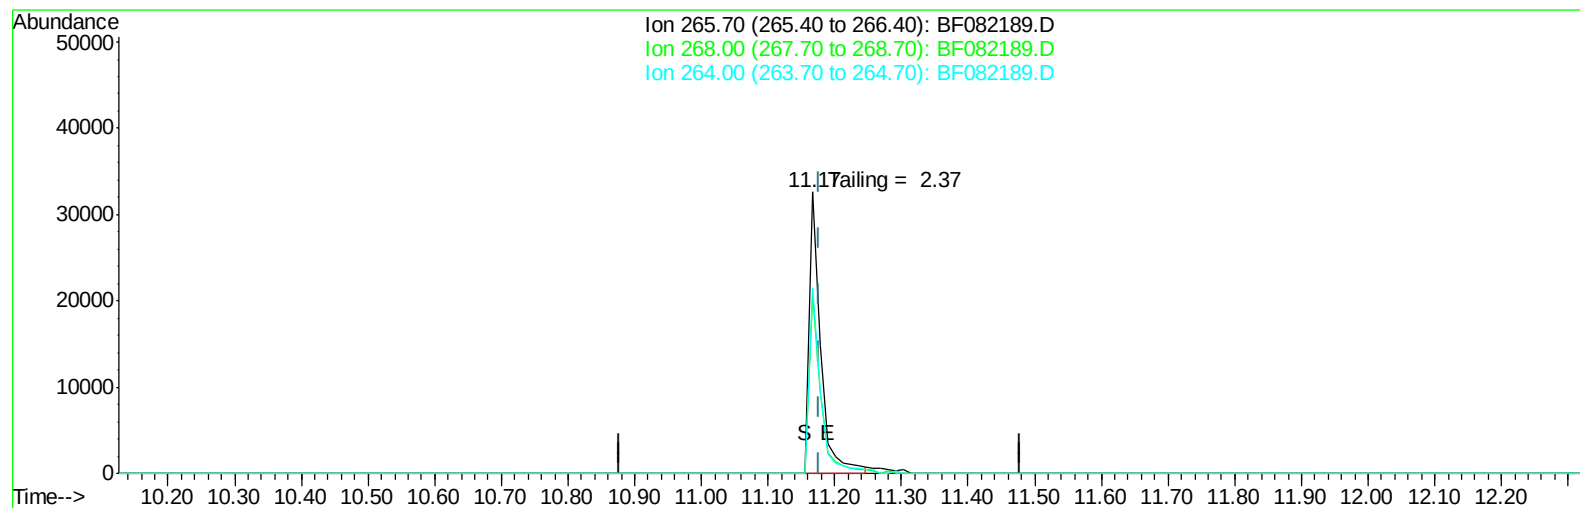

TIC: BF082189.D

(69) Pentachlorophenol (C)

11.166min (-0.012) 0.00ng

response 40435

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.24
264.00	64.20	66.10
0.00	0.00	0.00