

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101015\
 Data File : BF082205.D
 Acq On : 11 Oct 2015 5:40
 Operator : UM/IZ
 Sample : G3979-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 A16COMP

Manual Integrations
 APPROVED

MMDadoda
 10/12/2015 2:38:27 PM

Quant Time: Oct 12 04:09:14 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 12 02:59:50 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	85503	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	322176	20.00	ng	0.00
38) Acenaphthene-d10	9.87	164	140649	20.00	ng	-0.01
63) Phenanthrene-d10	11.36	188	230038	20.00	ng	-0.01
75) Chrysene-d12	14.00	240	191546	20.00	ng	-0.01
86) Perylene-d12	15.44	264	194403	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	531002	125.34	ng	0.01
7) Phenol-d6	6.48	99	675114	122.45	ng	0.00
23) Nitrobenzene-d5	7.41	82	387270	80.72	ng	-0.01
41) 2,4,6-Tribromophenol	10.67	330	145713	110.47	ng	0.00
44) 2-Fluorobiphenyl	9.20	172	671014	79.12	ng	-0.01
78) Terphenyl-d14	12.95	244	472712	65.40	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	9.60	163	239890	24.22	ng	99
70) Phenanthrene	11.39	178	146312	12.98	ng	98
71) Anthracene	11.44	178	24060	2.07	ng	97
74) Fluoranthene	12.58	202	286250	23.64	ng	96
77) Pyrene	12.81	202	238804	21.01	ng	97
80) Benzo(a)anthracene	14.00	228	116147	11.65	ng	96
82) Chrysene	14.04	228	121393	11.56	ng	99
85) Indeno(1,2,3-cd)pyrene	16.85	276	81344	9.75	ng	96
87) Benzo(b)fluoranthene	15.03	252	183497m	15.51	ng	
88) Benzo(k)fluoranthene	15.04	252	82222m	8.27	ng	
89) Benzo(a)pyrene	15.38	252	118687	11.68	ng	98
91) Benzo(g,h,i)perylene	17.27	276	75705	9.36	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101015\
Data File : BF082205.D
Acq On : 11 Oct 2015 5:40
Operator : UM/IZ
Sample : G3979-08
Misc :
ALS Vial : 38 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
A16COMP

Manual Integrations
APPROVED

MMDadoda
10/12/2015 2:38:27 PM

Quant Time: Oct 12 04:09:14 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 02:59:50 2015
Response via : Initial Calibration

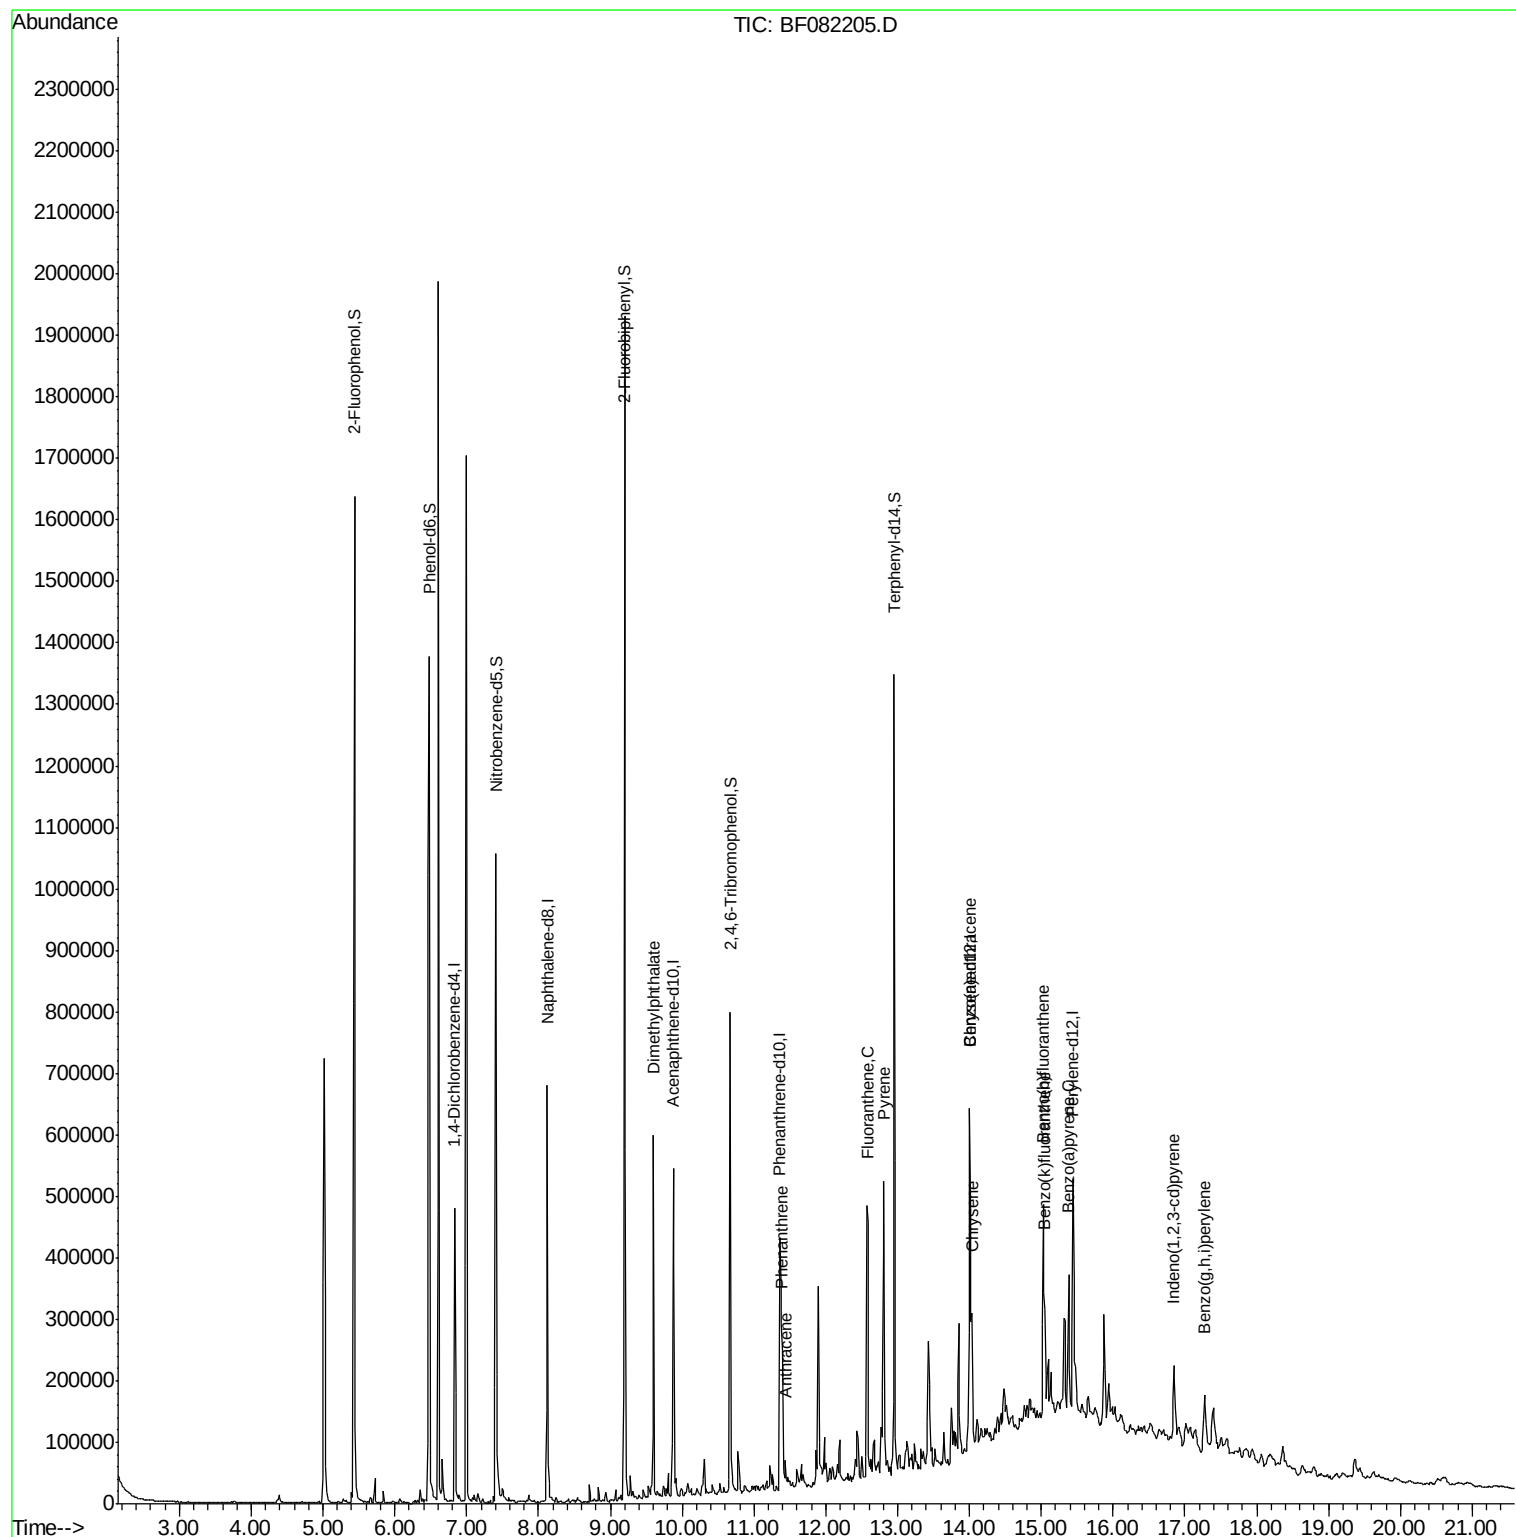



#1





1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.83 min Scan# 411
Delta R.T. 0.00 min
Lab File: BF082205.D
Acq: 11 Oct 2015 5:40

Instrument :
BNA_F
ClientSampleId :
A16COMP

Tgt Ion	Ratio	Lower	Upper
152	100		
150	157.9	129.0	193.4
115	62.3	52.1	78.1

Manual Integrations
APPROVED




MMDadoda
10/12/2015 2:38:27 PM

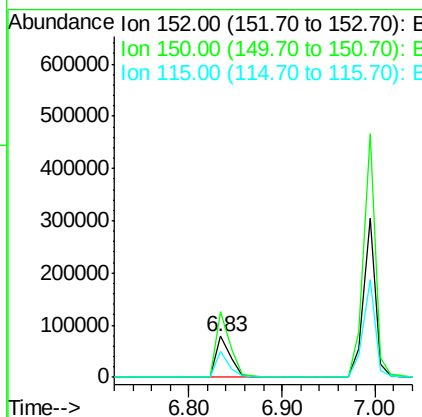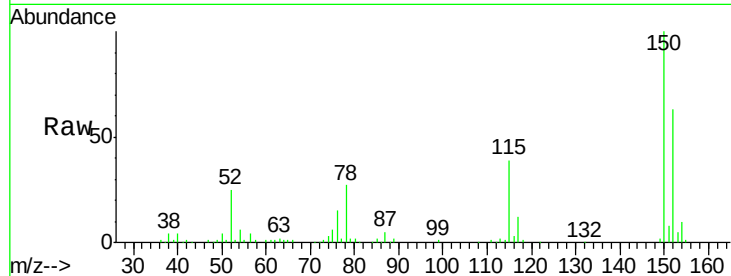


#5

2-Fluorophenol
Concen: 125.34 ng
RT: 5.44 min Scan# 289
Delta R.T. 0.01 min
Lab File: BF082205.D
Acq: 11 Oct 2015 5:40

Tgt Ion	Ratio	Lower	Upper
112	100		
64	57.7	48.6	73.0
63	30.3	25.1	37.7

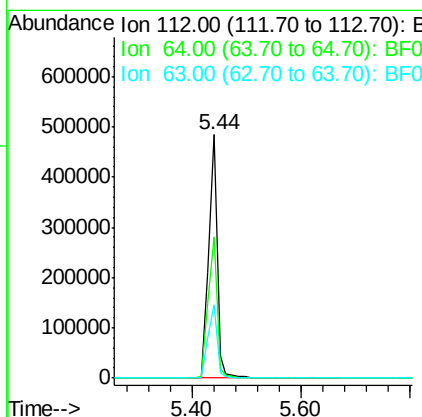

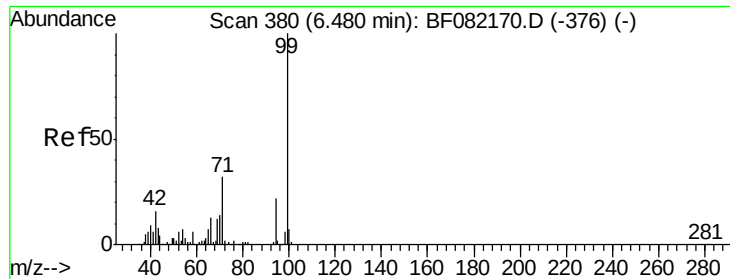

#7

Phenol-d6

Concen: 122.45 ng

RT: 6.48 min Scan# 380

Delta R.T. 0.00 min

Lab File: BF082205.D


Acq: 11 Oct 2015 5:40

Instrument :

BNA_F

ClientSampleId :




A16COMP

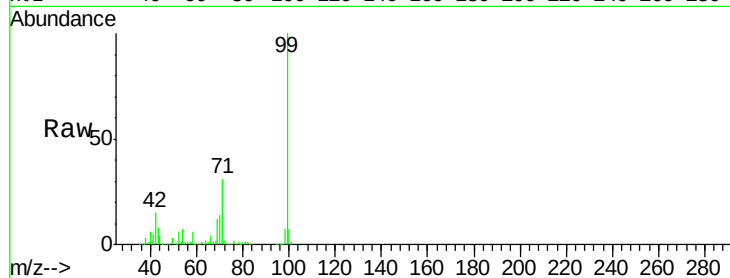

Tgt Ion	Ratio	Resp	Lower	Upper
99	100	675114		
42	15.0	13.2	19.8	
71	31.0	25.6	38.4	

Manual Integrations
APPROVED

MMDadoda
10/12/2015 2:38:27 PM

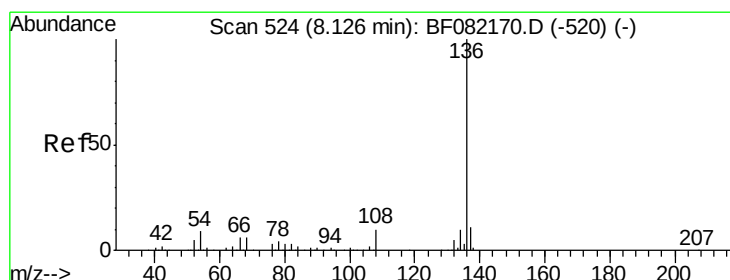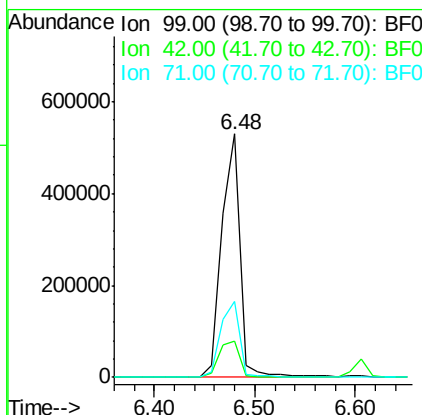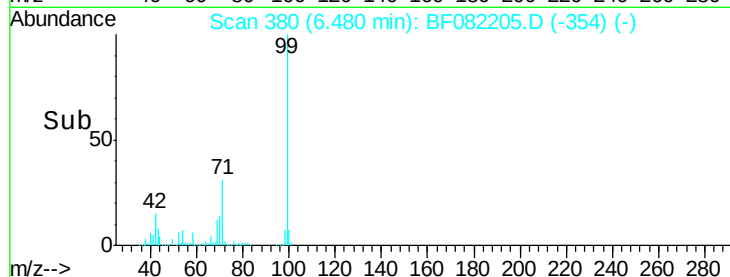

#21

Naphthalene-d8

Concen: 20.00 ng




RT: 8.13 min Scan# 524


Delta R.T. 0.00 min

Lab File: BF082205.D

Acq: 11 Oct 2015 5:40

Tgt Ion	Ratio	Resp	Lower	Upper
136	100	322176		
137	10.8	9.0	13.6	
54	7.2	7.5	11.3#	
68	4.6	4.6	7.0#	

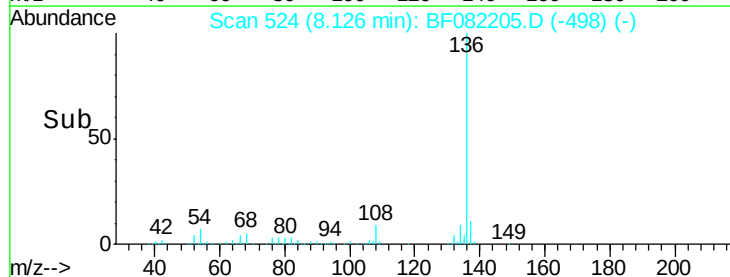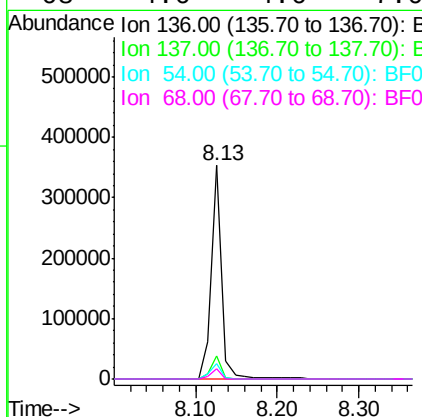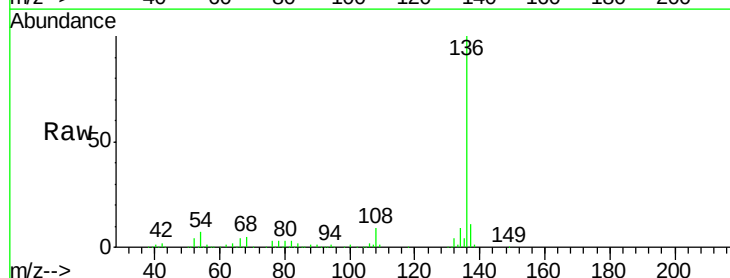







#23
Nitrobenzene-d5
Concen: 80.72 ng
RT: 7.41 min Scan# 461
Delta R.T. -0.01 min
Lab File: BF082205.D
Acq: 11 Oct 2015 5:40

Instrument :
BNA_F
ClientSampleId :
A16COMP

Tgt Ion	Ratio	Resp	Lower	Upper
82	100	387270		
128	41.4	38.7	58.1	
54	54.5	40.1	60.1	




Manual Integrations
APPROVED


MMDadoda
10/12/2015 2:38:27 PM

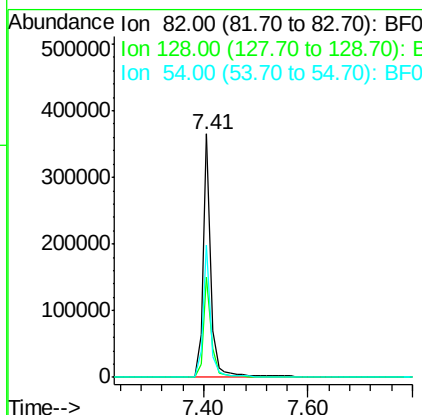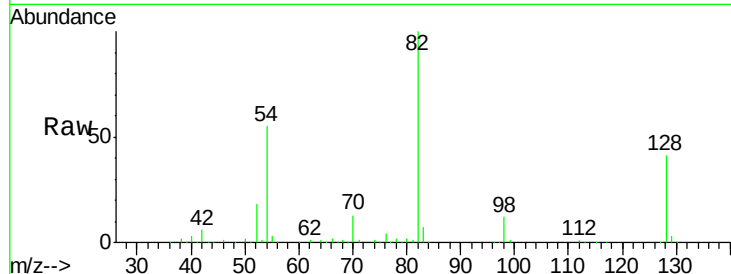

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.87 min Scan# 677
Delta R.T. -0.01 min
Lab File: BF082205.D
Acq: 11 Oct 2015 5:40

Tgt Ion	Ratio	Resp	Lower	Upper
164	100	140649		
162	103.4	81.6	122.4	
160	44.6	36.4	54.6	

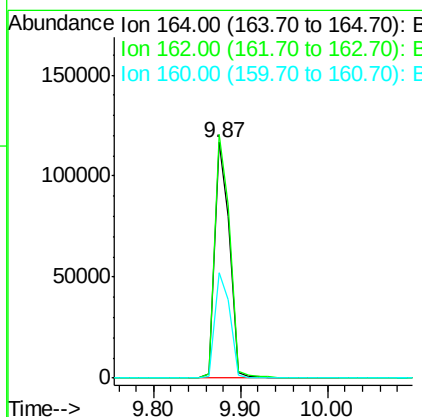

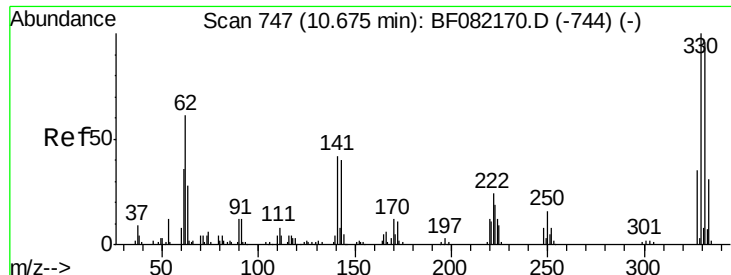





#41
 2,4,6-Tribromophenol
 Concen: 110.47 ng
 RT: 10.67 min Scan# 747
 Delta R.T. 0.00 min
 Lab File: BF082205.D
 Acq: 11 Oct 2015 5:40

Instrument :
 BNA_F
 ClientSampleId :
 A16COMP

Tgt Ion	Ratio	Resp	Lower	Upper
330	100	145713		
332	97.7	77.1	115.7	
141	33.3	29.8	44.8	




Manual Integrations
 APPROVED


MMDadoda
 10/12/2015 2:38:27 PM

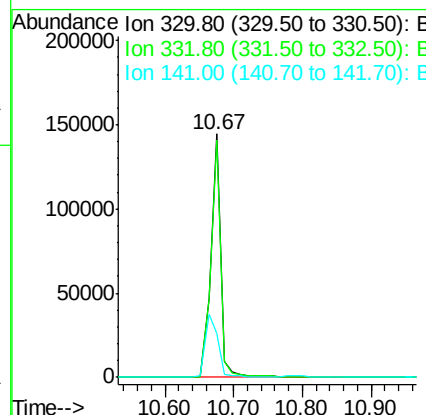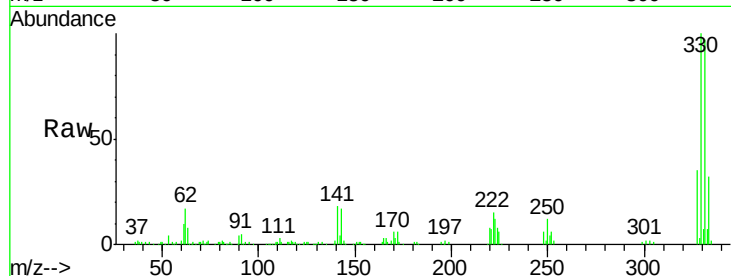

#44
 2-Fluorobiphenyl
 Concen: 79.12 ng
 RT: 9.20 min Scan# 618
 Delta R.T. -0.01 min
 Lab File: BF082205.D
 Acq: 11 Oct 2015 5:40

Tgt Ion	Ratio	Resp	Lower	Upper
172	100	671014		
171	35.6	28.6	42.8	
170	23.8	19.7	29.5	

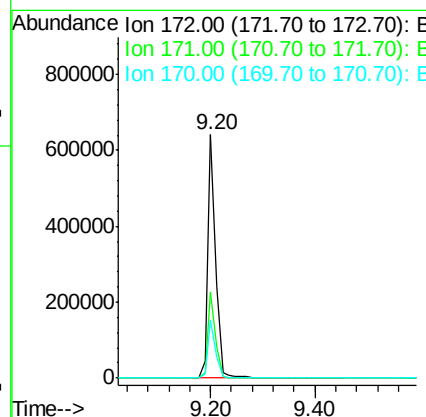

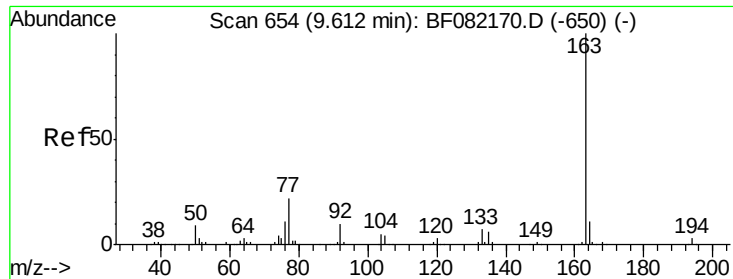





#49
Dimethylphthalate
Concen: 24.22 ng
RT: 9.60 min Scan# 653
Delta R.T. -0.01 min
Lab File: BF082205.D
Acq: 11 Oct 2015 5:40

Instrument :
BNA_F
ClientSampleId :
A16COMP

Tgt Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	3.5	2.6	4.0
164	10.1	8.5	12.7




Manual Integrations
APPROVED


MMDadoda
10/12/2015 2:38:27 PM

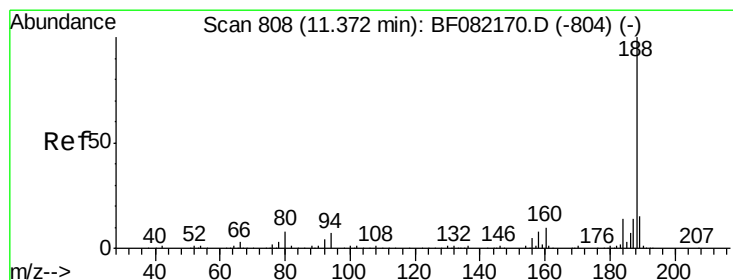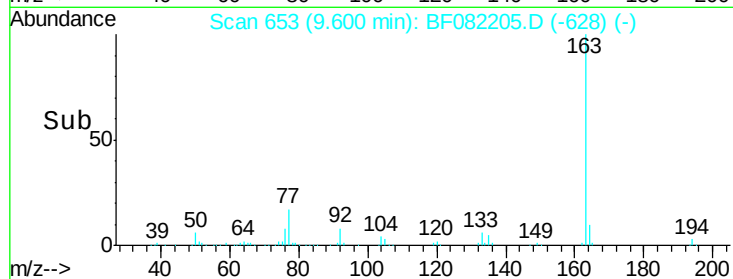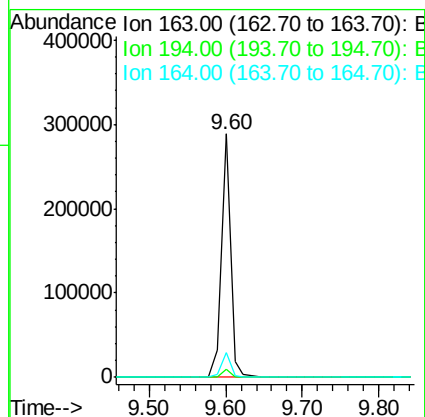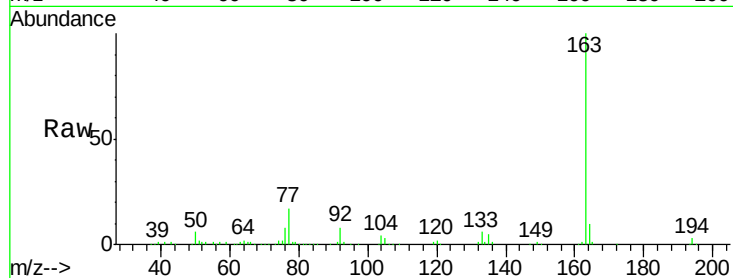

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.36 min Scan# 807
Delta R.T. -0.01 min
Lab File: BF082205.D
Acq: 11 Oct 2015 5:40

Tgt Ion	Ratio	Resp Lower	Resp Upper
188	100		
94	11.6	5.8	8.6#
80	12.9	6.4	9.6#

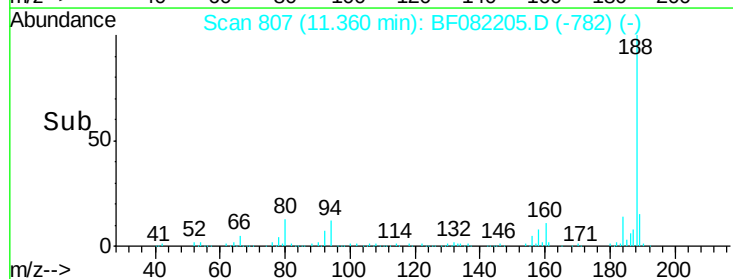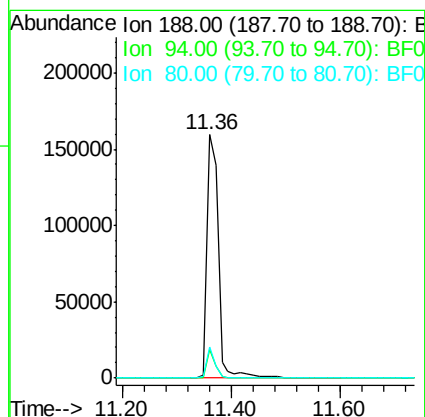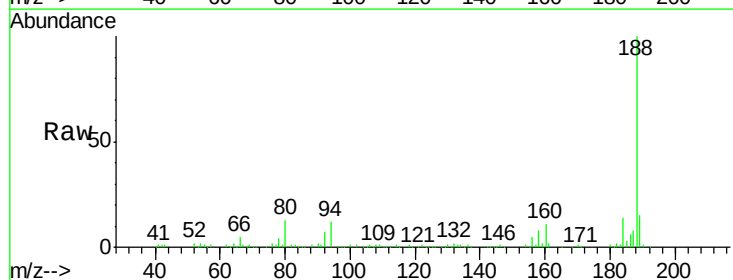

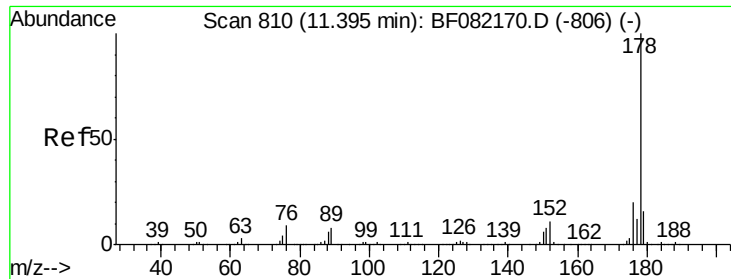





#70
Phenanthrene
Concen: 12.98 ng
RT: 11.39 min Scan# 810
Delta R.T. 0.00 min
Lab File: BF082205.D
Acq: 11 Oct 2015 5:40

Instrument :
BNA_F
ClientSampleId :
A16COMP

Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.9	16.0	24.0
179	14.7	12.6	19.0




Manual Integrations
APPROVED


MMDadoda
10/12/2015 2:38:27 PM

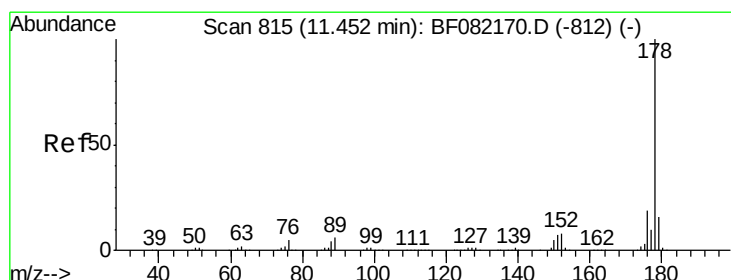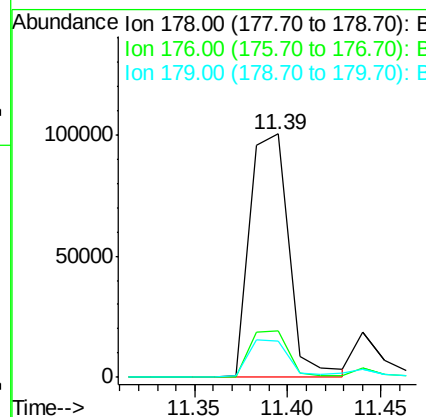

#71
Anthracene
Concen: 2.07 ng
RT: 11.44 min Scan# 814
Delta R.T. -0.01 min
Lab File: BF082205.D
Acq: 11 Oct 2015 5:40

Tgt Ion	Ratio	Lower	Upper
178	100		
176	20.1	15.4	23.0
179	17.7	12.5	18.7

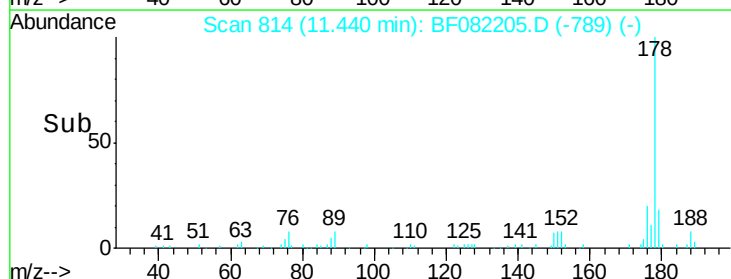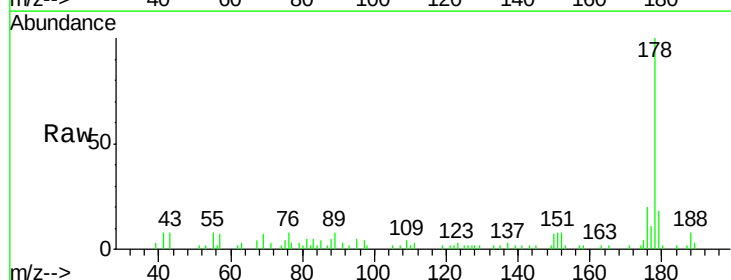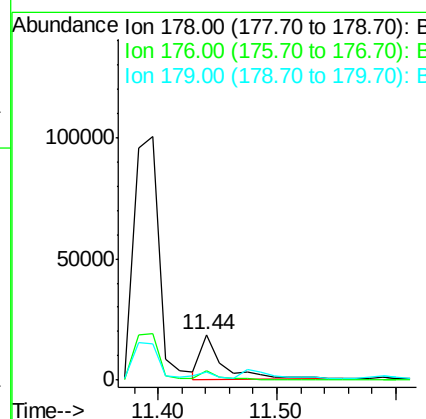



#74

Fluoranthene

Concen: 23.64 ng

RT: 12.58 min Scan# 914

Delta R.T. 0.00 min

Lab File: BF082205.D

Acq: 11 Oct 2015 5:40

Instrument :

BNA_F





ClientSampleId :

A16COMP

Tgt	Ion	Ratio	Resp	Lower	Upper
202	100		286250		
101	6.4	0.0	29.3		
203	16.7	0.0	37.8		

Manual Integrations
APPROVED

MMDadoda
10/12/2015 2:38:27 PM

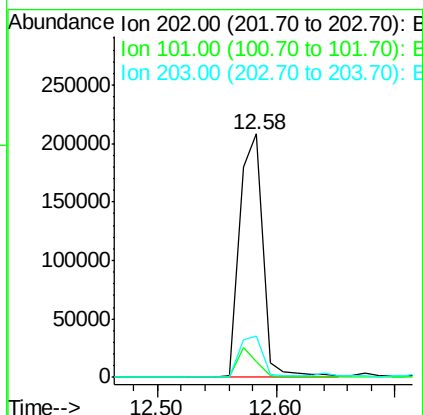

#75

Chrysene-d12

Concen: 20.00 ng




RT: 14.00 min Scan# 1038


Delta R.T. -0.01 min

Lab File: BF082205.D

Acq: 11 Oct 2015 5:40

Tgt	Ion	Ratio	Resp	Lower	Upper
240	100		191546		
120	13.2	8.1	12.1#		
236	26.4	21.3	31.9		

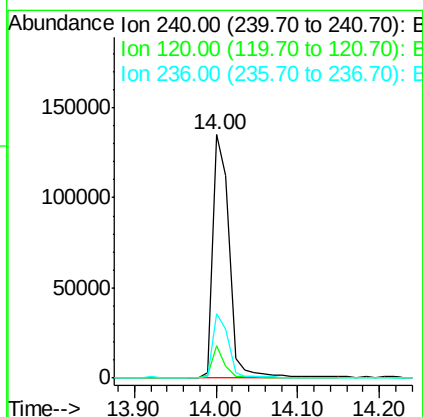

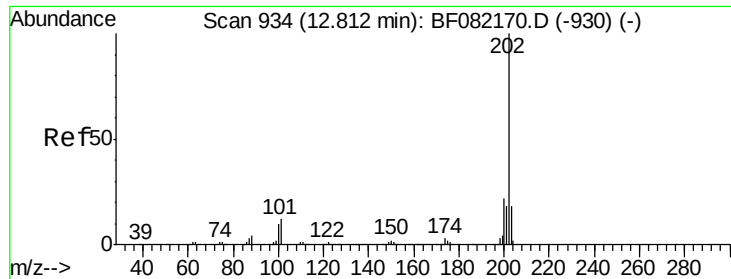

#77

Pyrene

Concen: 21.01 ng

RT: 12.81 min Scan# 934

Delta R.T. 0.00 min

Lab File: BF082205.D

Acq: 11 Oct 2015 5:40

Instrument :

BNA_F


ClientSampleId :

A16COMP




Tgt	Ion	Resp	Lower	Upper
202	100			
200	20.3	17.9	26.9	
203	17.1	14.5	21.7	

Manual Integrations
APPROVED

MMDadoda
10/12/2015 2:38:27 PM

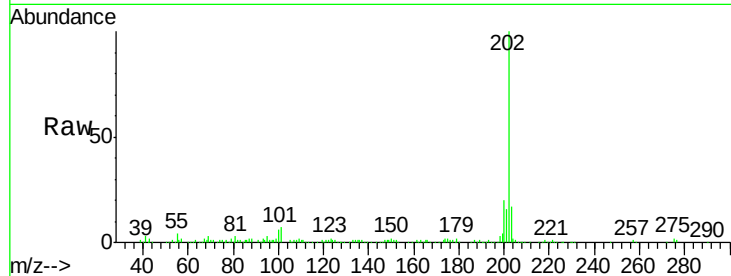

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E

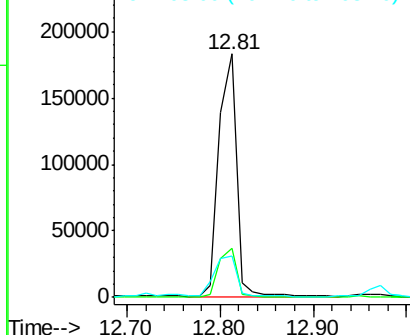

#78

Terphenyl-d14

Concen: 65.40 ng


RT: 12.95 min Scan# 946

Delta R.T. -0.01 min



Lab File: BF082205.D


Acq: 11 Oct 2015 5:40

Tgt	Ion	Resp	Lower	Upper
244	100			
212	7.6	5.8	8.6	
122	12.7	5.9	8.9#	



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

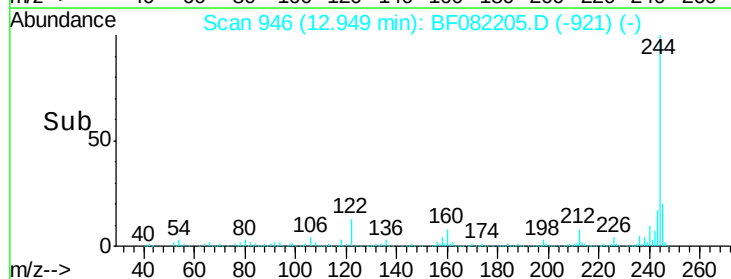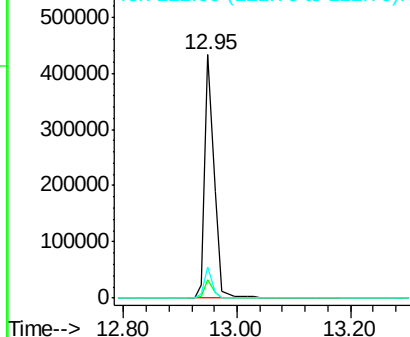

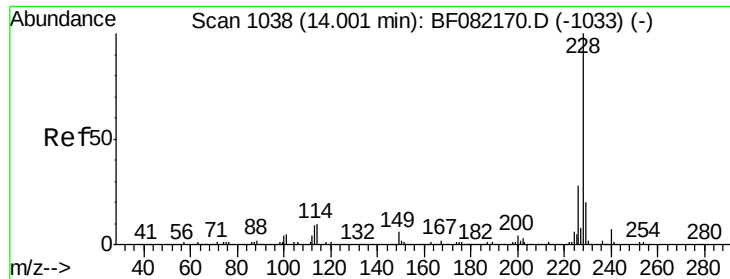





#80
Benzo(a)anthracene
Concen: 11.65 ng
RT: 14.00 min Scan# 1038
Delta R.T. 0.00 min
Lab File: BF082205.D
Acq: 11 Oct 2015 5:40

Instrument :
BNA_F
ClientSampleId :
A16COMP

Tgt Ion	Ratio	Lower	Upper
228	100		
226	29.8	22.3	33.5
229	21.8	16.2	24.2




Manual Integrations
APPROVED


MMDadoda
10/12/2015 2:38:27 PM

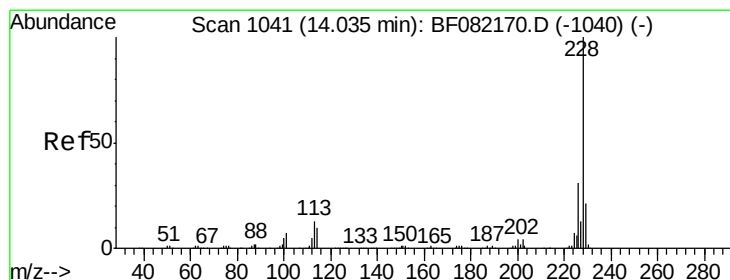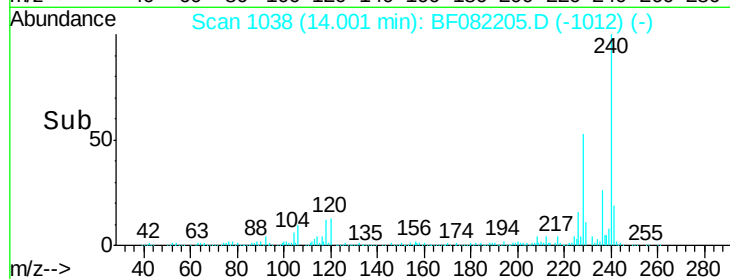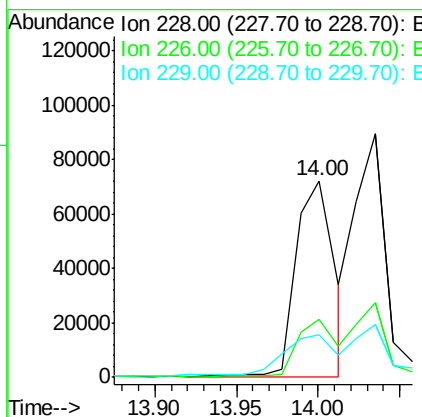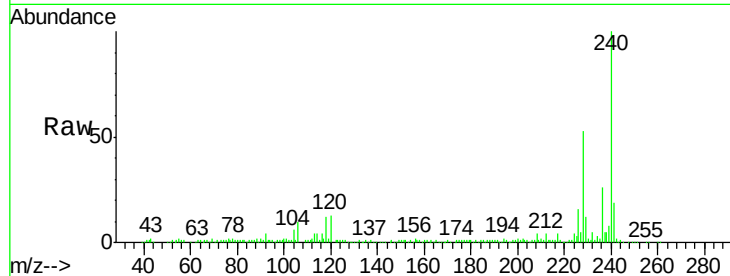

#82
Chrysene
Concen: 11.56 ng
RT: 14.04 min Scan# 1041
Delta R.T. 0.00 min
Lab File: BF082205.D
Acq: 11 Oct 2015 5:40

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.4	24.4	36.6
229	21.6	16.3	24.5

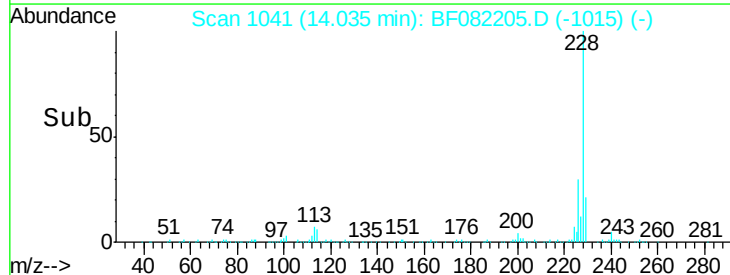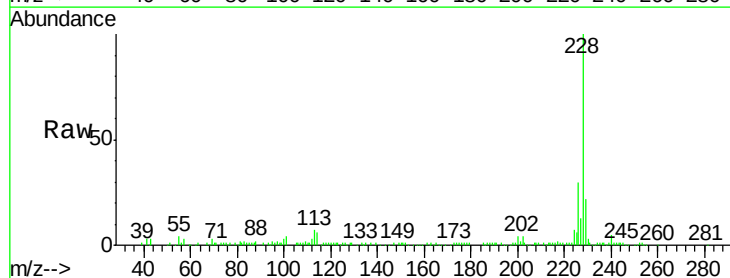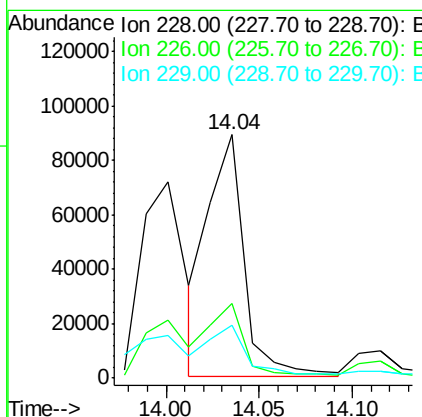

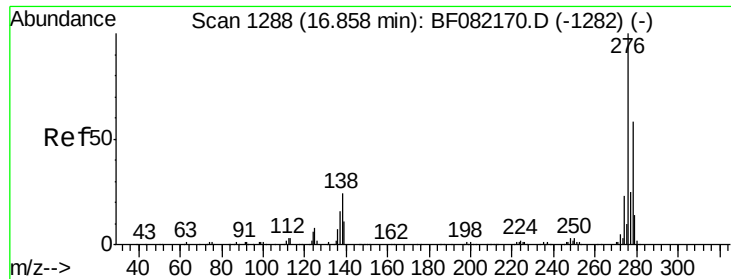





#85
Indeno(1,2,3-cd)pyrene
Concen: 9.75 ng
RT: 16.85 min Scan# 1287
Delta R.T. -0.01 min
Lab File: BF082205.D
Acq: 11 Oct 2015 5:40

Instrument :
BNA_F
ClientSampleId :
A16COMP

Tgt Ion	Ratio	Lower	Upper
276	100		
138	23.0	19.7	29.5
277	22.6	20.1	30.1




Manual Integrations
APPROVED


MMDadoda
10/12/2015 2:38:27 PM

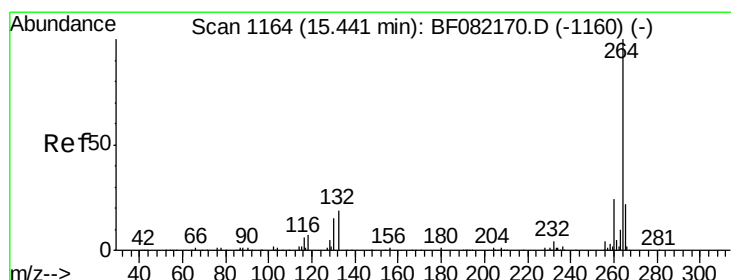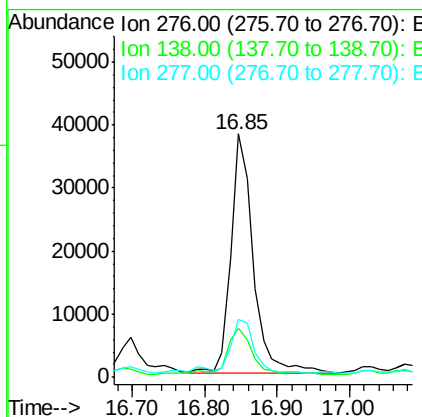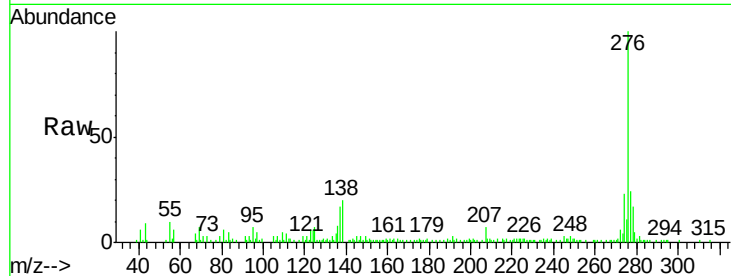

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.44 min Scan# 1164
Delta R.T. 0.00 min
Lab File: BF082205.D
Acq: 11 Oct 2015 5:40

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.7	19.0	28.6
265	22.7	17.3	25.9

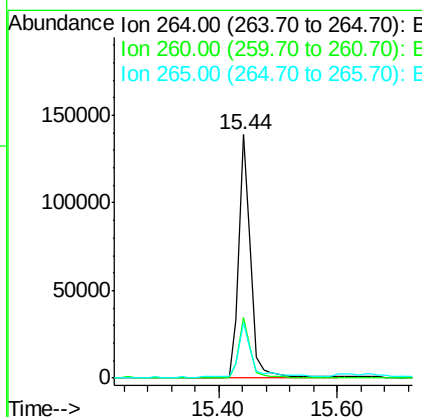

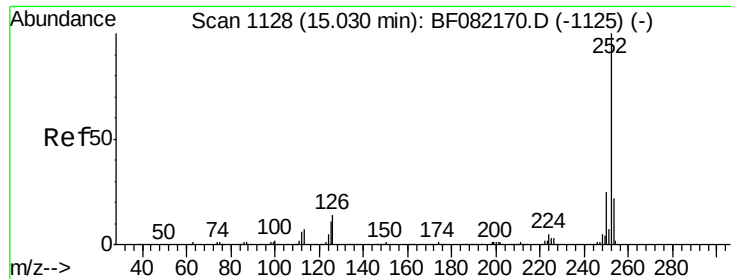

#87

Benzo(b)fluoranthene

Concen: 15.51 ng m

RT: 15.03 min Scan# 1128

Delta R.T. 0.00 min

Lab File: BF082205.D

Acq: 11 Oct 2015 5:40

Instrument :

BNA_F





ClientSampleId :

A16COMP

Tgt Ion:	252	Resp:	183497
Ion Ratio	Lower	Upper	
252	100		
253	23.0	18.0	27.0
125	10.1	8.6	12.8

Manual Integrations
APPROVED

MMDadoda
10/12/2015 2:38:27 PM

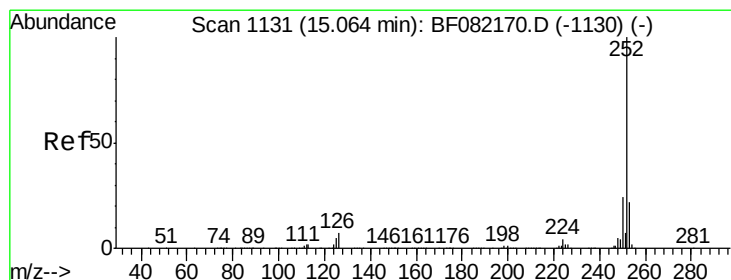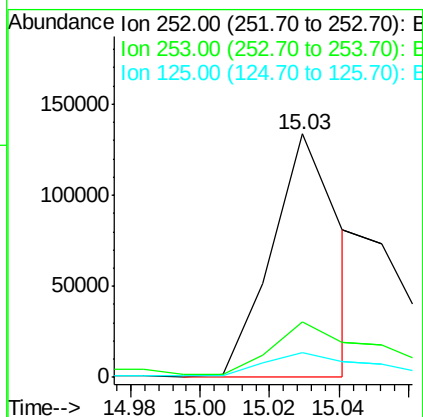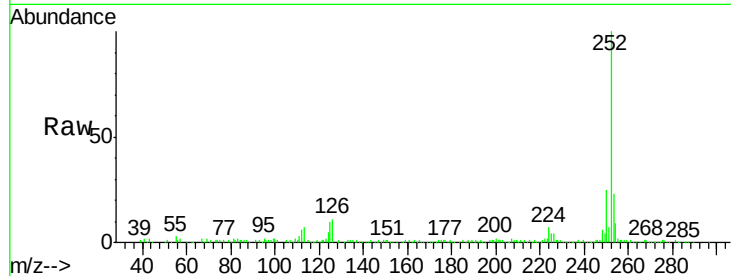

#88

Benzo(k)fluoranthene

Concen: 8.27 ng m




RT: 15.04 min Scan# 1129


Delta R.T. -0.02 min

Lab File: BF082205.D

Acq: 11 Oct 2015 5:40

Tgt Ion:	252	Resp:	82222
Ion Ratio	Lower	Upper	
252	100		
253	23.5	17.8	26.6
125	10.5	6.7	10.1#

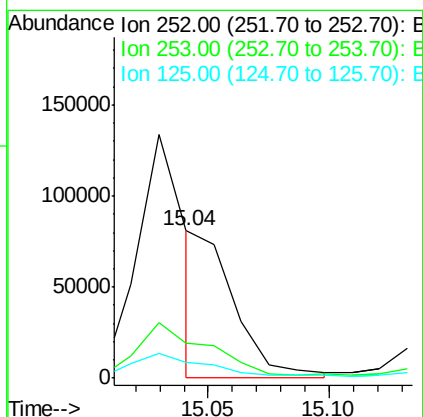



#89

Benzo(a)pyrene

Concen: 11.68 ng

RT: 15.38 min Scan# 1159

Delta R.T. 0.00 min

Lab File: BF082205.D

Acq: 11 Oct 2015 5:40

Instrument :

BNA_F


ClientSampleId :

A16COMP




Tgt Ion:	252	Resp:	118687
Ion Ratio		Lower	Upper
252	100		
253	23.1	18.2	27.2
125	9.5	8.9	13.3

Manual Integrations
APPROVED

MMDadoda
10/12/2015 2:38:27 PM



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

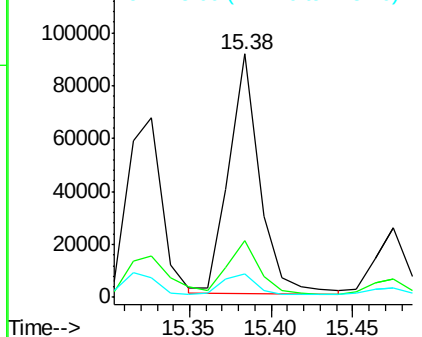

#91

Benzo(g,h,i)perylene

Concen: 9.36 ng


RT: 17.27 min Scan# 1324

Delta R.T. -0.01 min

Lab File: BF082205.D

Acq: 11 Oct 2015 5:40

Tgt Ion:	276	Resp:	75705
Ion Ratio		Lower	Upper
276	100		
277	24.9	18.8	28.2
138	22.8	17.4	26.2



Abundance Ion 276.00 (275.70 to 276.70): E
Ion 277.00 (276.70 to 277.70): E
Ion 138.00 (137.70 to 138.70): E

