


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101015\
 Data File : BF082165.D
 Acq On : 10 Oct 2015 9:26
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 12 01:46:21 2015

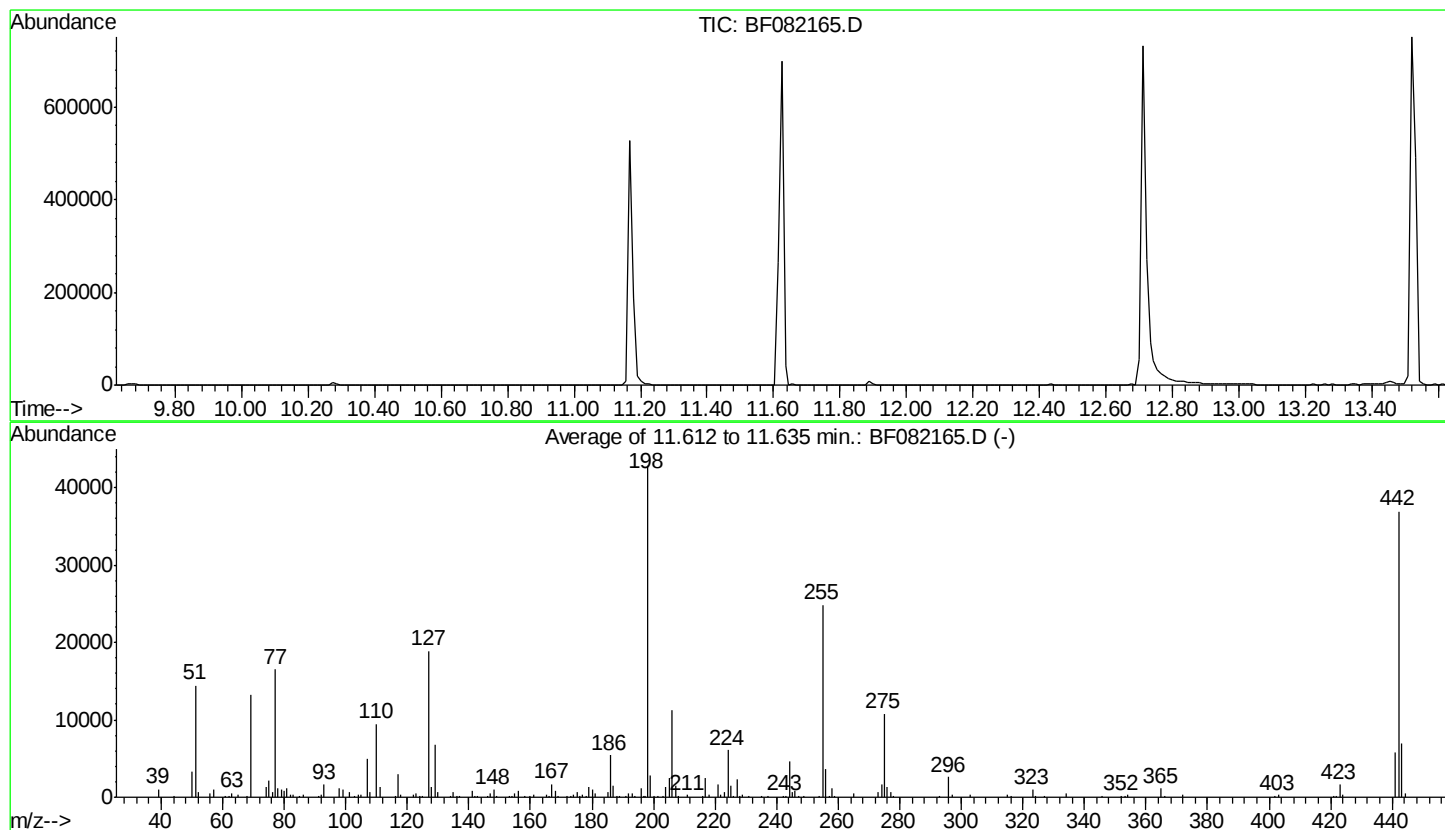

AutoFind: Scans 829, 830, 831; Background Corrected with Scan 826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	14458	PASS
68	69	0.00	2	1.6	219	PASS
69	198	0.00	100	31.0	13302	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.1	18886	PASS
197	198	0.00	2	0.4	158	PASS
198	198	100	100	100.0	42854	PASS
199	198	5	9	6.6	2823	PASS
275	198	10	60	25.2	10782	PASS
365	198	1	100	2.7	1146	PASS
441	442	0.01	24	15.5	5733	PASS
442	198	50	100	86.1	36904	PASS
443	442	15	24	18.8	6932	PASS