


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101015\
 Data File : BF082189.D
 Acq On : 10 Oct 2015 21:41
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 12 01:46:21 2015

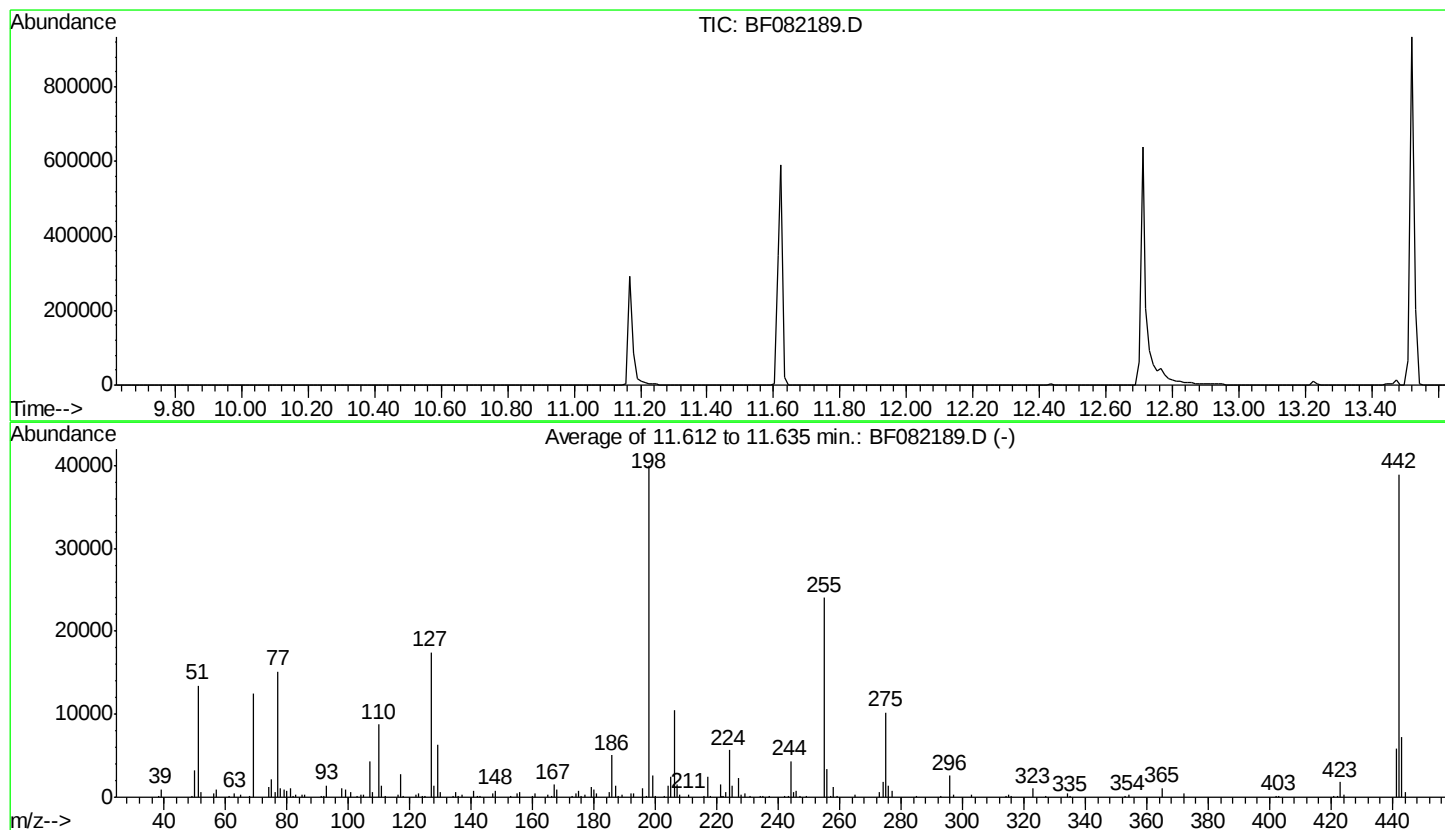

AutoFind: Scans 829, 830, 831; Background Corrected with Scan 825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	13457	PASS
68	69	0.00	2	1.1	131	PASS
69	198	0.00	100	31.2	12461	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.8	17492	PASS
197	198	0.00	2	0.3	124	PASS
198	198	100	100	100.0	39968	PASS
199	198	5	9	6.7	2687	PASS
275	198	10	60	25.5	10192	PASS
365	198	1	100	2.8	1106	PASS
441	442	0.01	24	15.1	5878	PASS
442	198	50	100	97.5	38949	PASS
443	442	15	24	18.8	7309	PASS