


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101016\
Data File : BF090483.D
Acq On : 10 Oct 2016 12:05
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF100516.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 05 14:57:00 2016

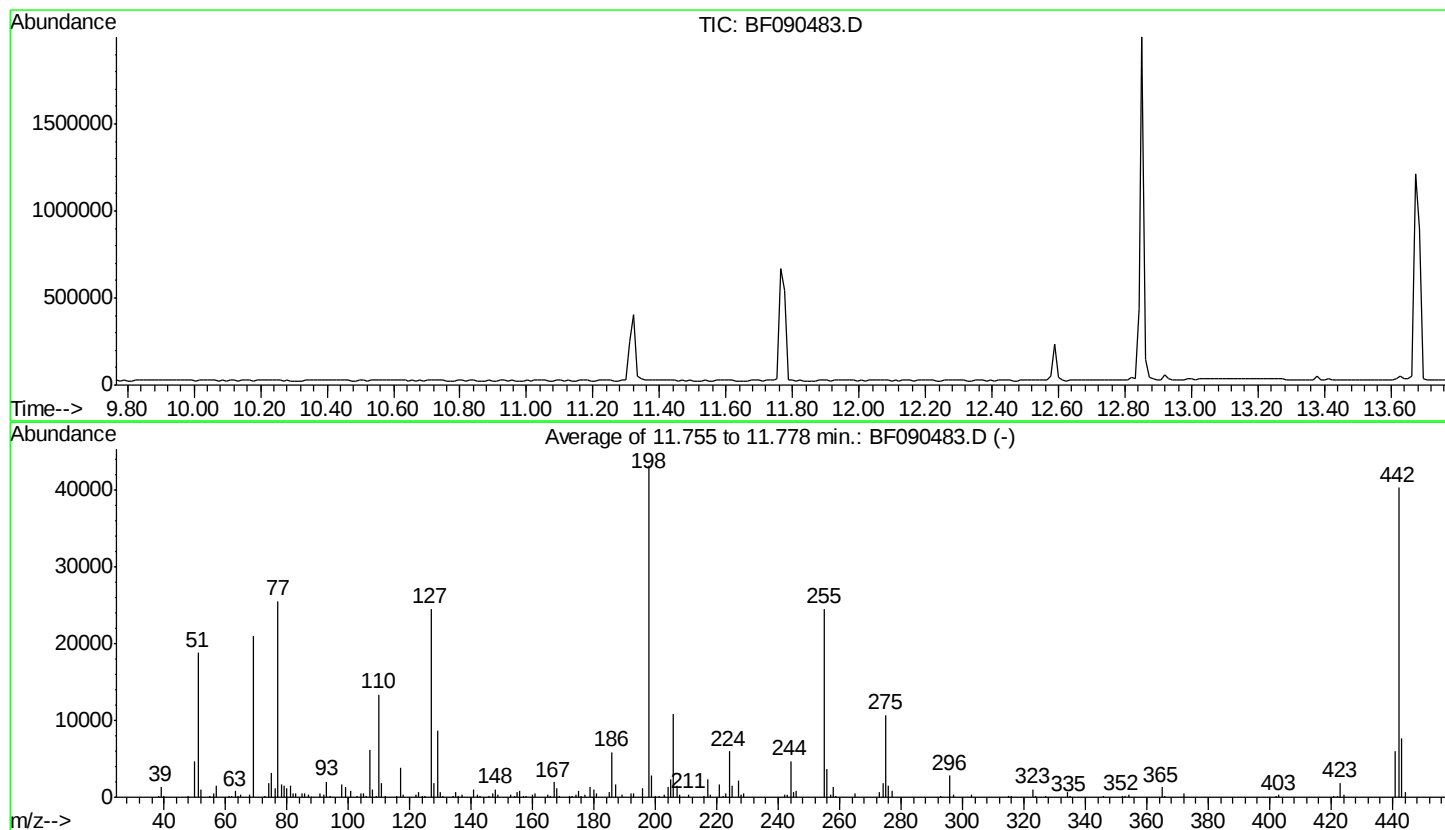

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 821

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	18779	PASS
68	69	0.00	2	1.3	273	PASS
69	198	0.00	100	48.5	20962	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.8	24522	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43186	PASS
199	198	5	9	6.6	2855	PASS
275	198	10	60	24.9	10756	PASS
365	198	1	100	3.0	1310	PASS
441	442	0.01	24	15.0	6053	PASS
442	198	50	100	93.3	40280	PASS
443	442	15	24	19.0	7664	PASS