
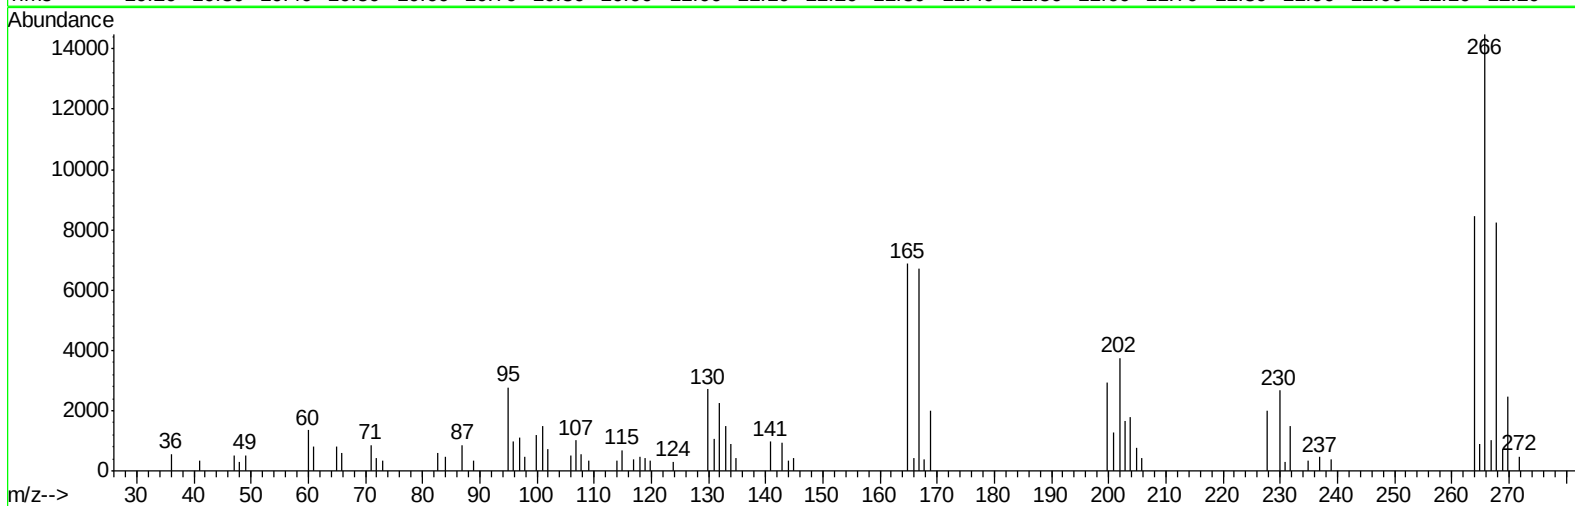


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101017\  
Data File : BF099329.D  
Acq On : 11 Oct 2017 4:54  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 11 08:42:56 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 05 17:20:48 2017  
Response via : Initial Calibration

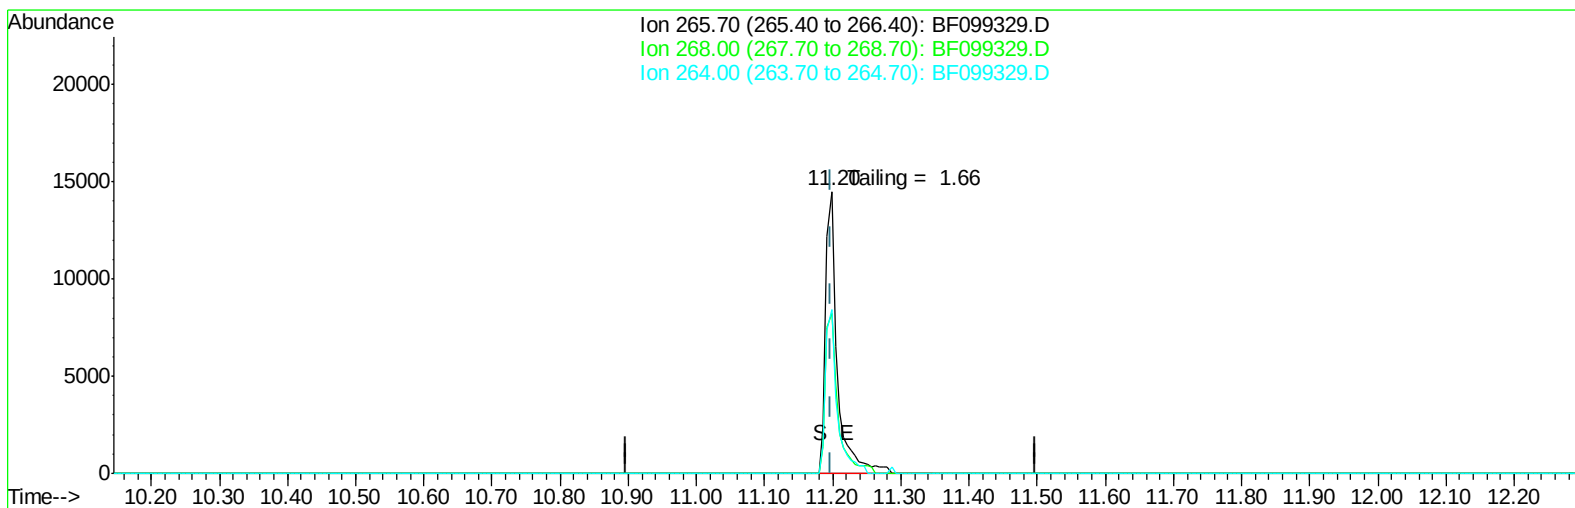

TIC: BF099329.D

(69) Pentachlorophenol (C)



11.198min (-0.000) 0.00ng

response 16798

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 57.01 |
| 264.00 | 61.90 | 58.24 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101017\  
Data File : BF099329.D  
Acq On : 11 Oct 2017 4:54  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 11 08:42:56 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 05 17:20:48 2017  
Response via : Initial Calibration

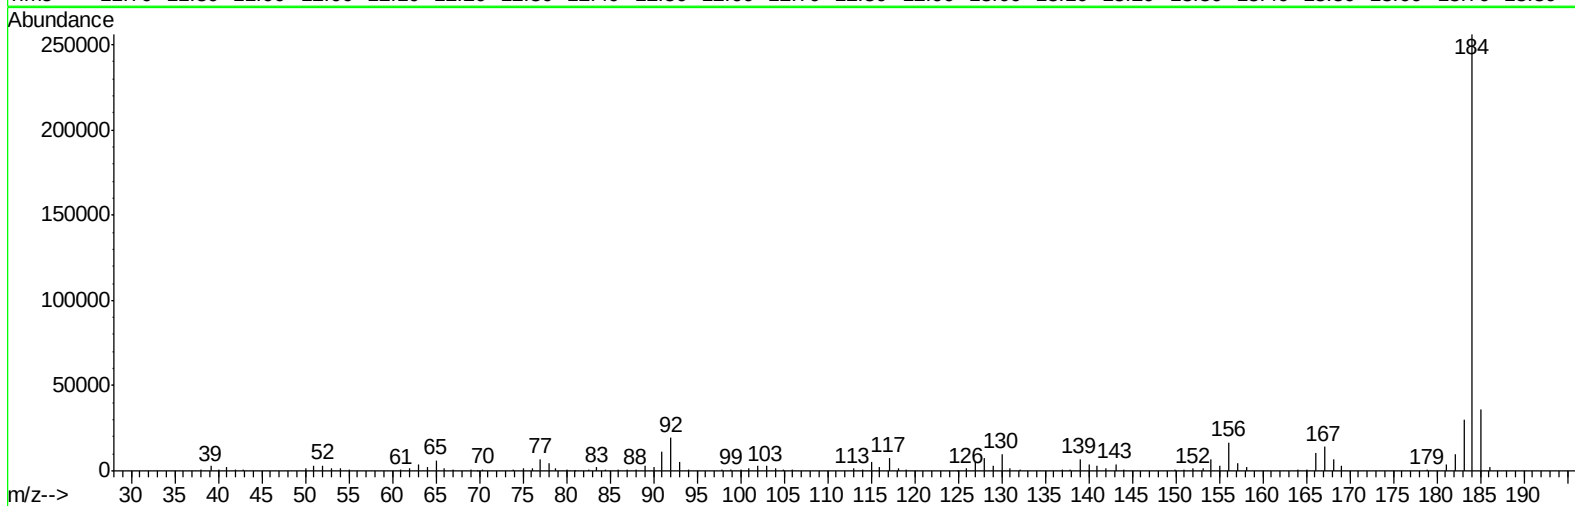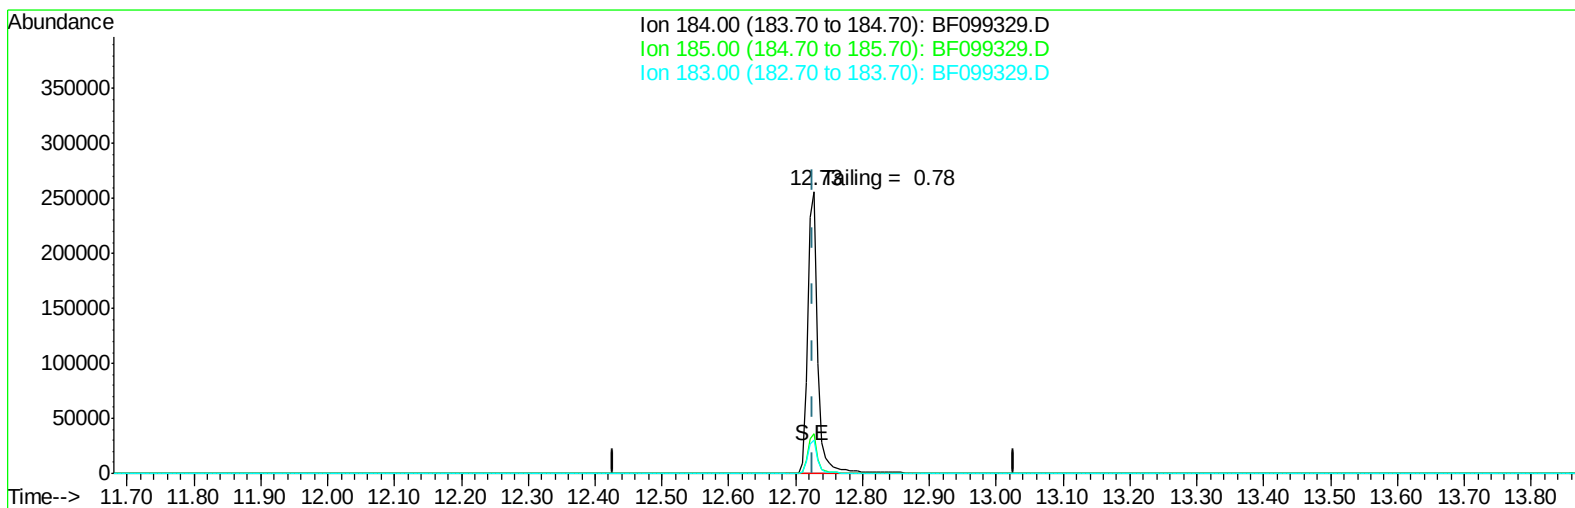

TIC: BF099329.D

(76) Benzidine

12.727min (-0.000) 57286.72ng

response 271211

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 13.96 |
| 183.00 | 11.60 | 11.65 |
| 0.00   | 0.00  | 0.00  |