


Data Path : Z:\HPCHEM1\BNA F\Data\BF101017\
 Data File : BF099290.D
 Acq On : 10 Oct 2017 9:36
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 05 17:20:48 2017

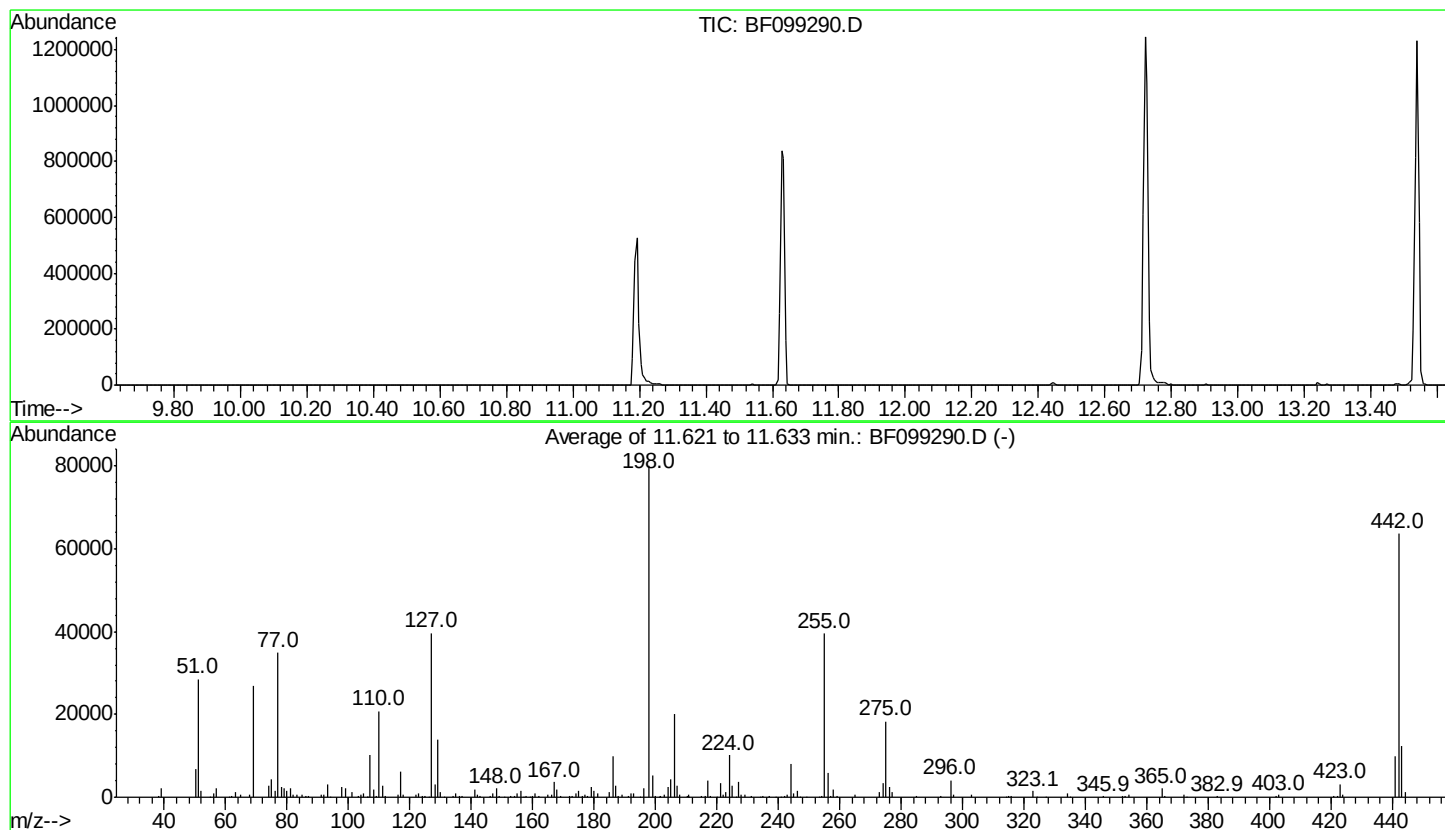

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	28586	PASS
68	69	0.00	2	2.0	543	PASS
69	198	0.00	100	33.8	27044	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.4	39597	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80098	PASS
199	198	5	9	6.7	5406	PASS
275	198	10	60	22.8	18297	PASS
365	198	1	100	2.6	2058	PASS
441	442	0.01	24	15.8	10055	PASS
442	198	50	100	79.4	63564	PASS
443	442	15	24	19.3	12264	PASS