


Data Path : Z:\HPCHEM1\BNA F\Data\BF101017\
 Data File : BF099329.D
 Acq On : 11 Oct 2017 4:54
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 05 17:20:48 2017

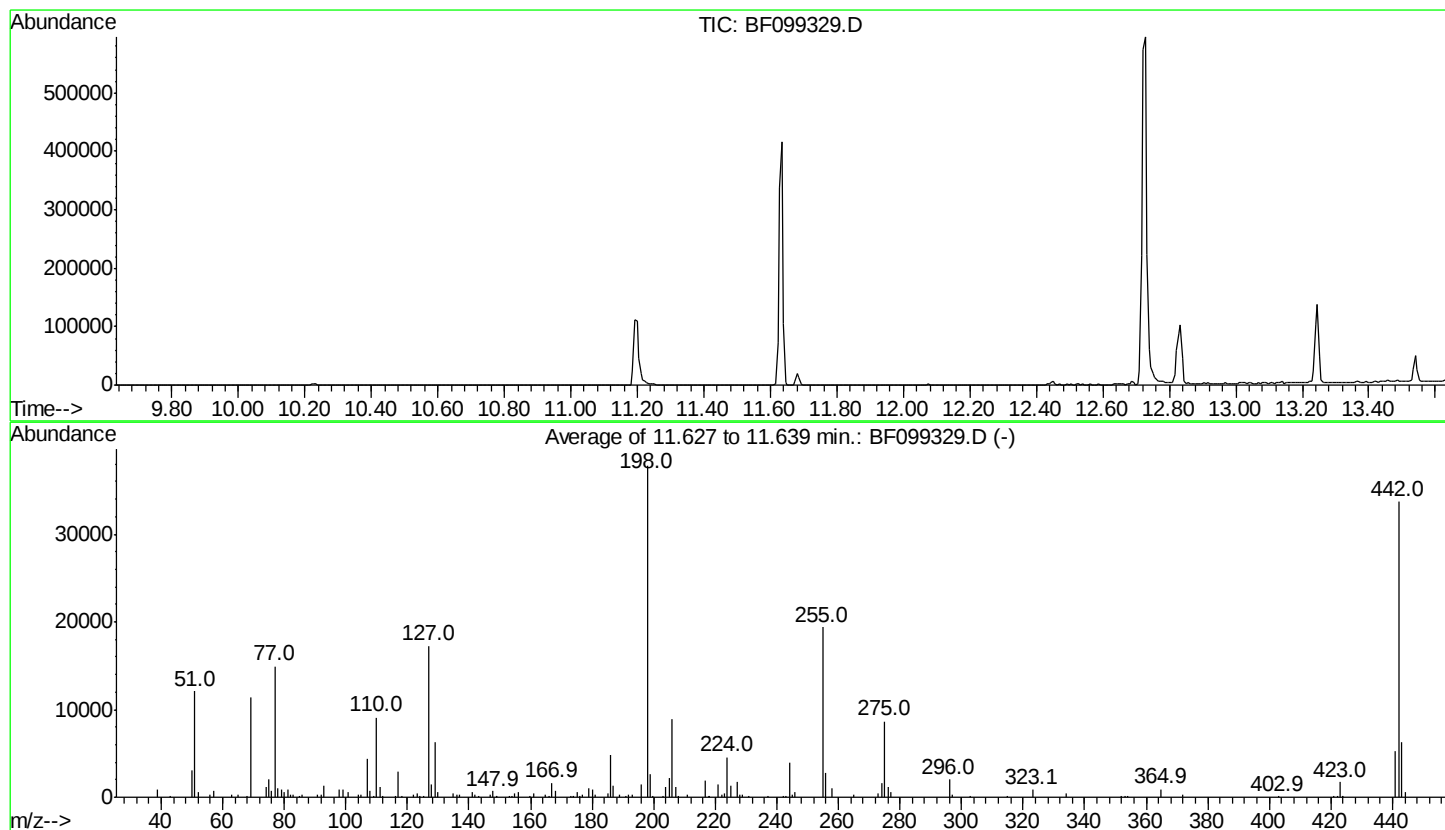

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	12073	PASS
68	69	0.00	2	1.1	122	PASS
69	198	0.00	100	30.3	11456	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.7	17280	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	37822	PASS
199	198	5	9	7.0	2630	PASS
275	198	10	60	22.8	8638	PASS
365	198	1	100	2.3	887	PASS
441	442	0.01	24	15.7	5276	PASS
442	198	50	100	89.1	33701	PASS
443	442	15	24	18.6	6282	PASS