
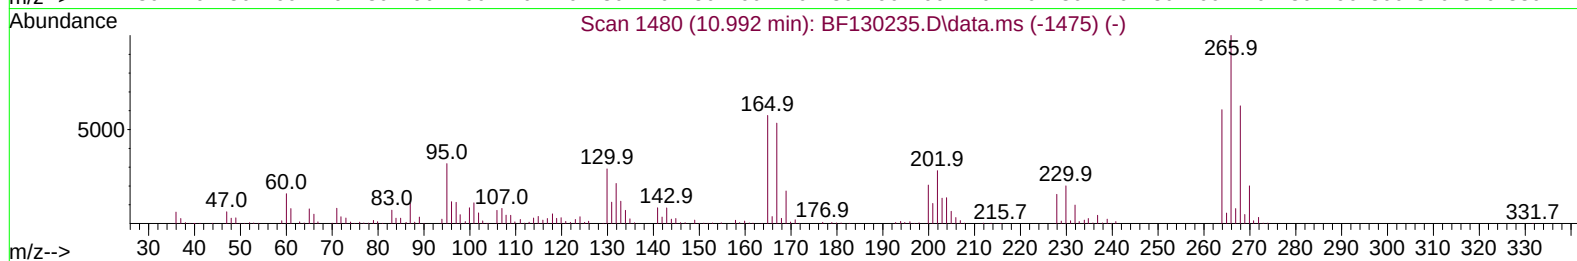
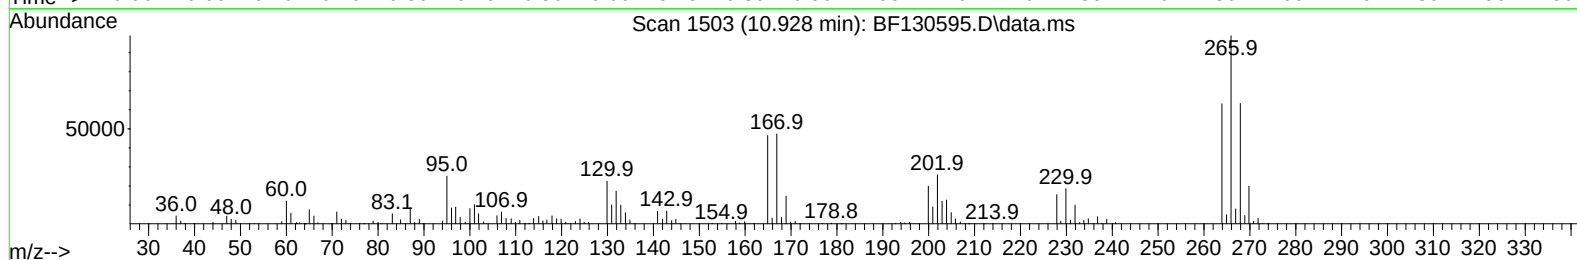


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101022\
 Data File : BF130595.D
 Acq On : 10 Oct 2022 10:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 10 14:07:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 10 13:41:25 2022
 Response via : Initial Calibration

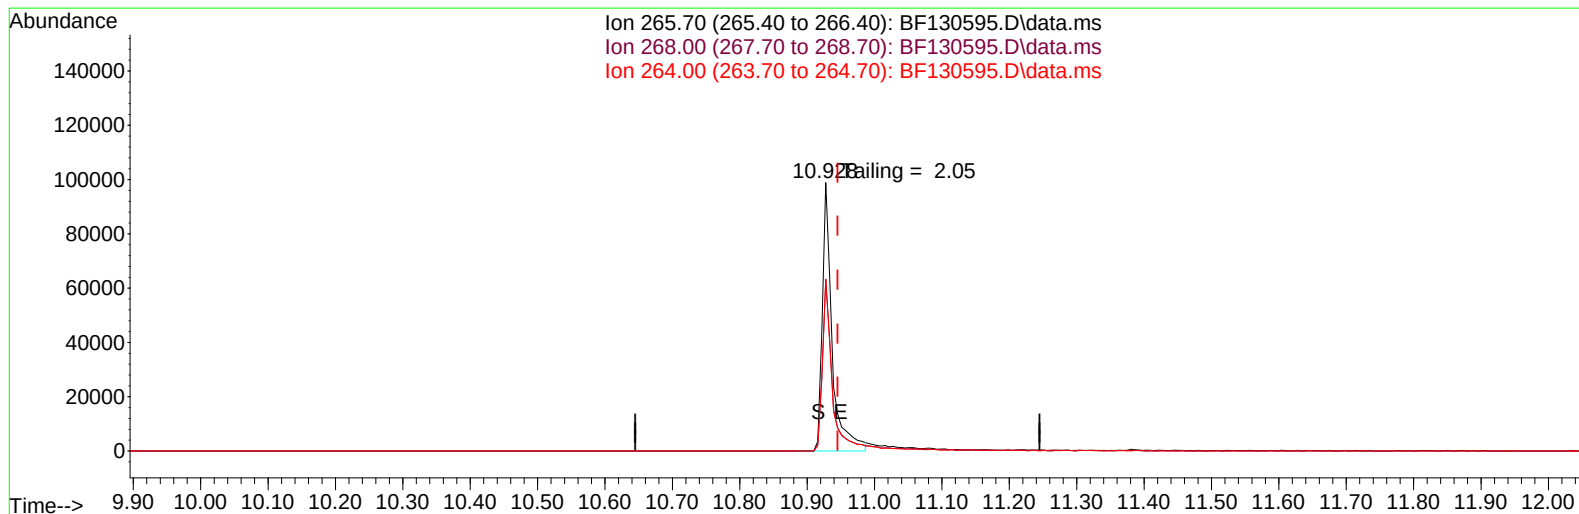

TIC: BF130595.D\data.ms




(70) Pentachlorophenol (C)

10.928min (-0.018) 34727.15 ng

response 106744

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.06
264.00	63.10	63.90
0.00	0.00	0.00

Quant Time: Oct 10 14:07:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 10 13:41:25 2022
Response via : Initial Calibration

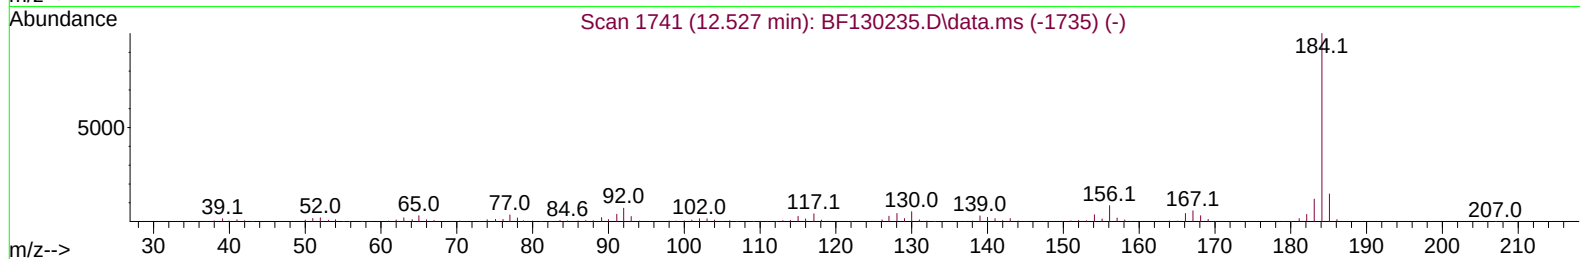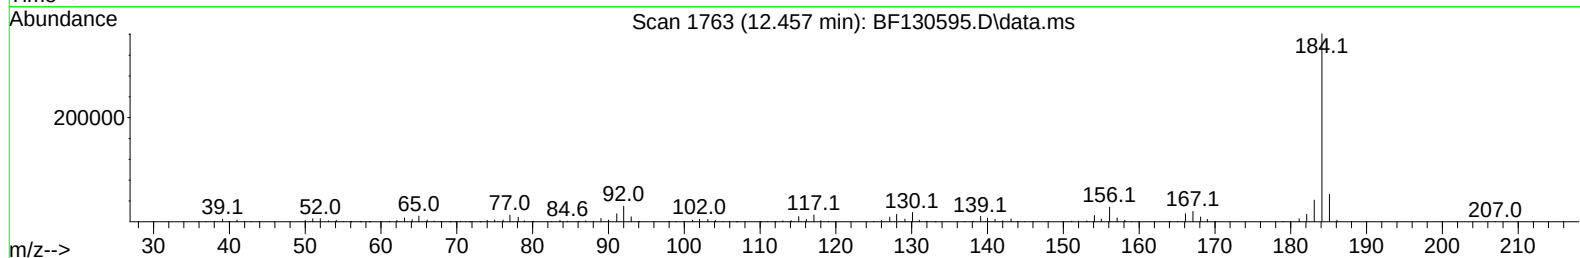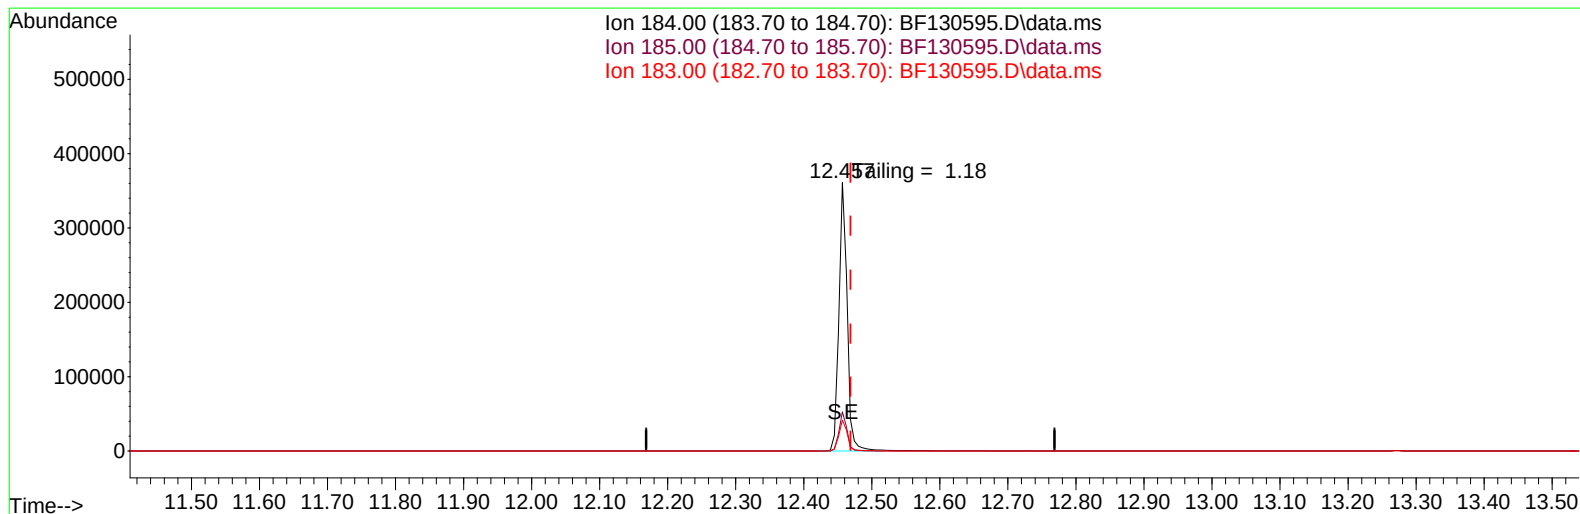

TIC: BF130595.D\data.ms

(77) Benzidine

12.457min (-0.012) 0.00 ng

response **304106**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.61
183.00	11.40	11.55
0.00	0.00	0.00