


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101022\
 Data File : BF130595.D
 Acq On : 10 Oct 2022 10:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 10 16:07:40 2022

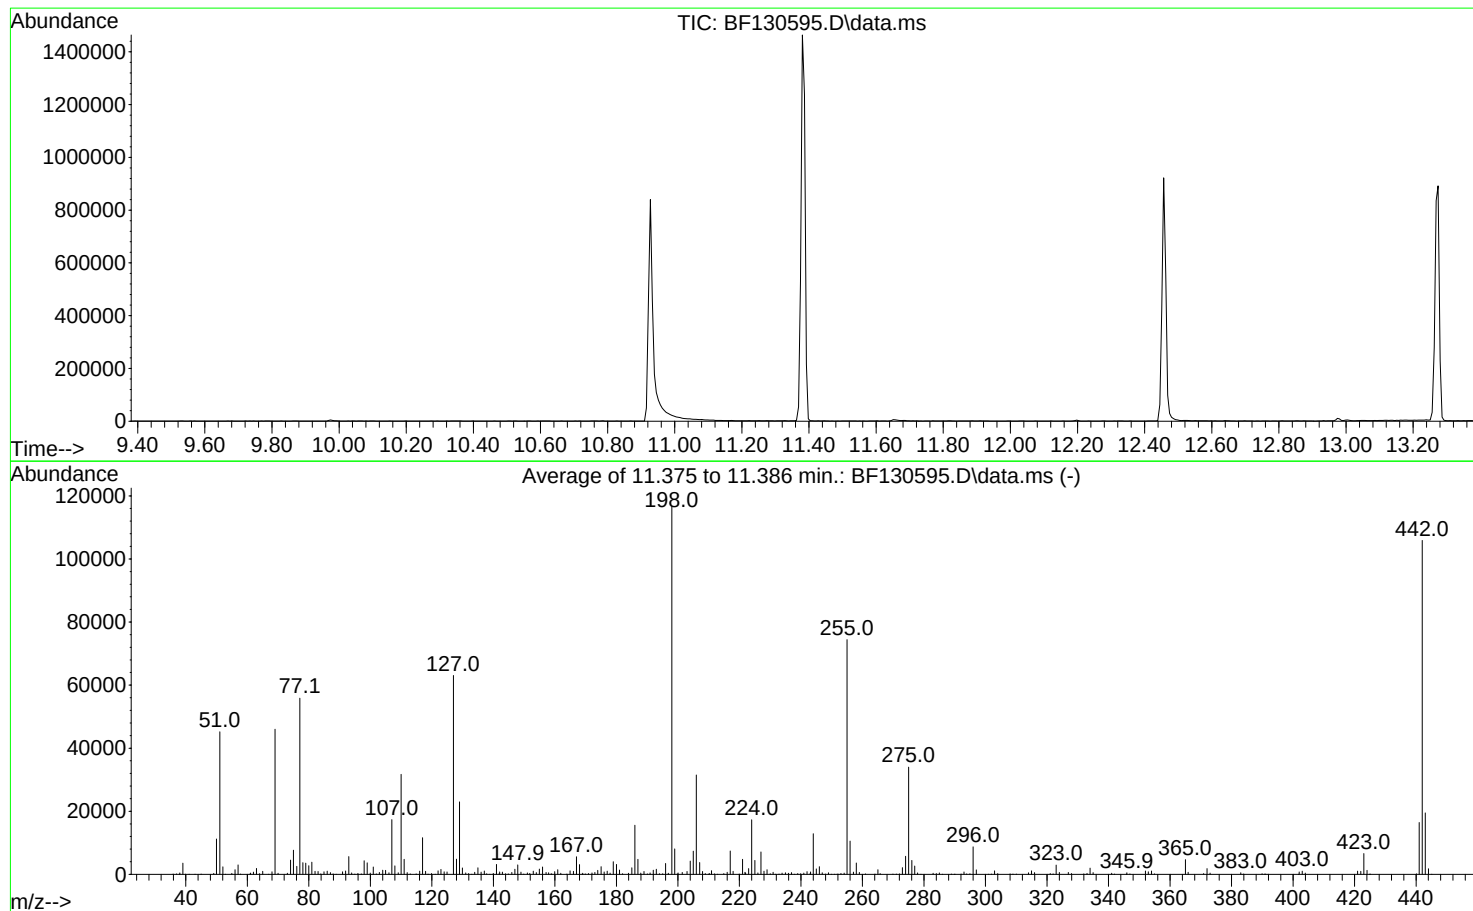

AutoFind: Scans 1579, 1580, 1581; Background Corrected with Scan 1574

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	45227	PASS
68	69	0.00	2	1.8	837	PASS
69	198	0.00	100	39.4	46008	PASS
70	69	0.00	2	0.7	335	PASS
127	198	10	80	54.1	63061	PASS
197	198	0.00	2	0.3	349	PASS
198	198	100	100	100.0	116632	PASS
199	198	5	9	6.9	8080	PASS
275	198	10	60	29.1	33989	PASS
365	198	1	100	4.0	4682	PASS
441	198	0.01	100	14.1	16462	PASS
442	442	50	100	100.0	105867	PASS
443	442	15	24	18.4	19501	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
10/10/2022	BNA_F	<u>BF130595.D</u>
Compound Name	Response	Retention Time
DDT	156599	13.27
DDD	2187	12.97
DDE	166	12.63
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2353	158952	1.48

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101022\
 Data File : BF130595.D
 Acq On : 10 Oct 2022 10:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 10 14:07:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 10 13:41:25 2022
 Response via : Initial Calibration

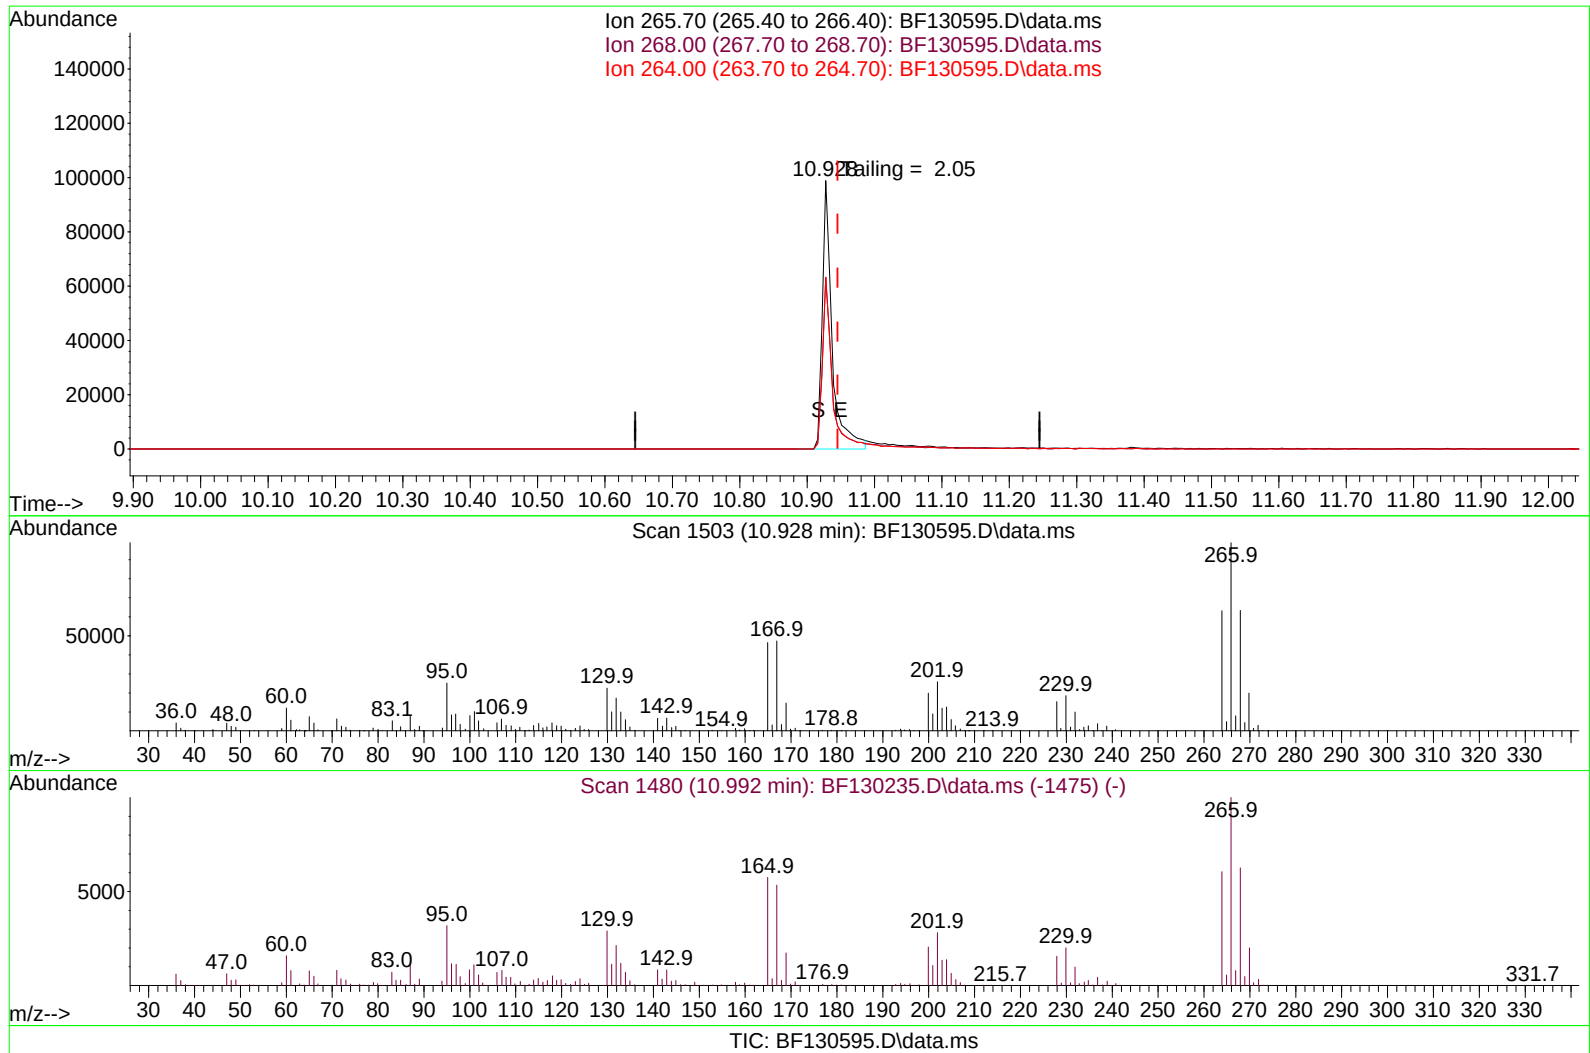

(70) Pentachlorophenol (C)

10.928min (-0.018) 34727.15 ng




response 106744

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.06
264.00	63.10	63.90
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101022\  
Data File : BF130595.D  
Acq On    : 10 Oct 2022  10:09  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 10 14:07:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 10 13:41:25 2022
Response via : Initial Calibration

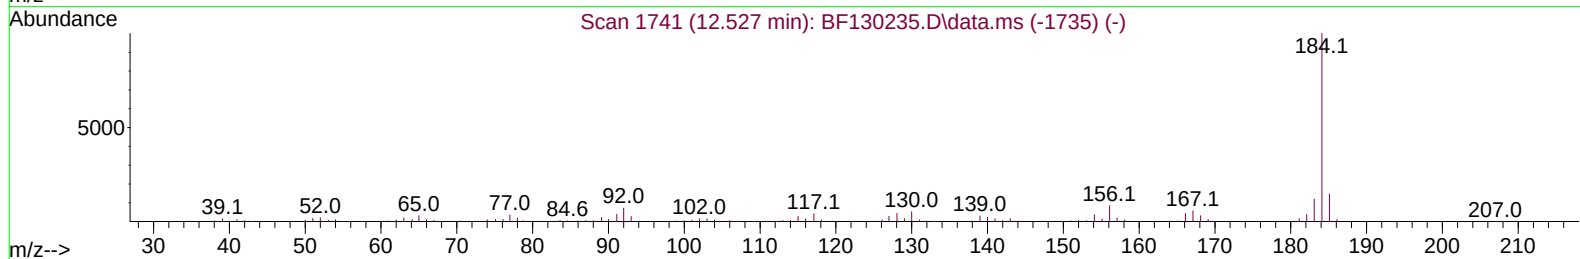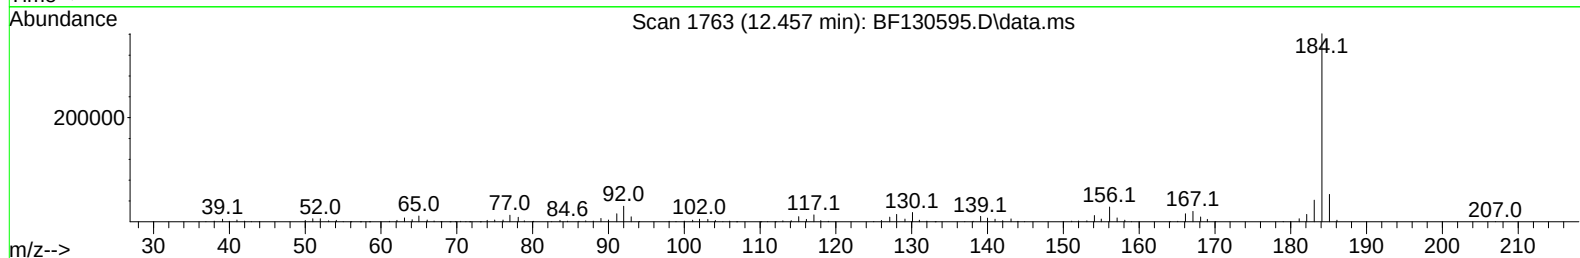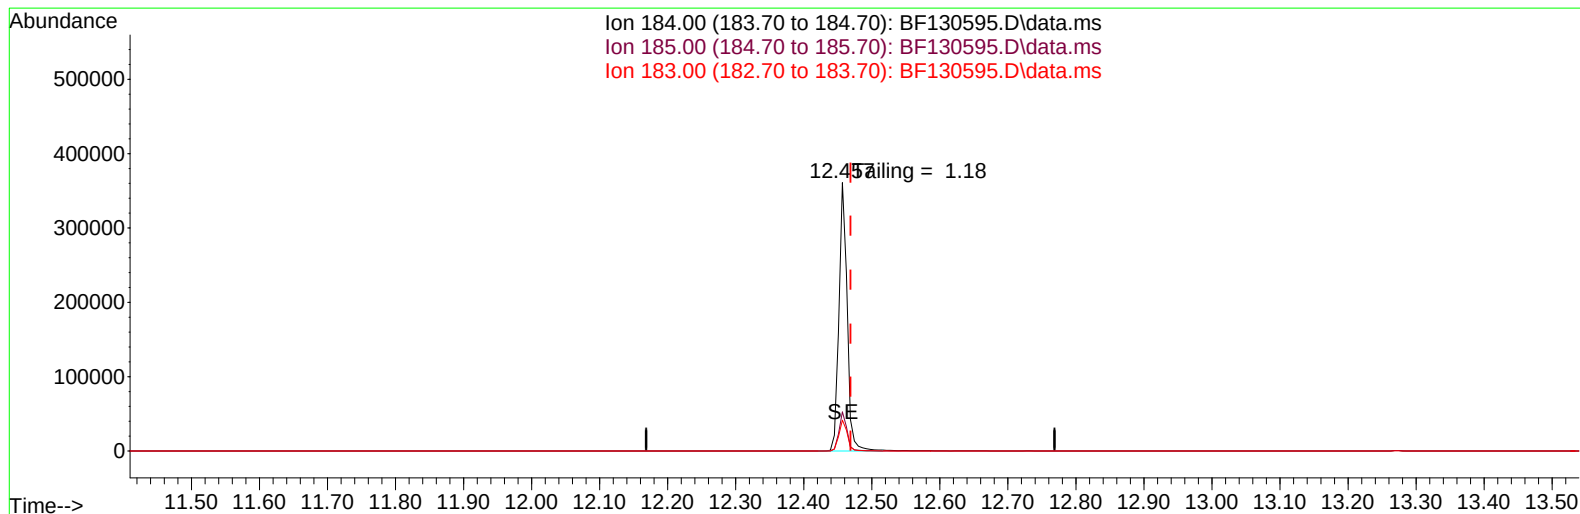

TIC: BF130595.D\data.ms

(77) Benzidine

12.457min (-0.012) 0.00 ng

response **304106**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.61
183.00	11.40	11.55
0.00	0.00	0.00