


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101024\
Data File : BF139736.D
Acq On : 10 Oct 2024 10:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 02 04:58:47 2024

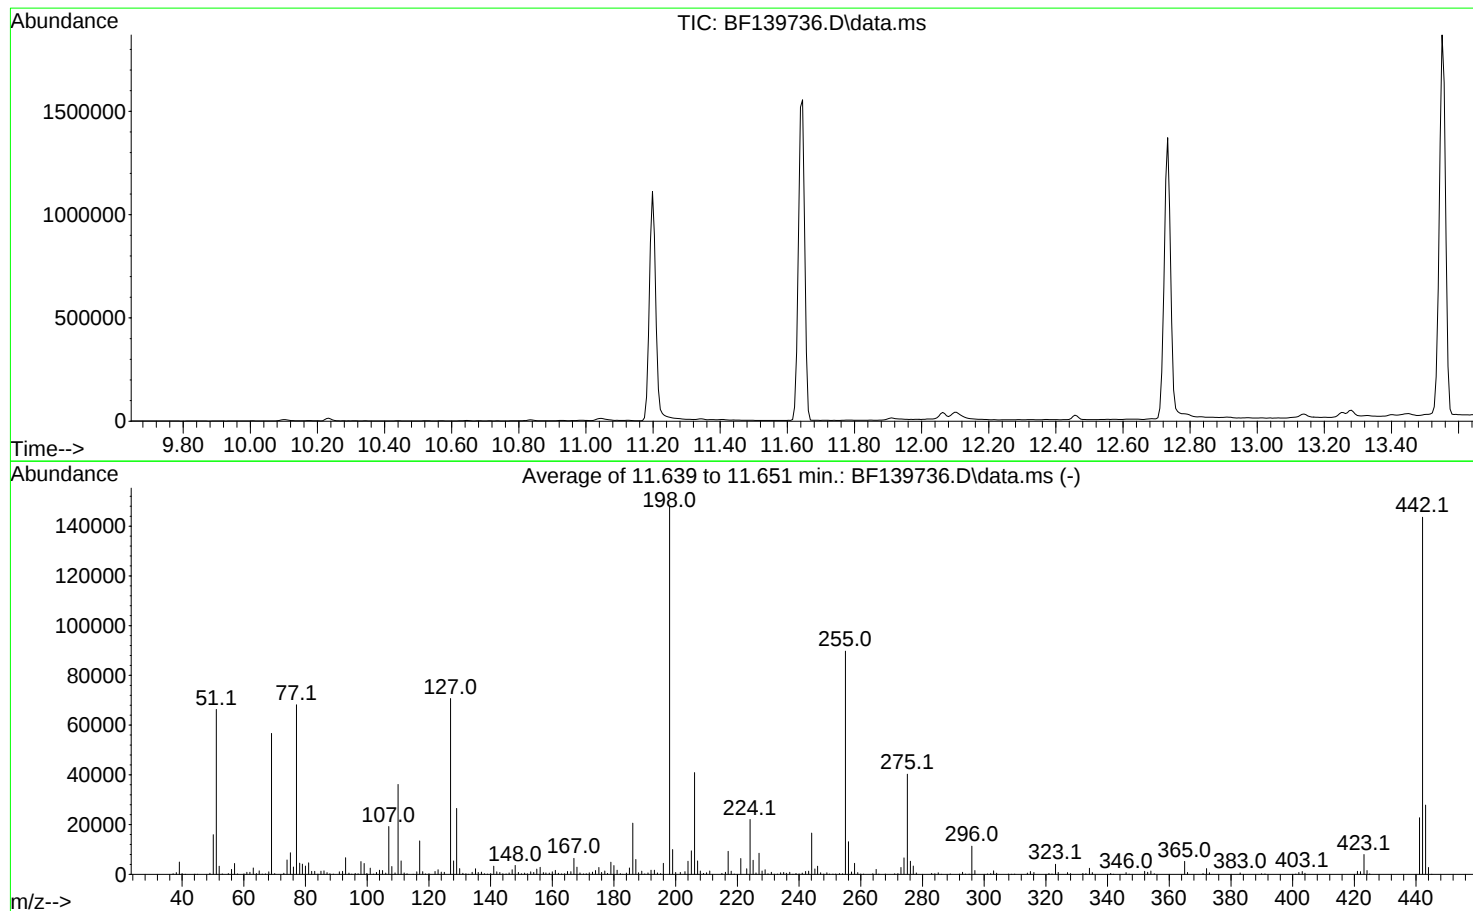




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	66325	PASS
68	69	0.00	2	1.9	1061	PASS
69	198	0.00	100	38.3	56669	PASS
70	69	0.00	2	0.6	351	PASS
127	198	10	80	47.8	70685	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	147896	PASS
199	198	5	9	6.8	10004	PASS
275	198	10	60	27.2	40259	PASS
365	198	1	100	3.5	5187	PASS
441	198	0.01	100	15.4	22803	PASS
442	442	50	100	100.0	143603	PASS
443	442	15	24	19.4	27856	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101024\
Data File : BF139736.D
Acq On : 10 Oct 2024 10:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 10 11:45:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

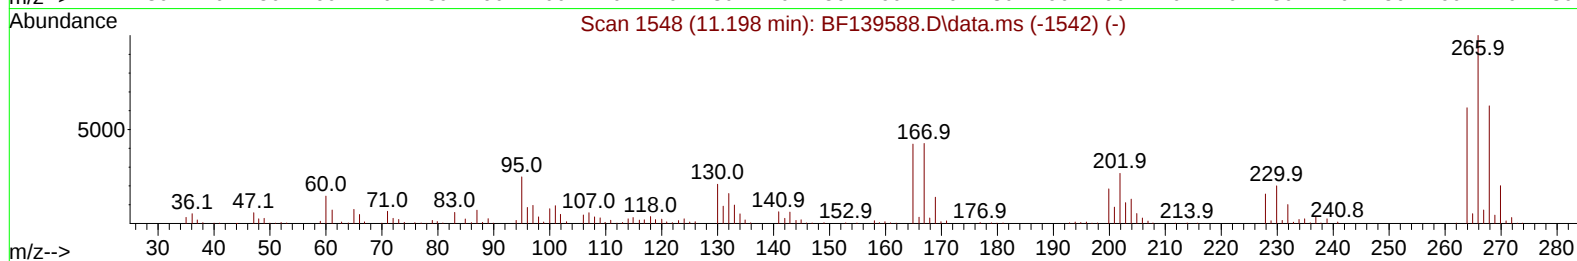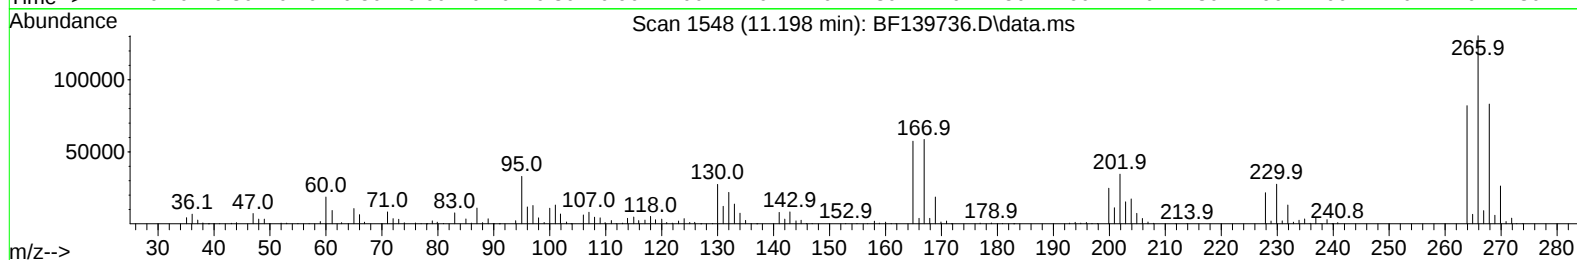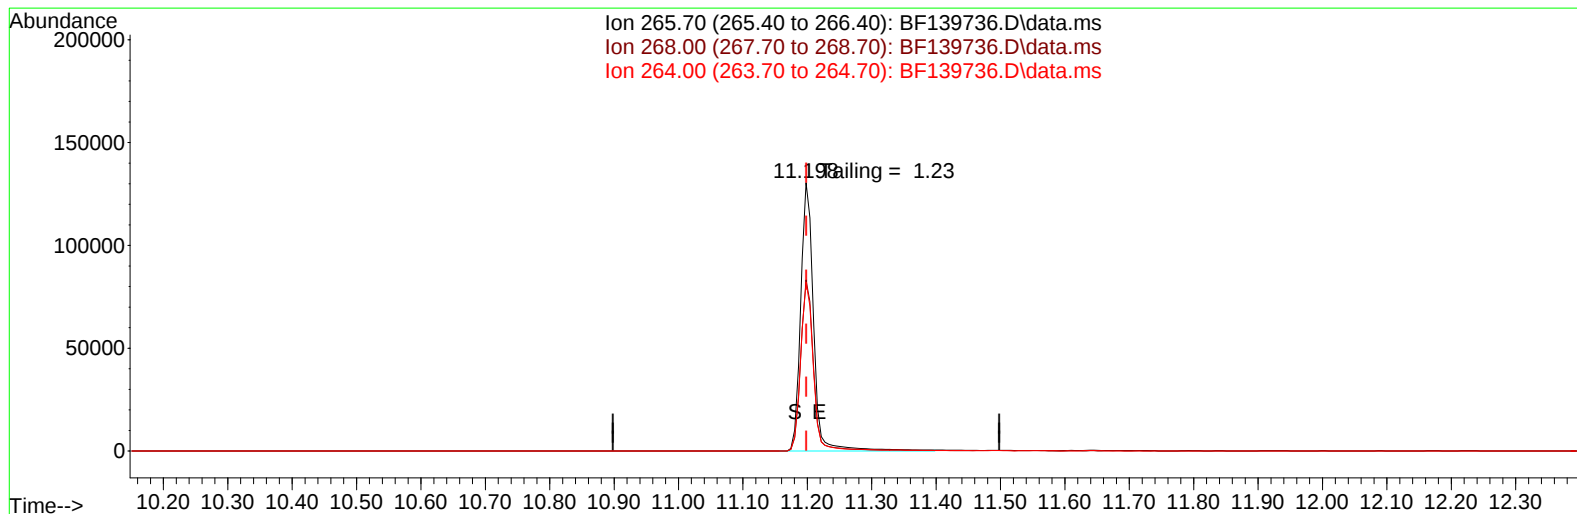

TIC: BF139736.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 29084.41 ng




response 182454

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	63.73
264.00	61.60	62.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101024\
Data File : BF139736.D
Acq On : 10 Oct 2024 10:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 10 11:45:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

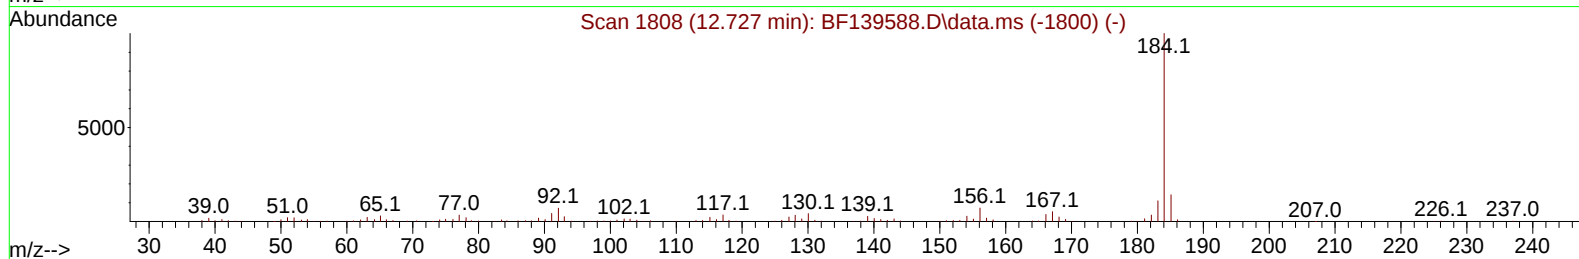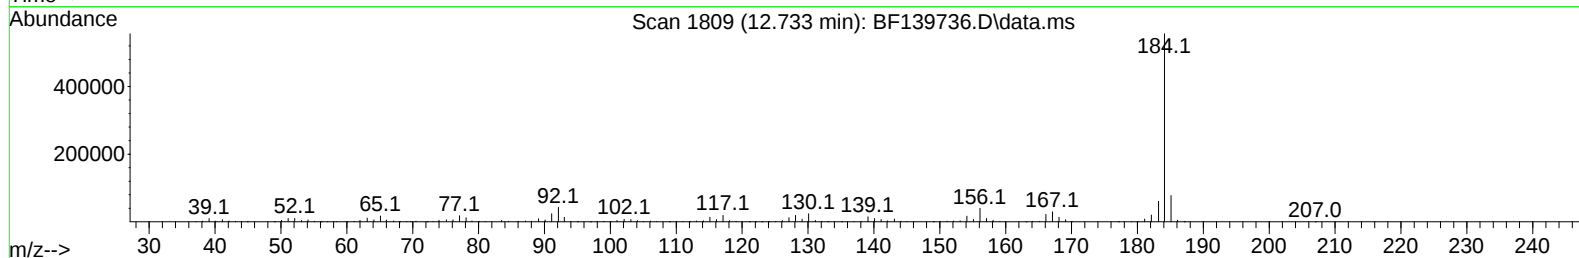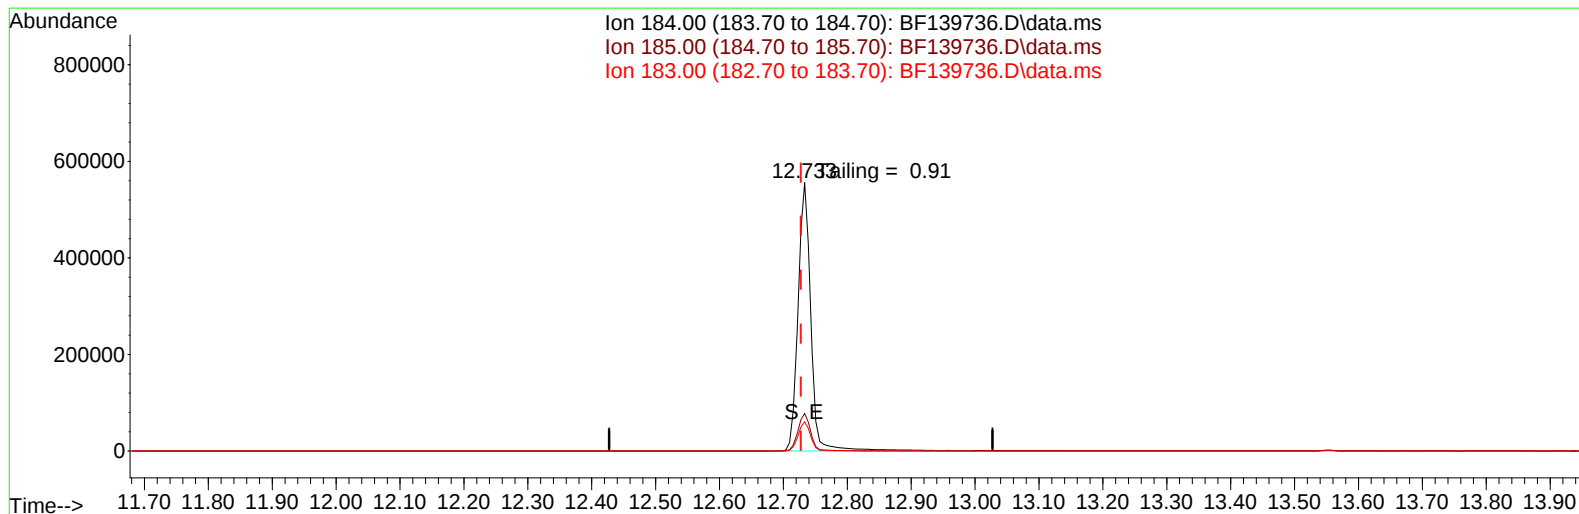

TIC: BF139736.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 798524.11 ng

response 774676

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.03
183.00	11.00	10.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/10/2024	BNA_F	<u>BF139736.D</u>
Compound Name	Response	Retention Time
DDT	458256	13.551
DDD	11223	13.28
DDE	643	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11866	470122	2.52

Instrument :
BNA_F
ClientSampleId :
DFTPP