


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101116\
 Data File : BF090492.D
 Acq On : 11 Oct 2016 9:58
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 11 16:14:43 2016

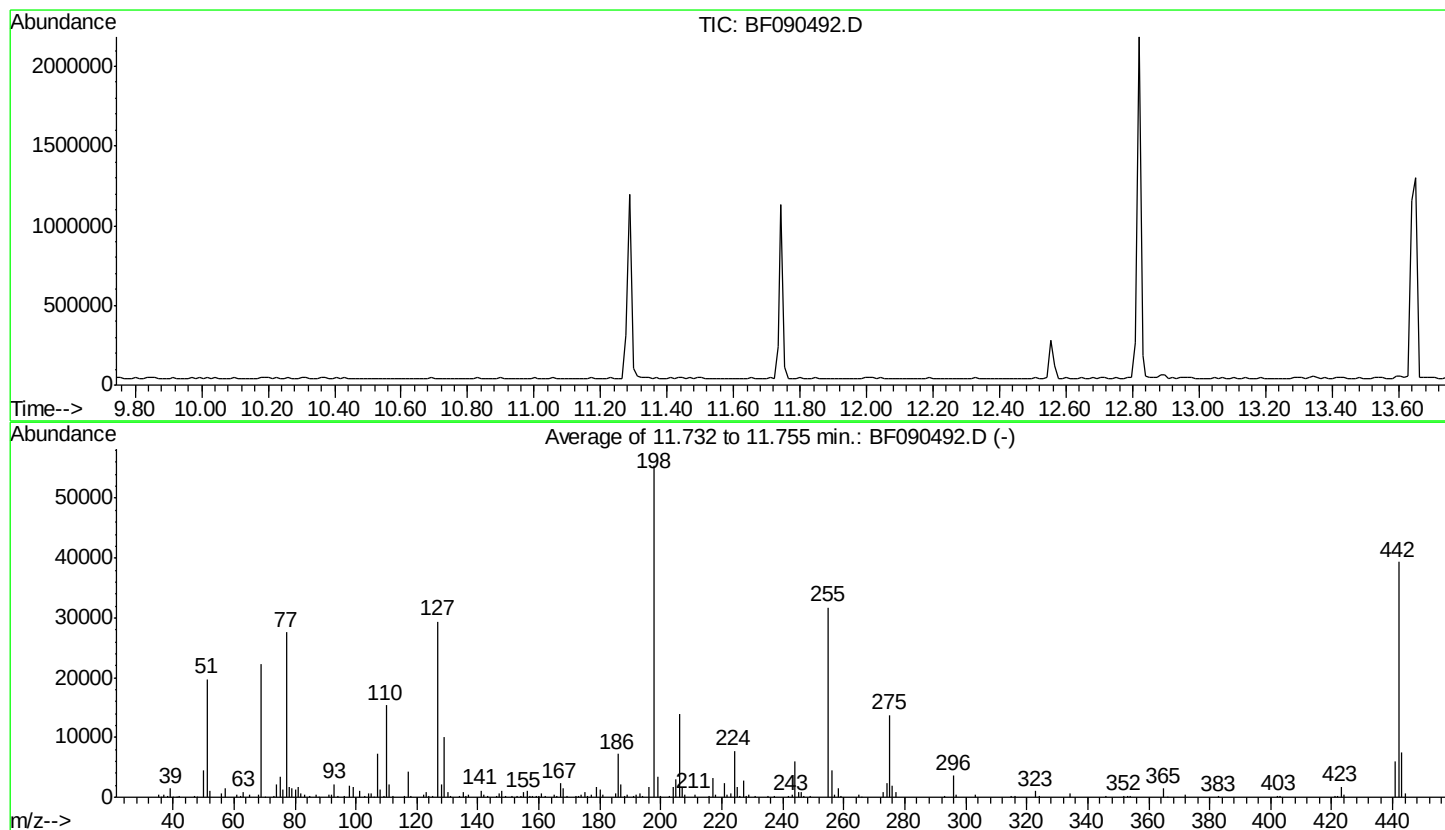

AutoFind: Scans 822, 823, 824; Background Corrected with Scan 819

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	19704	PASS
68	69	0.00	2	1.5	334	PASS
69	198	0.00	100	40.0	22198	PASS
70	69	0.00	2	0.5	104	PASS
127	198	10	80	52.9	29332	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55458	PASS
199	198	5	9	6.3	3502	PASS
275	198	10	60	24.7	13714	PASS
365	198	1	100	2.5	1404	PASS
441	442	0.01	24	15.3	6031	PASS
442	198	50	100	71.0	39348	PASS
443	442	15	24	19.1	7511	PASS