


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101116\
 Data File : BF090503.D
 Acq On : 11 Oct 2016 15:50
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 11 16:14:43 2016

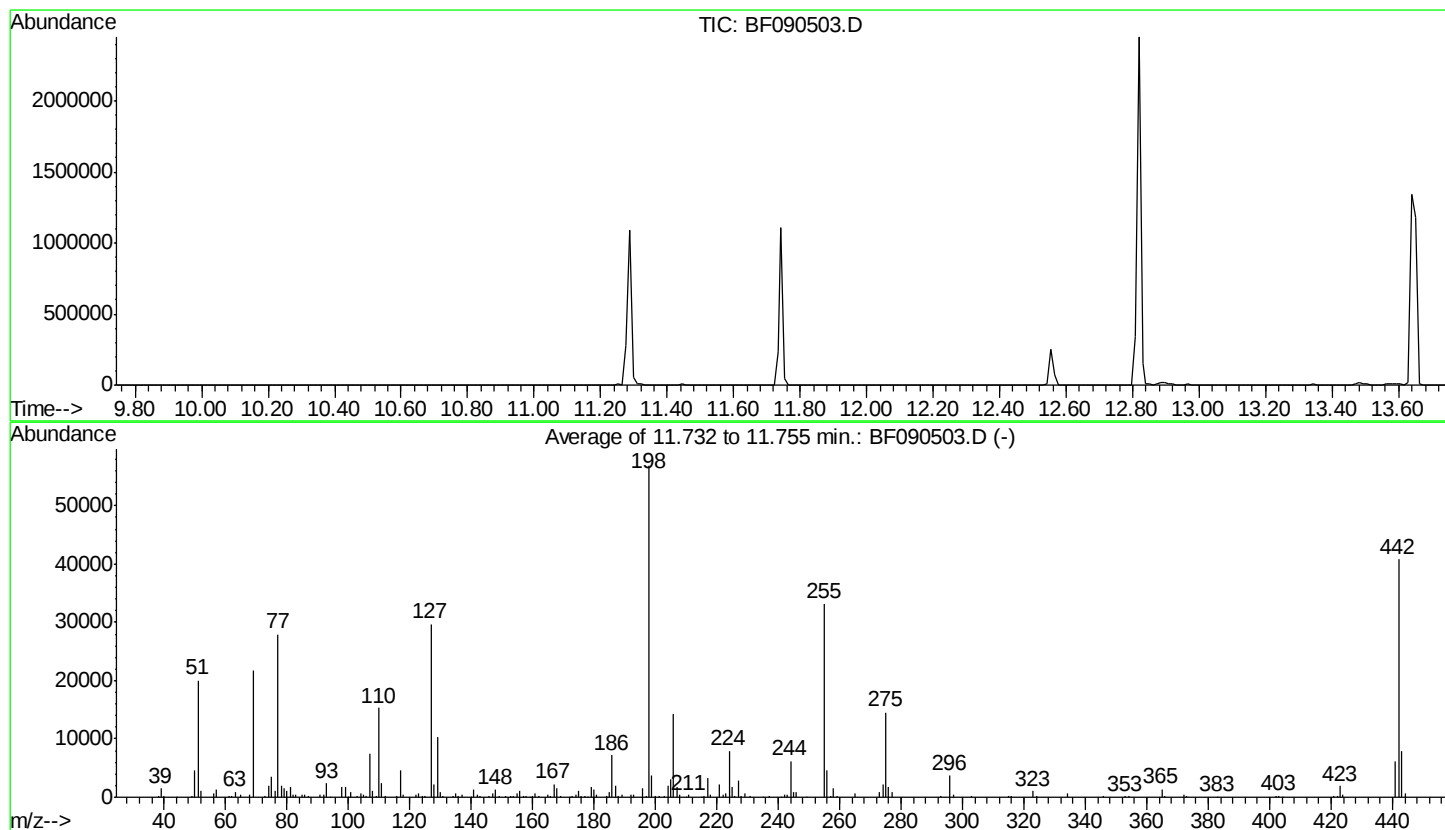

AutoFind: Scans 822, 823, 824; Background Corrected with Scan 819

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	20045	PASS
68	69	0.00	2	1.6	352	PASS
69	198	0.00	100	38.4	21840	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.2	29679	PASS
197	198	0.00	2	0.3	180	PASS
198	198	100	100	100.0	56886	PASS
199	198	5	9	6.7	3796	PASS
275	198	10	60	25.5	14497	PASS
365	198	1	100	2.4	1354	PASS
441	442	0.01	24	14.9	6081	PASS
442	198	50	100	71.7	40799	PASS
443	442	15	24	19.3	7884	PASS