
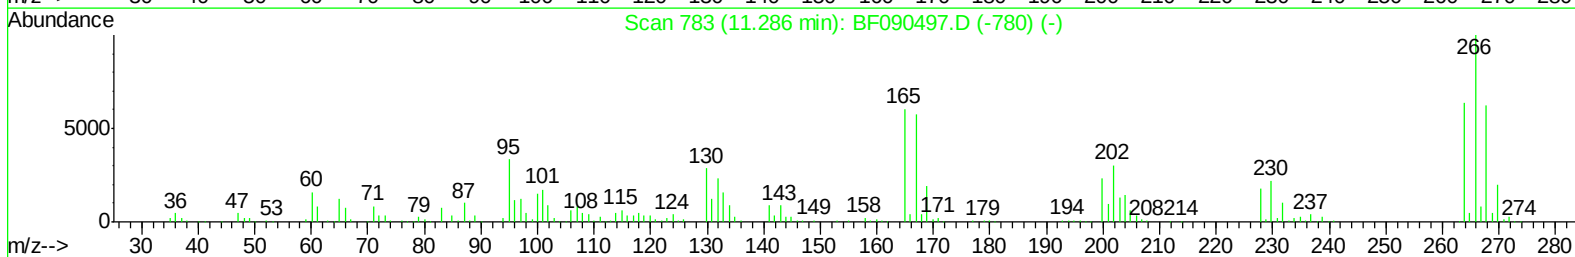
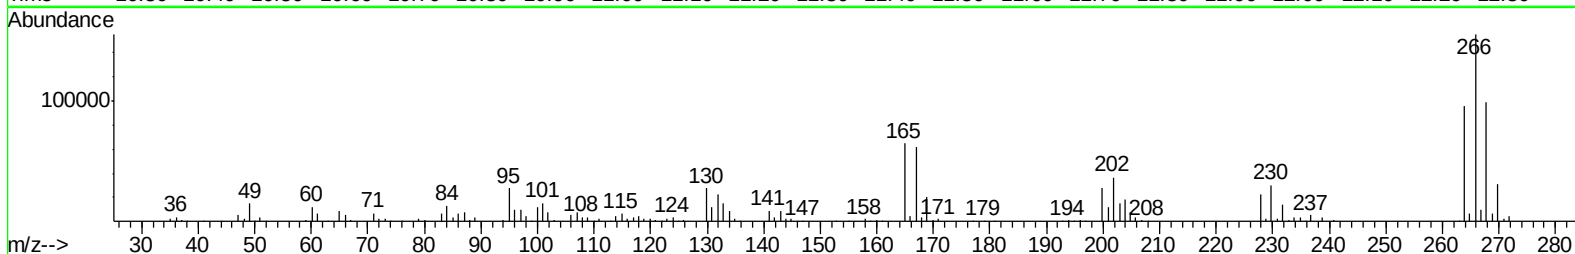


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101116\
Data File : BF090492.D
Acq On : 11 Oct 2016 9:58
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 07:41:13 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 16:14:43 2016
Response via : Initial Calibration

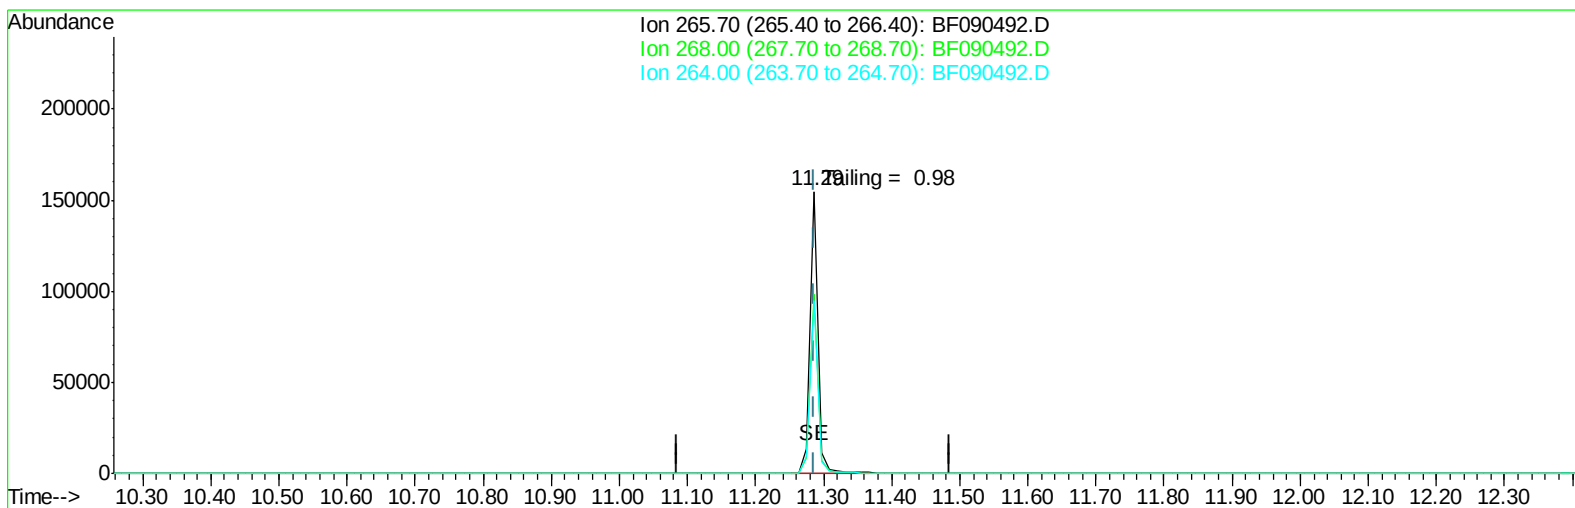

TIC: BF090492.D

(69) Pentachlorophenol (C)




11.286min (+0.000) 0.00ng

response 127069

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	63.58
264.00	64.40	61.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101116\
Data File : BF090492.D
Acq On : 11 Oct 2016 9:58
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 07:41:13 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 16:14:43 2016
Response via : Initial Calibration

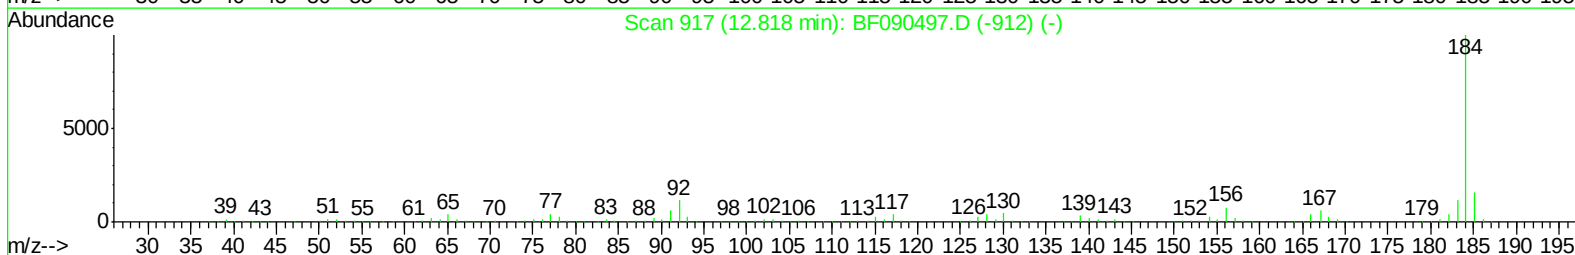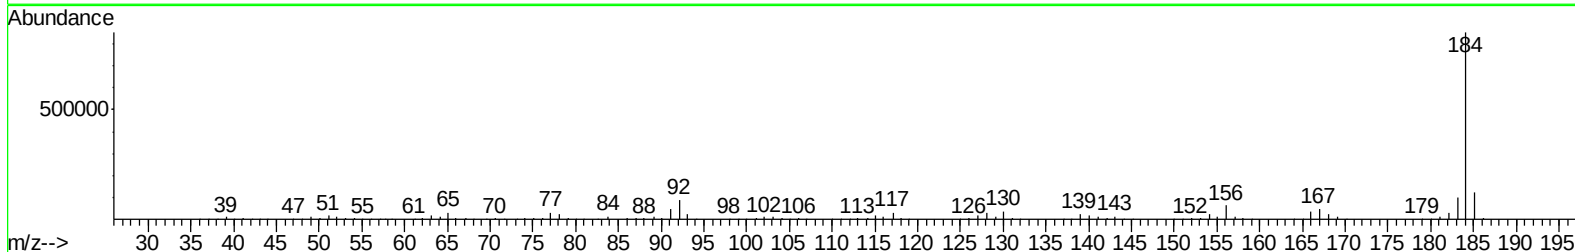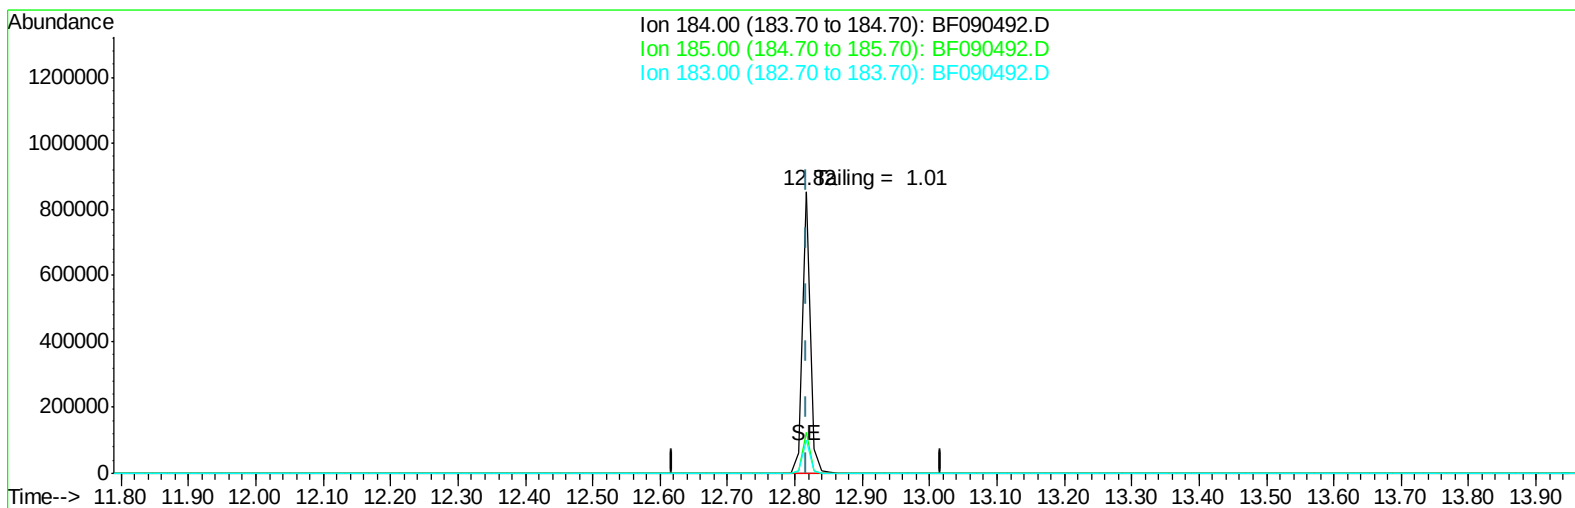

TIC: BF090492.D

(76) Benzidine

12.818min (+0.000) 75893.10ng

response 689336

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.77
183.00	12.00	11.94
0.00	0.00	0.00