
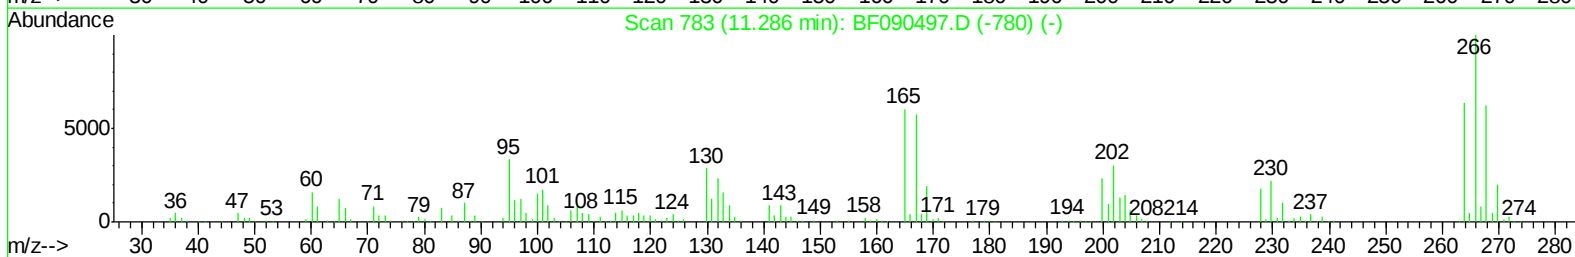
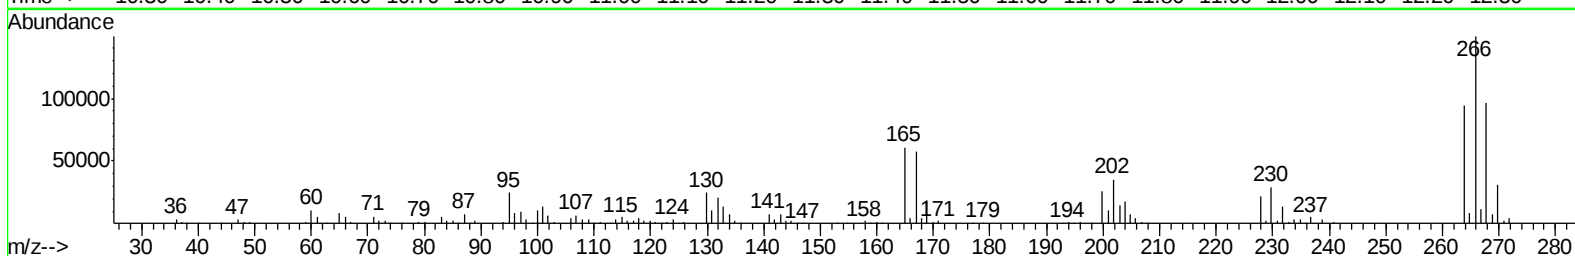


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101116\
Data File : BF090503.D
Acq On : 11 Oct 2016 15:50
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 08:49:01 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 16:14:43 2016
Response via : Initial Calibration

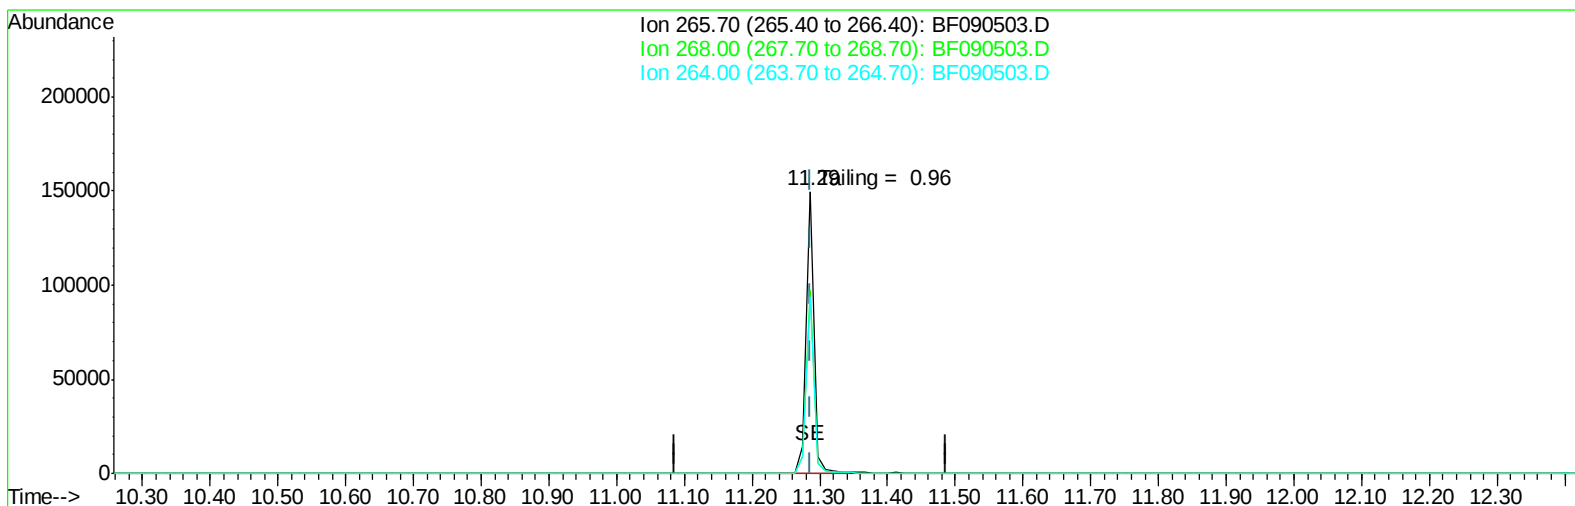

TIC: BF090503.D

(69) Pentachlorophenol (C)




11.286min (+0.000) 0.00ng

response 123456

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	64.82
264.00	64.40	62.79
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101116\
 Data File : BF090503.D
 Acq On : 11 Oct 2016 15:50
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 08:49:01 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 16:14:43 2016
 Response via : Initial Calibration

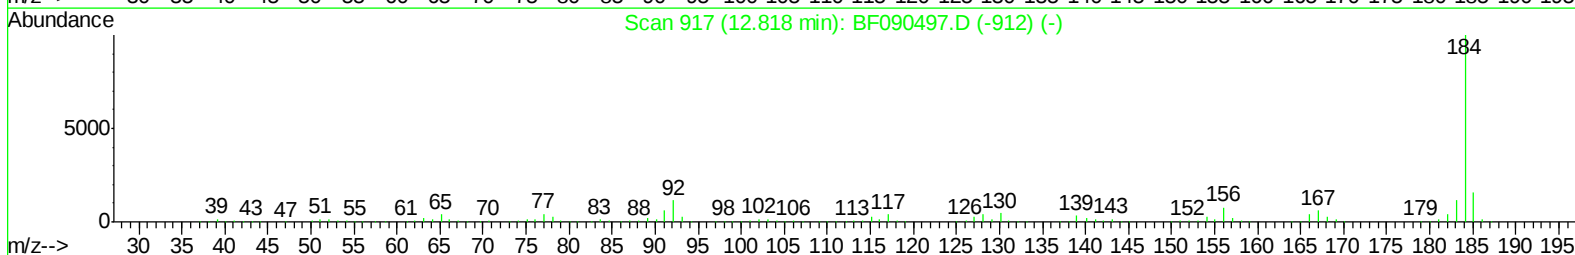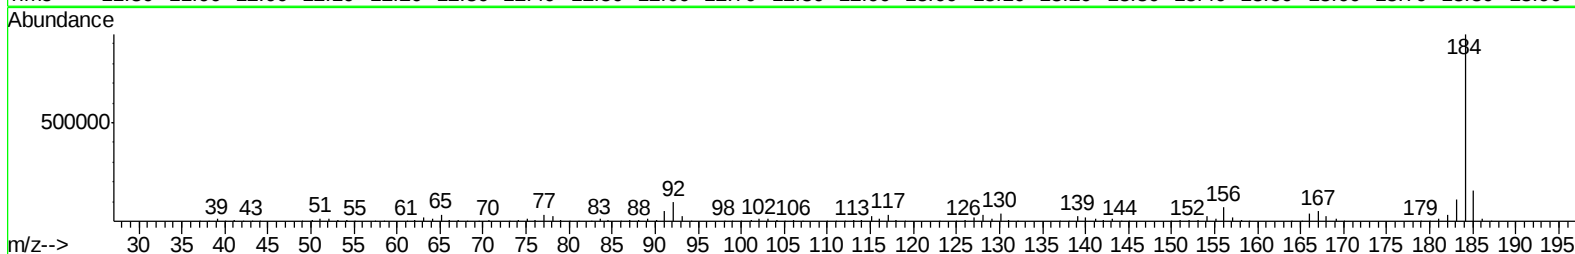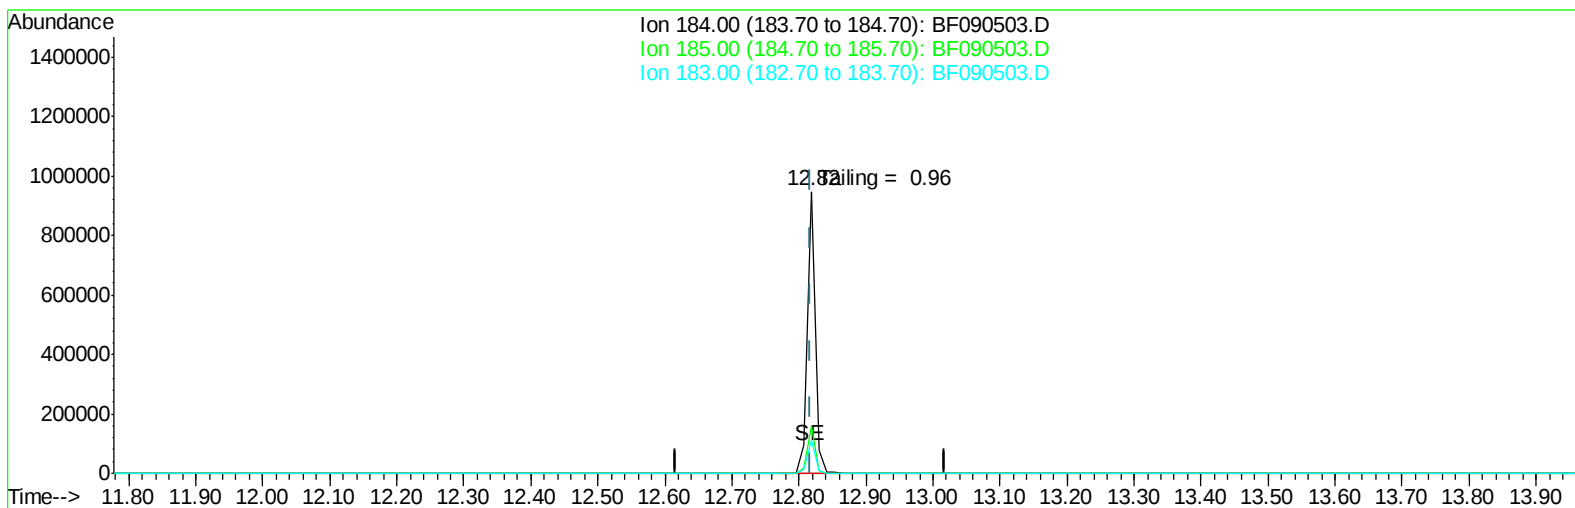

TIC: BF090503.D

(76) Benzidine

12.818min (+0.000) 0.00ng

response 781808

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	16.68
183.00	12.00	11.96
0.00	0.00	0.00