
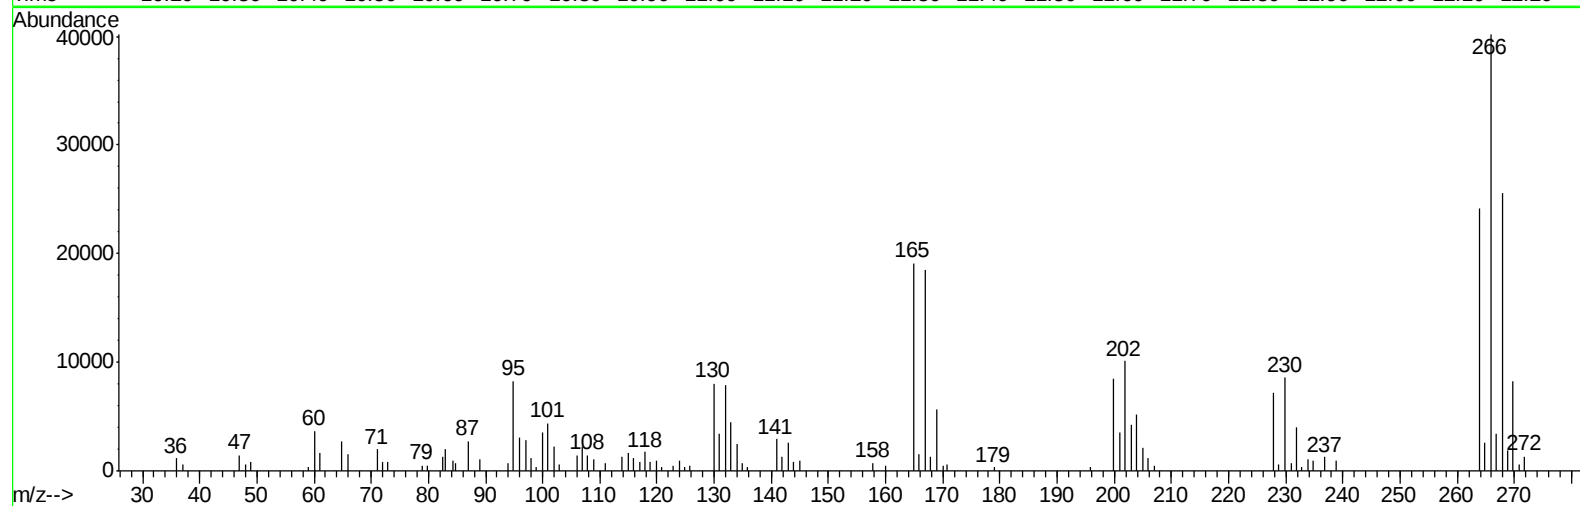


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101117\
Data File : BF099373.D
Acq On : 12 Oct 2017 5:11
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 07:31:47 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

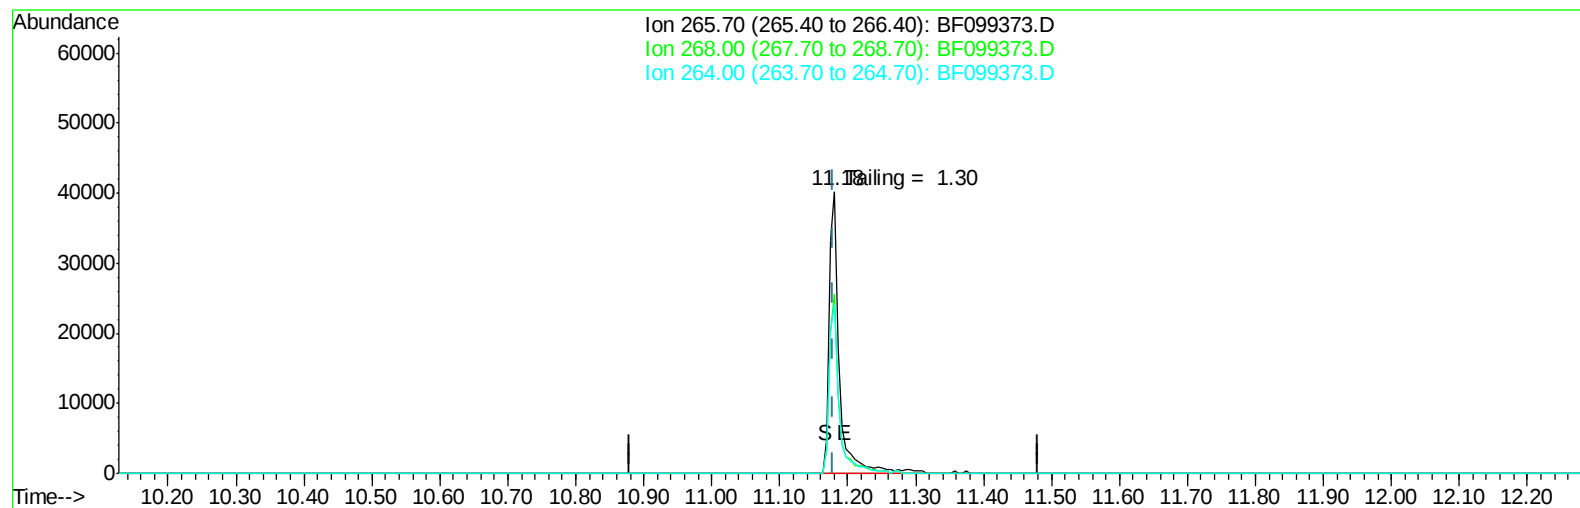

TIC: BF099373.D

(69) Pentachlorophenol (C)



11.180min (+0.000) 23442.94ng

response 42403

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.69
264.00	61.90	60.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101117\
Data File : BF099373.D
Acq On : 12 Oct 2017 5:11
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 07:31:47 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

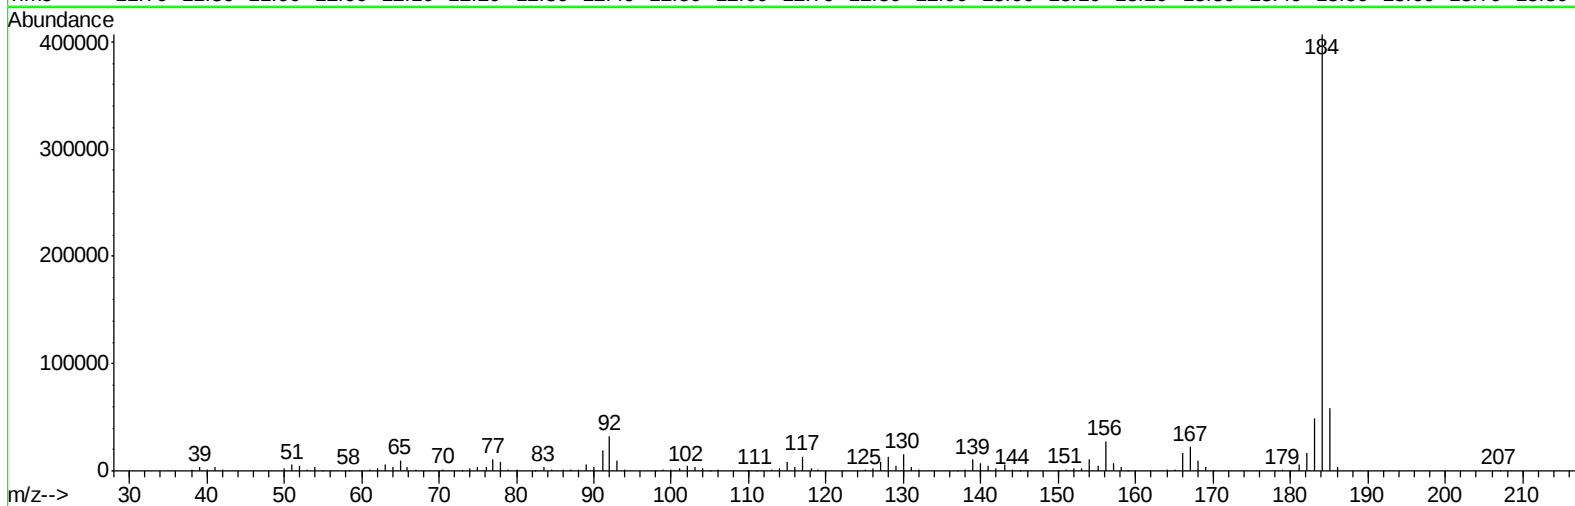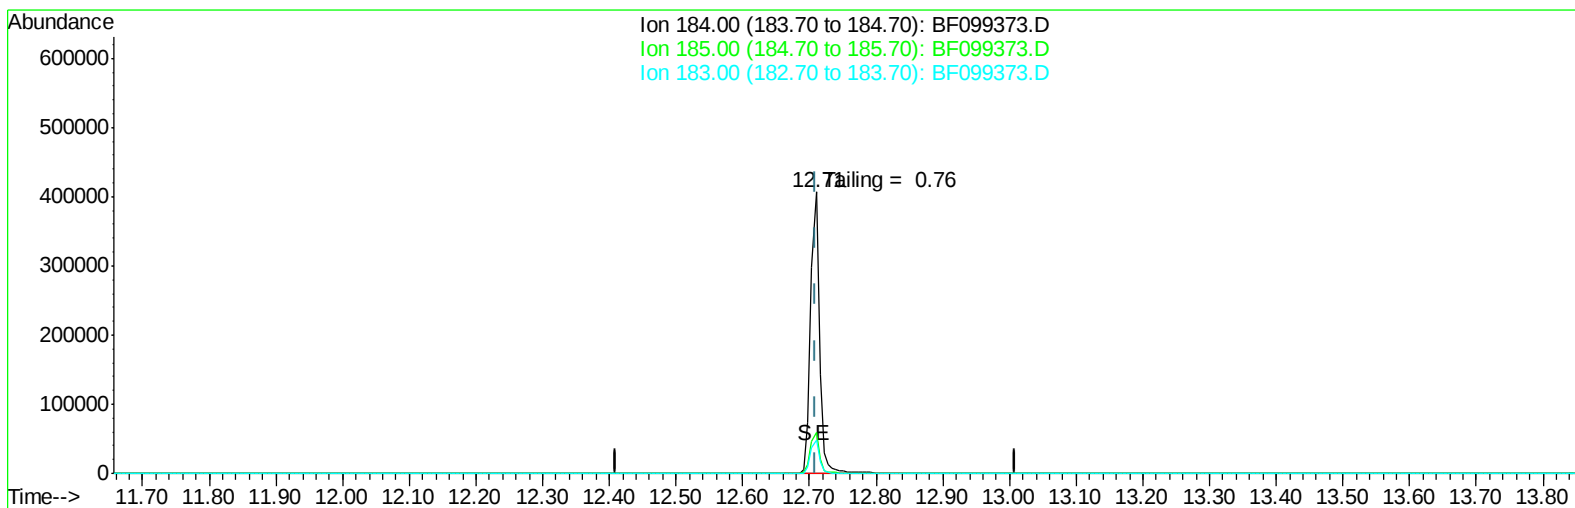

TIC: BF099373.D

(76) Benzidine

12.710min (+0.000) 0.00ng

response 355594

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.51
183.00	11.60	11.96
0.00	0.00	0.00