

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101117\
 Data File : BF099369.D
 Acq On : 12 Oct 2017 2:49
 Operator : SJ/JU
 Sample : I5710-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B-42A

Quant Time: Oct 12 04:10:15 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 11 16:25:21 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	112262	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	462304	20.00	ng	0.00
38) Acenaphthene-d10	9.89	164	207243	20.00	ng	0.00
63) Phenanthrene-d10	11.37	188	363851	20.00	ng	0.00
75) Chrysene-d12	14.01	240	196591	20.00	ng	0.00
86) Perylene-d12	15.48	264	174712	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	900855	127.74	ng	0.01
7) Phenol-d6	6.49	99	1077009	123.80	ng	0.00
23) Nitrobenzene-d5	7.42	82	653328	90.63	ng	0.00
41) 2,4,6-Tribromophenol	10.68	330	215679	127.18	ng	0.00
44) 2-Fluorobiphenyl	9.21	172	1047023	84.34	ng	0.00
78) Terphenyl-d14	12.96	244	808204	93.49	ng	0.00
Target Compounds						
10) Phenol	6.50	94	32533	3.344	ng	85
49) Dimethylphthalate	9.60	163	152403	9.743	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101117\
Data File : BF099369.D
Acq On : 12 Oct 2017 2:49
Operator : SJ/JU
Sample : I5710-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-42A

Quant Time: Oct 12 04:10:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

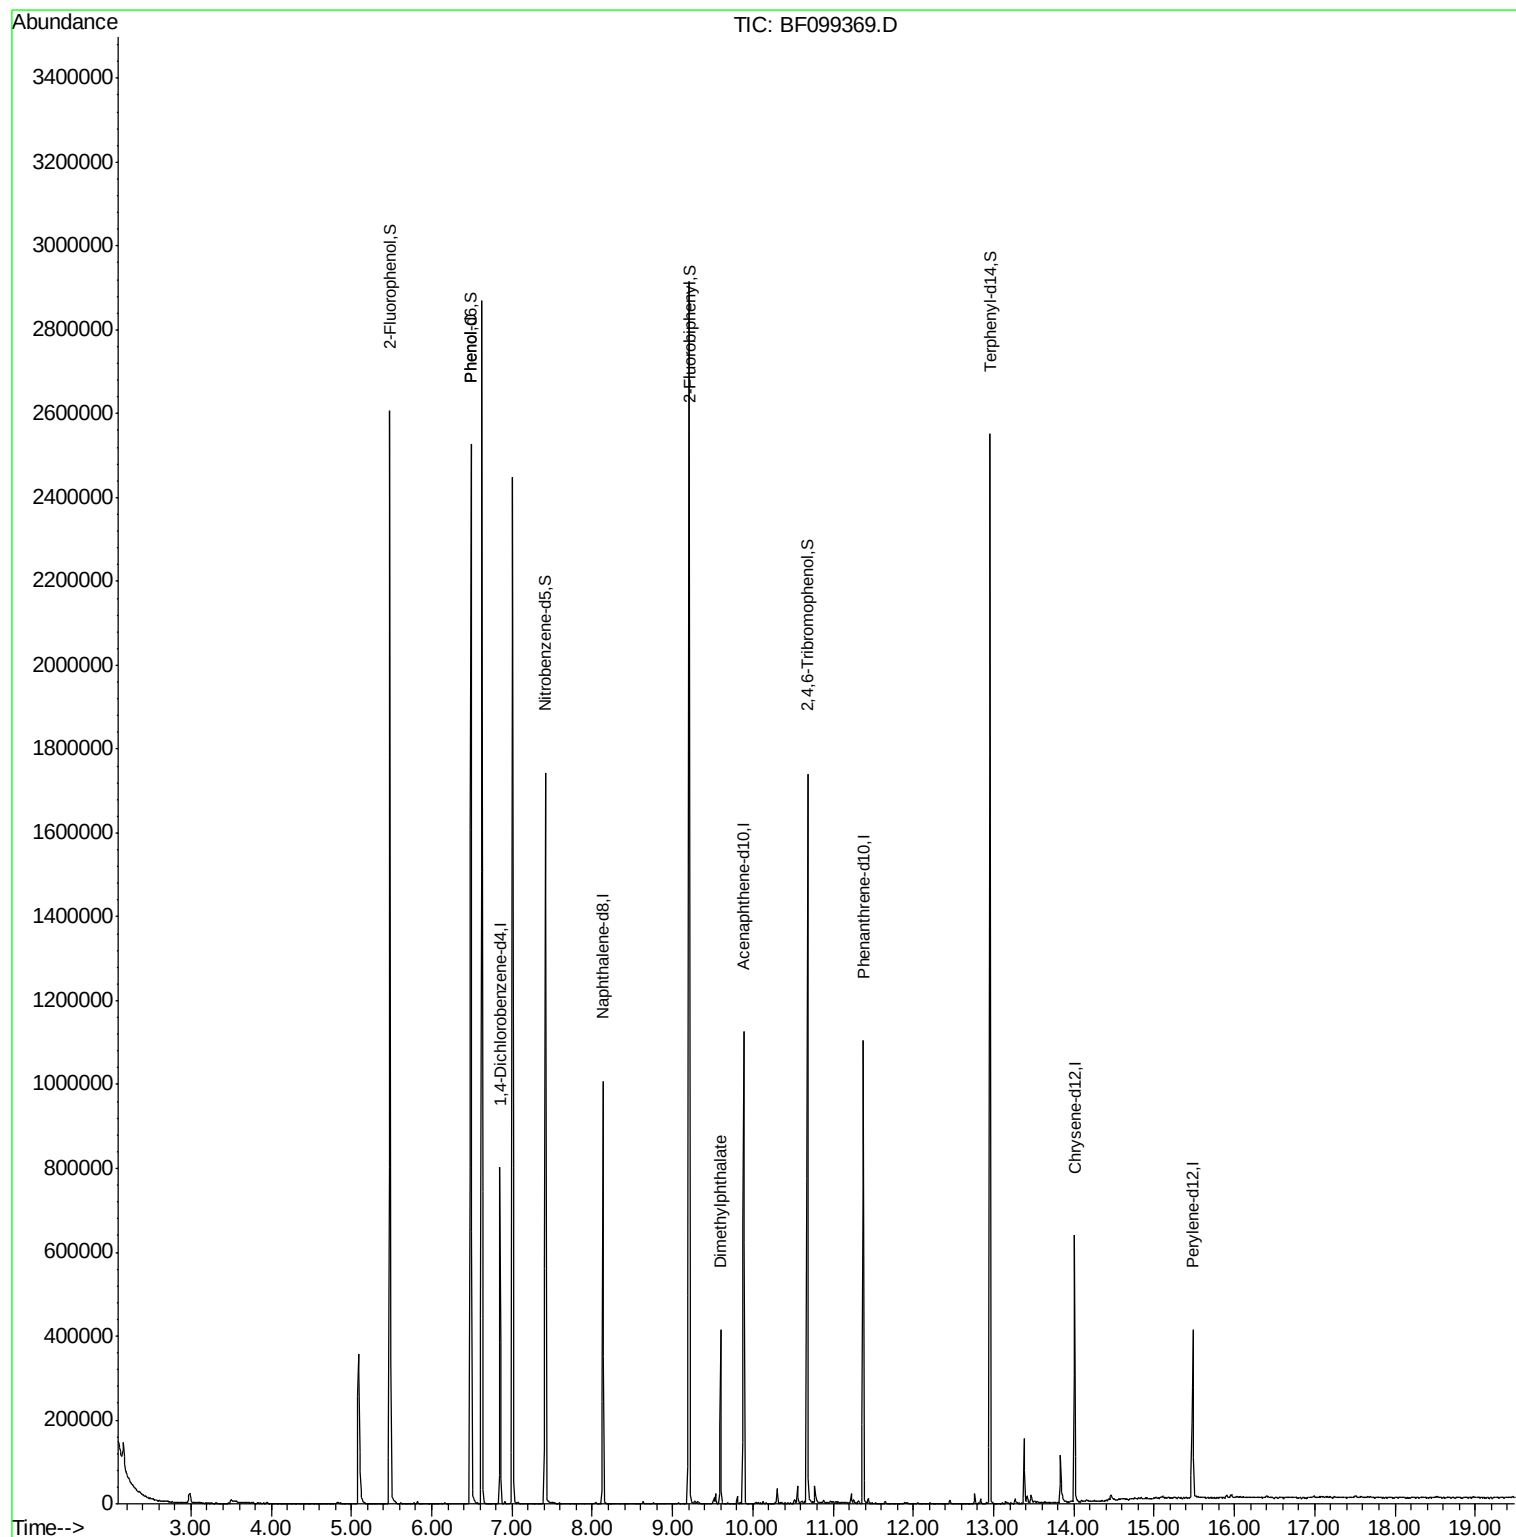

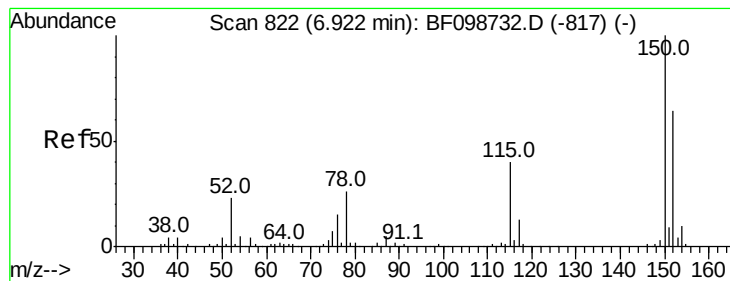


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.85 min Scan# 810
 Delta R.T. 0.00 min
 Lab File: BF099369.D
 Acq: 12 Oct 2017 2:49

Instrument :
 BNA_F
 ClientSampleId :
 B-42A

Tot Ion:152 Resp: 112262
 Ion Ratio Lower Upper
 152 100
 150 159.0 124.6 186.8
 115 59.4 50.1 75.1

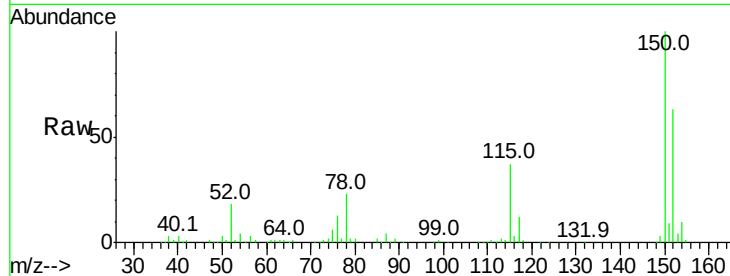


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

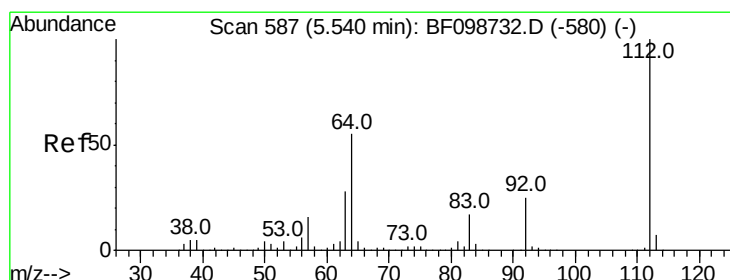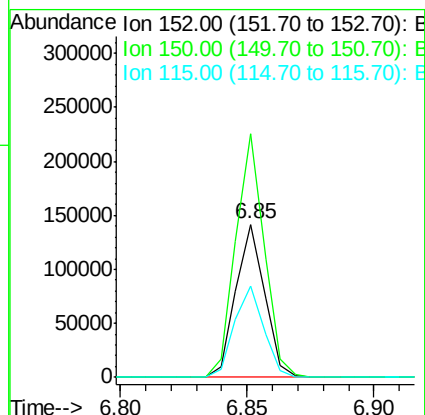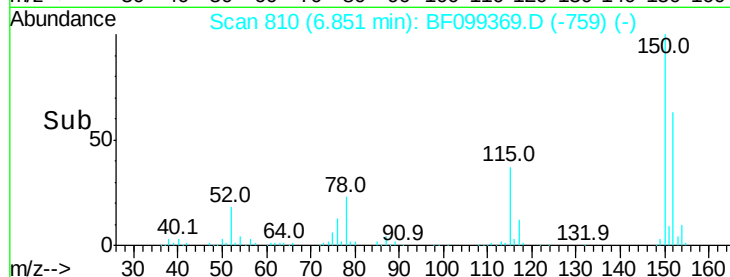



#5


2-Fluorophenol
 Concen: 127.743 ng
 RT: 5.48 min Scan# 577
 Delta R.T. 0.01 min
 Lab File: BF099369.D
 Acq: 12 Oct 2017 2:49

Tgt Ion:112 Resp: 900855
 Ion Ratio Lower Upper
 112 100
 64 55.8 47.9 71.9
 63 27.1 23.7 35.5

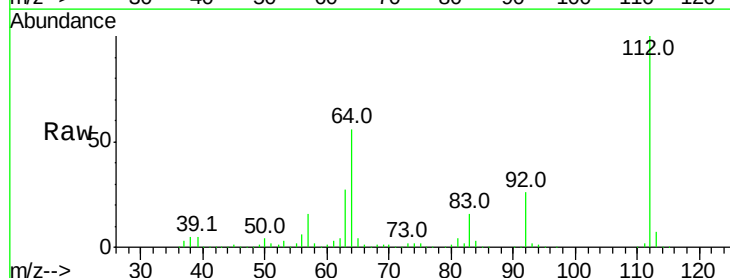

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

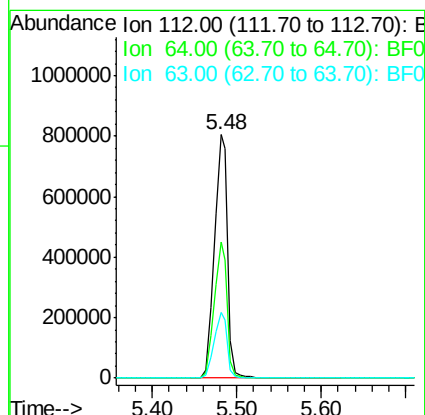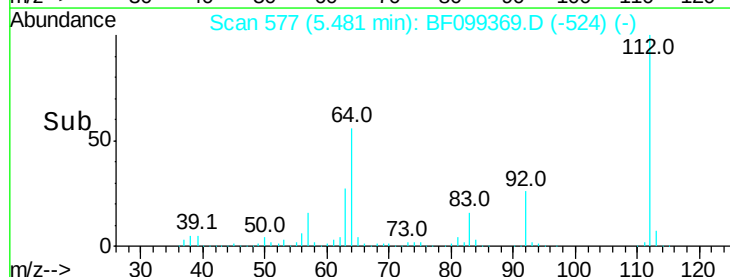

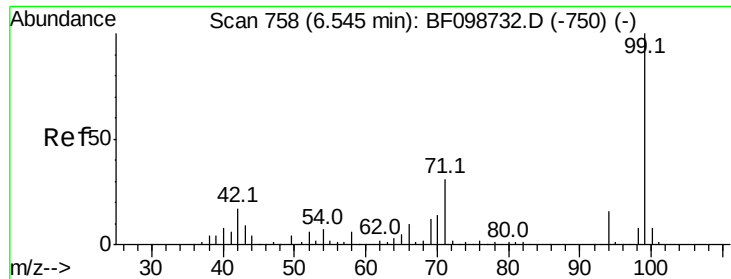

#7

Phenol-d6

Concen: 123.801 ng

RT: 6.49 min Scan# 749

Delta R.T. 0.01 min

Lab File: BF099369.D

Acq: 12 Oct 2017 2:49

Instrument :

BNA_F

ClientSampleId :

B-42A


Tot Ion: 99 Resp: 1077009

Ion Ratio Lower Upper




99 100

42 14.9 14.5 21.7

71 30.3 25.4 38.0

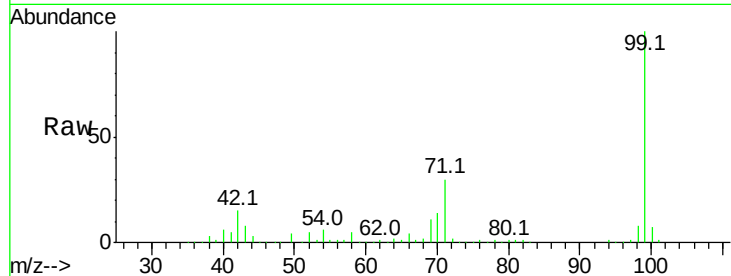

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

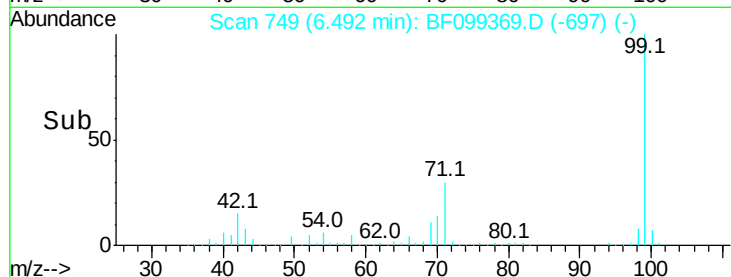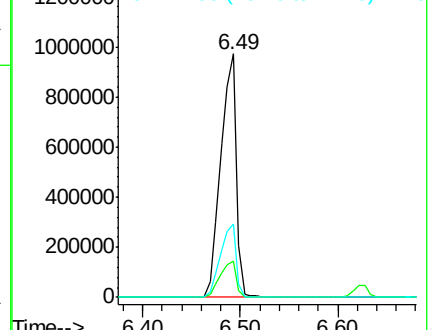

#10

Phenol

Concen: 3.344 ng

RT: 6.50 min Scan# 750

Delta R.T. 0.00 min

Lab File: BF099369.D

Acq: 12 Oct 2017 2:49


Tgt Ion: 94 Resp: 32533

Ion Ratio Lower Upper



94 100


65 29.6 7.9 47.9

66 50.7 16.2 56.2



Abundance Ion 94.00 (93.70 to 94.70): BF0
Ion 65.00 (64.70 to 65.70): BF0
Ion 66.00 (65.70 to 66.70): BF0



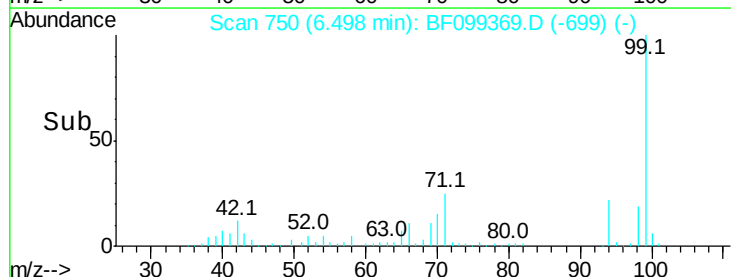
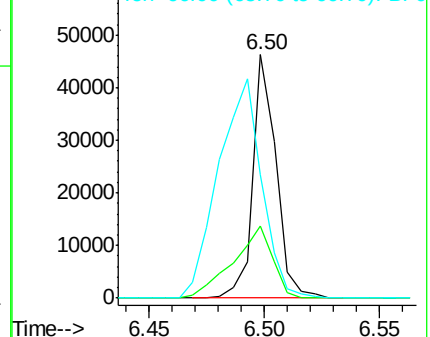


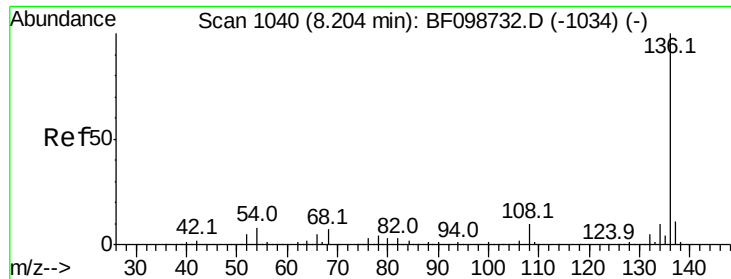

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.13 min Scan# 1028
Delta R.T. 0.00 min
Lab File: BF099369.D
Acq: 12 Oct 2017 2:49




Instrument :
BNA_F
ClientSampleId :
B-42A


Tot Ion:	136	Resp:	462304
Ion	Ratio	Lower	Upper
136	100		
137	10.5	8.9	13.3
54	7.0	6.6	9.8
68	5.4	5.0	7.4

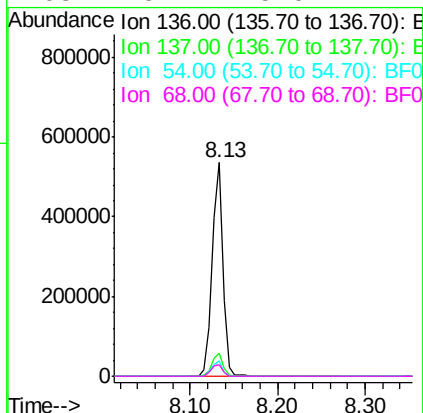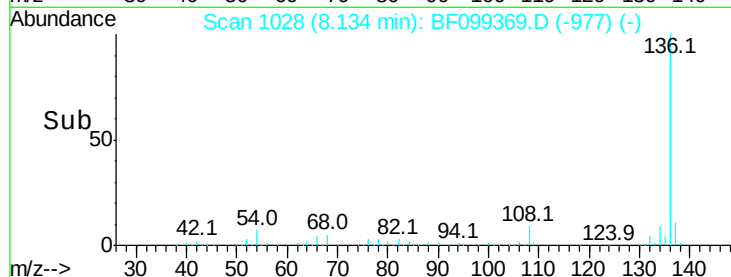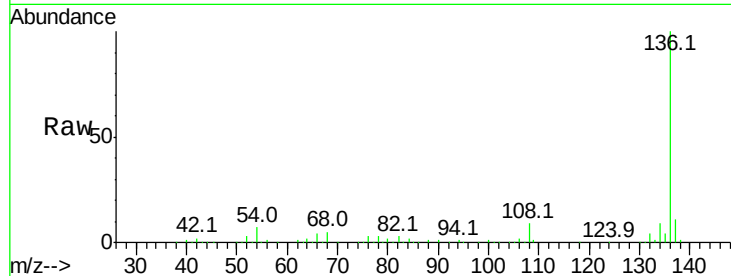

#23
Nitrobenzene-d5
Concen: 90.629 ng
RT: 7.42 min Scan# 906
Delta R.T. -0.01 min
Lab File: BF099369.D
Acq: 12 Oct 2017 2:49

Tgt Ion:	82	Resp:	653328
Ion	Ratio	Lower	Upper
82	100		
128	47.4	36.1	54.1
54	48.5	41.4	62.2

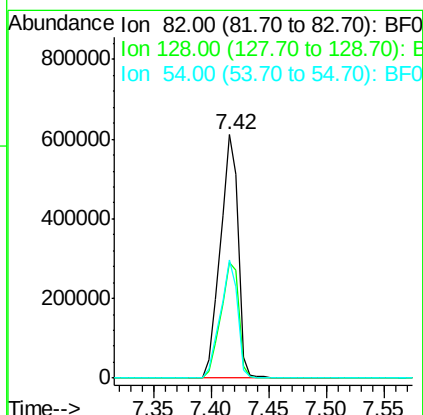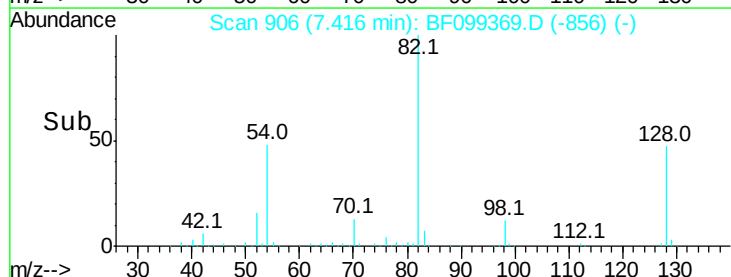

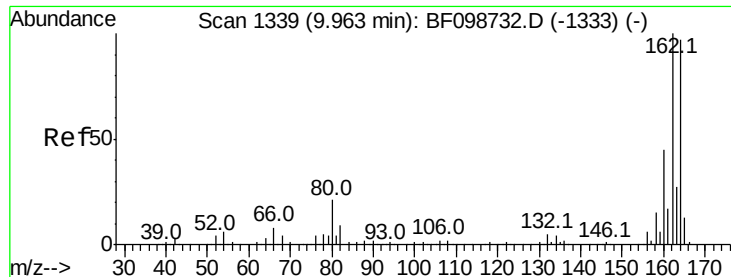

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.89 min Scan# 1326

Delta R.T. -0.01 min

Lab File: BF099369.D

Acq: 12 Oct 2017 2:49

Instrument :

BNA_F

ClientSampleId :

B-42A


Tot Ion:164 Resp: 207243

Ion Ratio Lower Upper

164 100

162 105.3 86.1 129.1




160 46.3 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

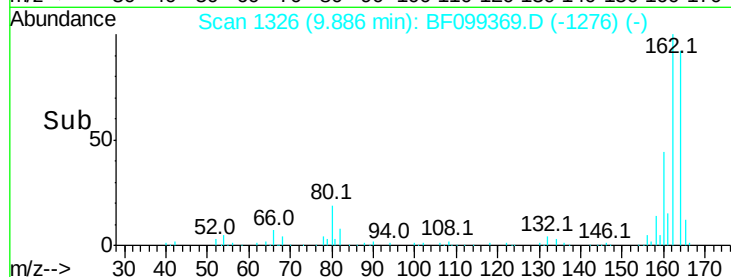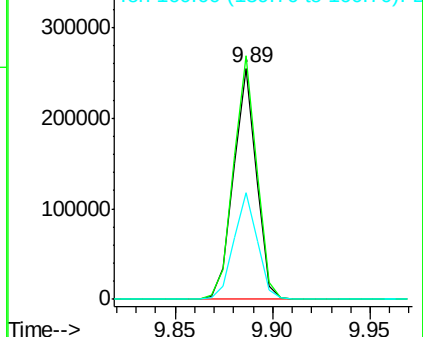

#41

2,4,6-Tribromophenol

Concen: 127.183 ng

RT: 10.68 min Scan# 1461

Delta R.T. 0.00 min

Lab File: BF099369.D

Acq: 12 Oct 2017 2:49


Tgt Ion:330 Resp: 215679

Ion Ratio Lower Upper

330 100

332 97.8 77.0 115.6



141 38.1 29.9 44.9




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

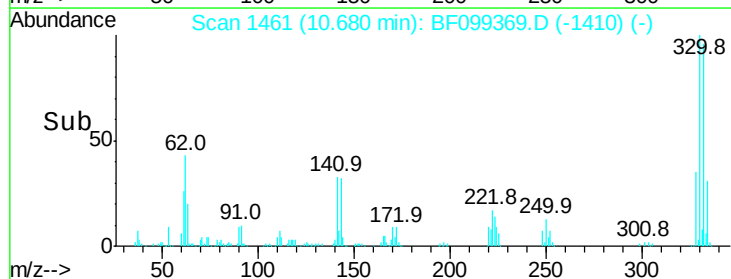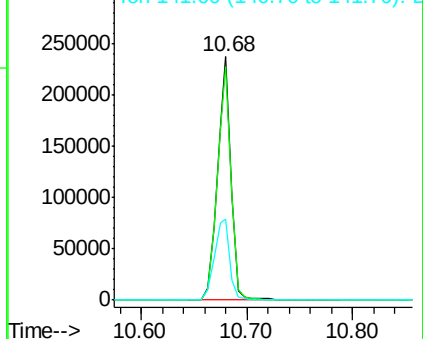

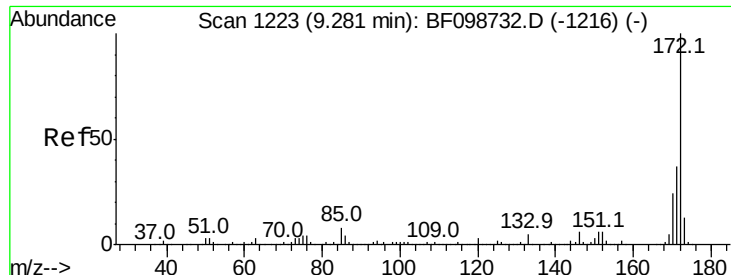


#44
 2-Fluorobiphenyl
 Concen: 84.341 ng
 RT: 9.21 min Scan# 1211
 Delta R.T. 0.00 min
 Lab File: BF099369.D
 Acq: 12 Oct 2017 2:49




Instrument :
 BNA_F
 ClientSampleId :
 B-42A

Tot Ion:172 Resp: 1047023

Ion	Ratio	Lower	Upper
172	100		
171	36.1	29.7	44.5
170	23.6	19.6	29.4

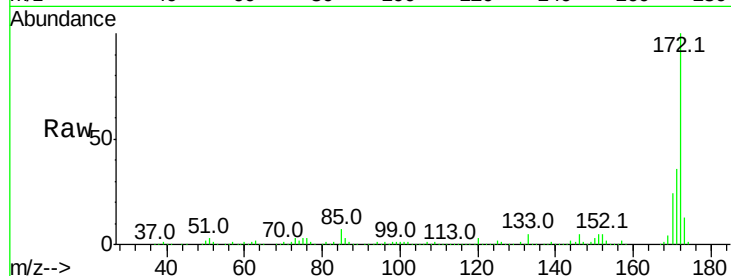


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

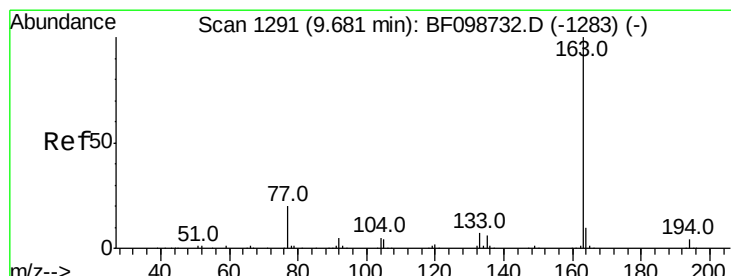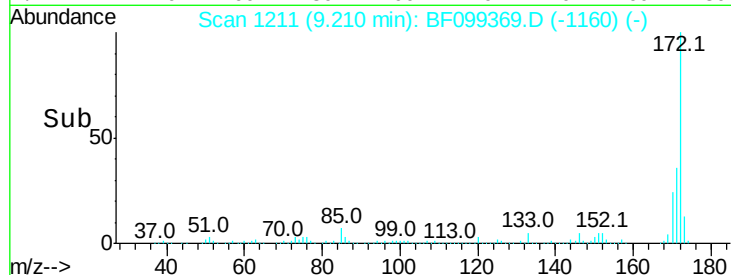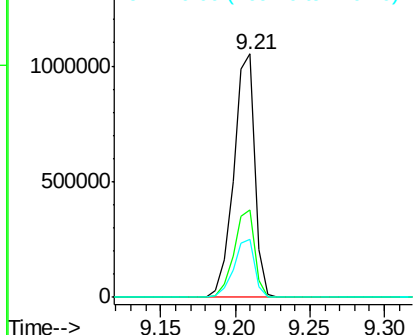



#49
 Dimethylphthalate
 Concen: 9.743 ng
 RT: 9.60 min Scan# 1277
 Delta R.T. -0.01 min
 Lab File: BF099369.D
 Acq: 12 Oct 2017 2:49


Tgt Ion:163 Resp: 152403

Ion	Ratio	Lower	Upper
163	100		
194	3.0	2.7	4.1
164	9.6	8.2	12.2

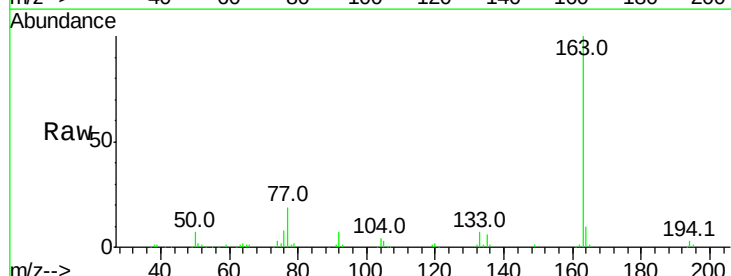

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E



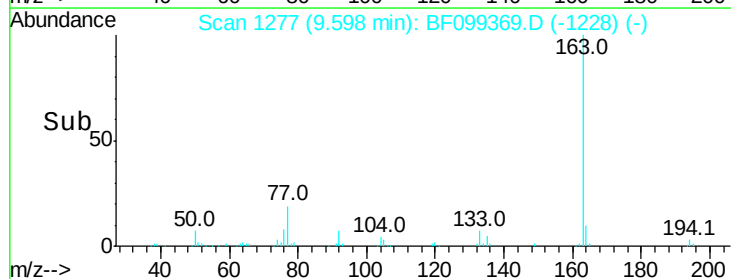
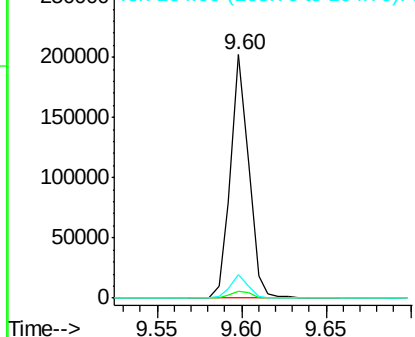


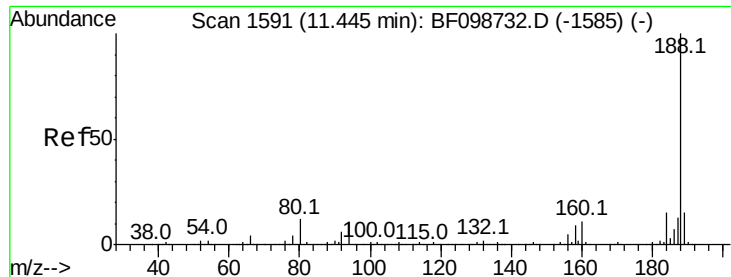

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.37 min Scan# 1579
Delta R.T. 0.00 min
Lab File: BF099369.D
Acq: 12 Oct 2017 2:49




Instrument :
BNA_F
ClientSampled :
B-42A


Tot Ion:188 Resp: 363851
Ion Ratio Lower Upper
188 100
94 10.2 8.5 12.7
80 10.8 9.2 13.8

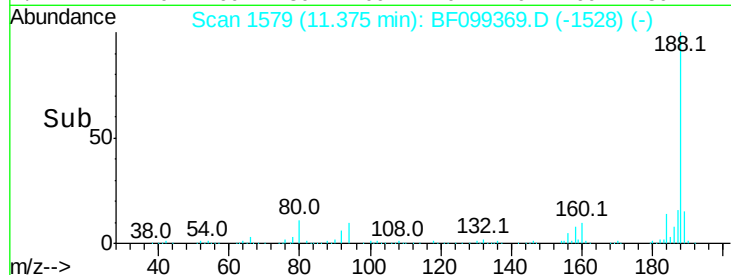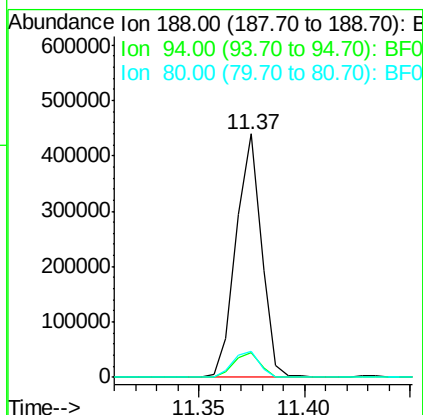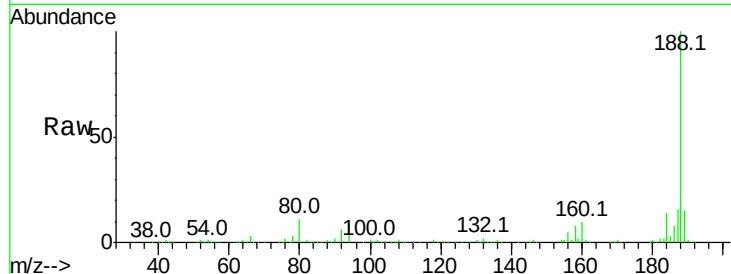

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.01 min Scan# 2027
Delta R.T. -0.01 min
Lab File: BF099369.D
Acq: 12 Oct 2017 2:49

Tgt Ion:240 Resp: 196591
Ion Ratio Lower Upper
240 100
120 14.8 9.5 14.3#
236 25.9 20.7 31.1

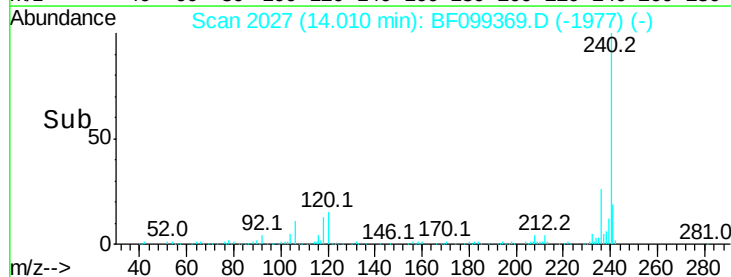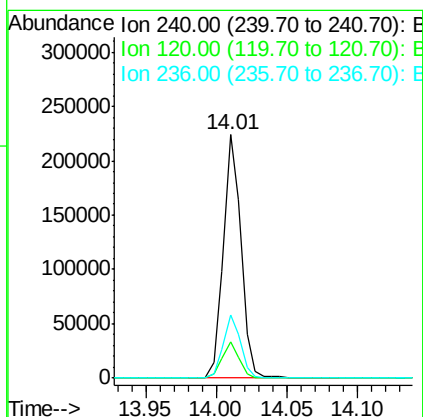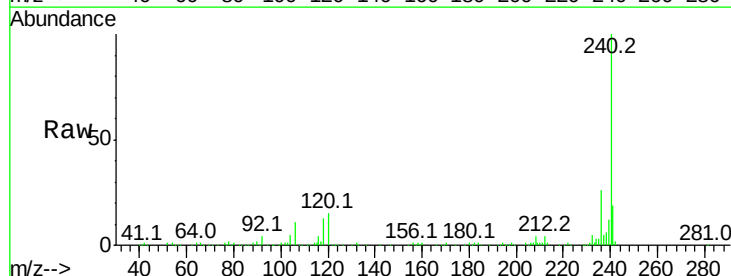

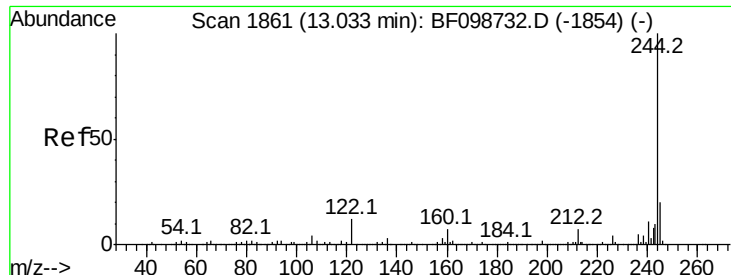

#78

Terphenyl-d14

Concen: 93.495 ng

RT: 12.96 min Scan# 1848

Delta R.T. 0.00 min

Lab File: BF099369.D

Acq: 12 Oct 2017 2:49

Instrument :

BNA_F

ClientSampleId :

B-42A


Tot Ion:244 Resp: 808204

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.0




122 13.9 11.0 16.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

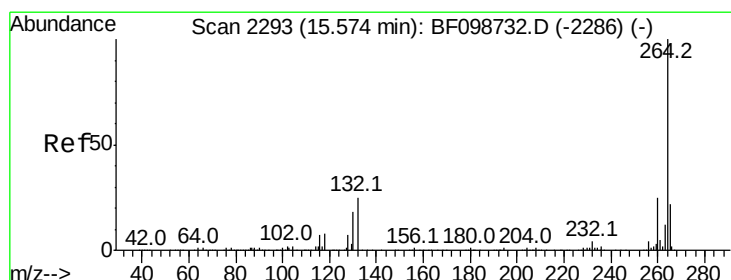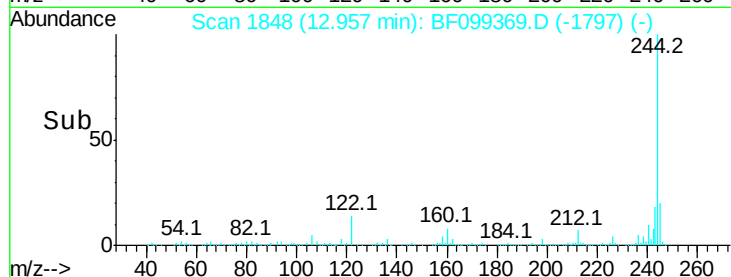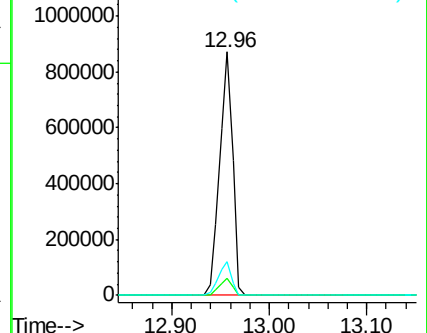

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.48 min Scan# 2277

Delta R.T. 0.00 min

Lab File: BF099369.D

Acq: 12 Oct 2017 2:49


Tgt Ion:264 Resp: 174712

Ion Ratio Lower Upper

264 100

260 23.6 19.2 28.8

265 20.7 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

