


Data Path : Z:\HPCHEM1\BNA F\Data\BF101117\
 Data File : BF099337.D
 Acq On : 11 Oct 2017 10:58
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 11 16:25:21 2017

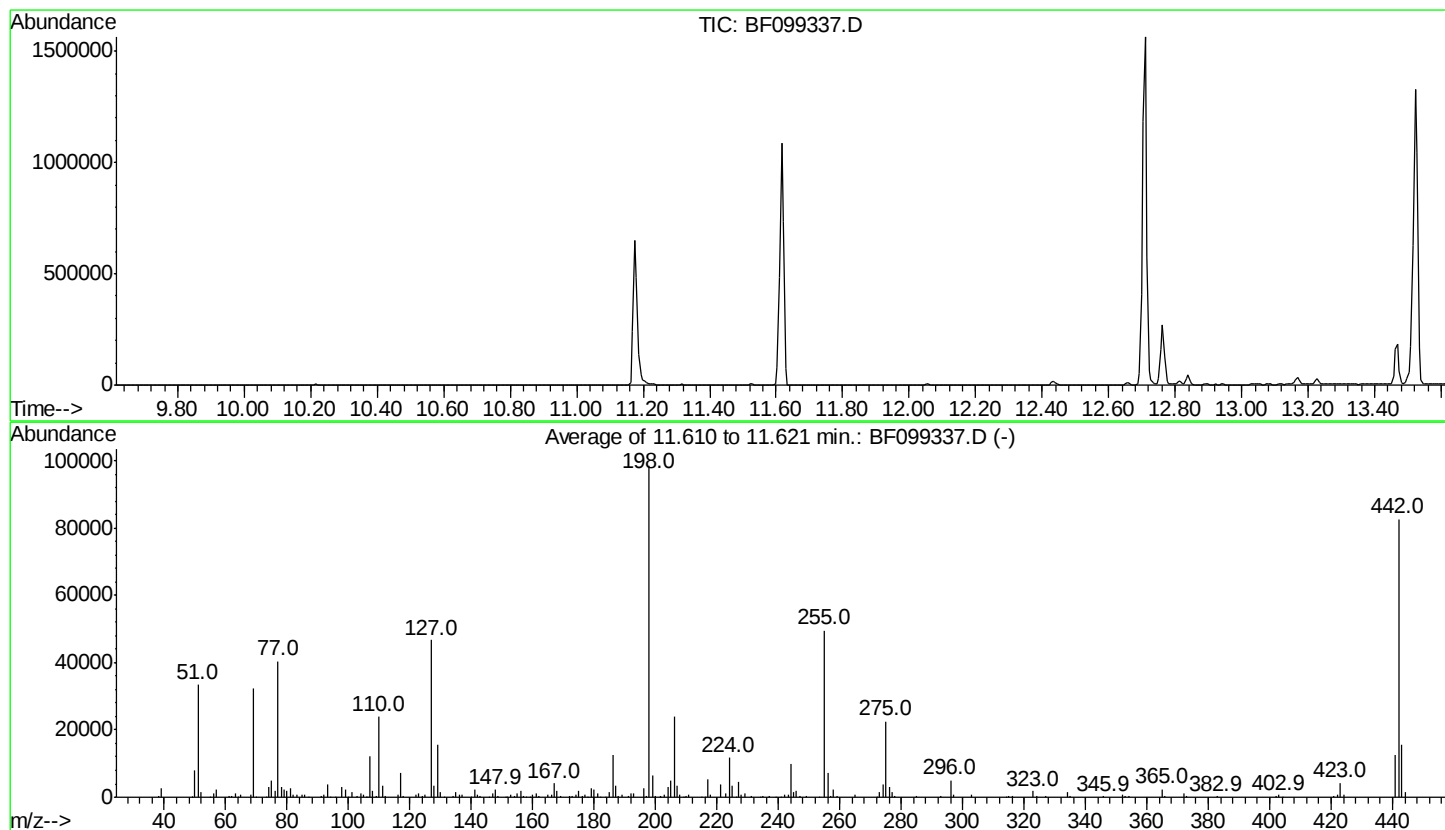

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	33357	PASS
68	69	0.00	2	2.0	636	PASS
69	198	0.00	100	32.8	32330	PASS
70	69	0.00	2	0.3	104	PASS
127	198	10	80	47.3	46661	PASS
197	198	0.00	2	0.3	273	PASS
198	198	100	100	100.0	98557	PASS
199	198	5	9	6.5	6435	PASS
275	198	10	60	23.0	22625	PASS
365	198	1	100	2.4	2329	PASS
441	442	0.01	24	15.4	12701	PASS
442	198	50	100	83.9	82680	PASS
443	442	15	24	18.9	15596	PASS