


Data Path : Z:\HPCHEM1\BNA F\Data\BF101117\
 Data File : BF099373.D
 Acq On : 12 Oct 2017 5:11
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 11 16:25:21 2017

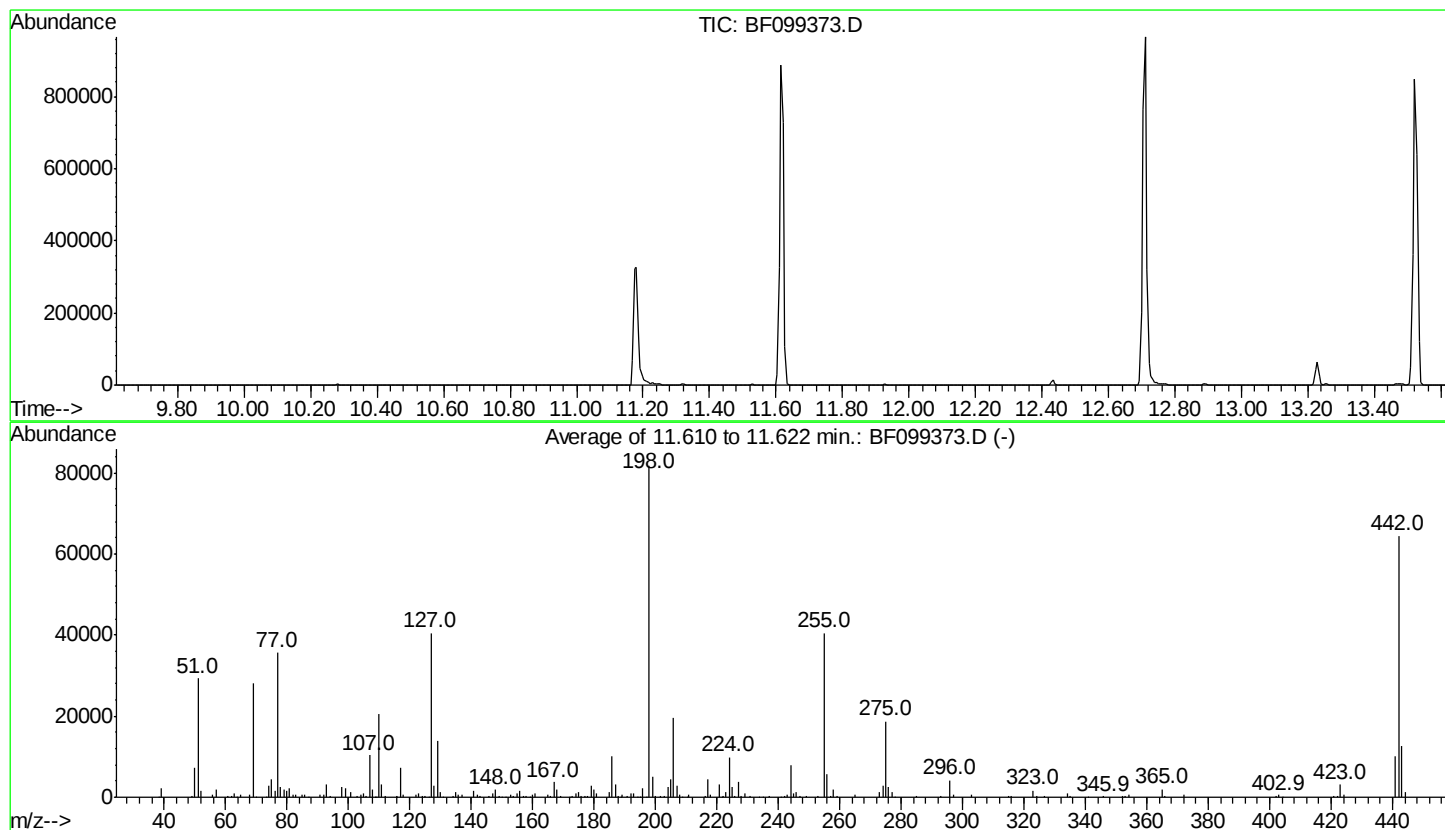

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	29341	PASS
68	69	0.00	2	2.0	572	PASS
69	198	0.00	100	34.2	28026	PASS
70	69	0.00	2	0.4	103	PASS
127	198	10	80	49.5	40530	PASS
197	198	0.00	2	0.2	150	PASS
198	198	100	100	100.0	81845	PASS
199	198	5	9	6.2	5068	PASS
275	198	10	60	22.9	18717	PASS
365	198	1	100	2.5	2007	PASS
441	442	0.01	24	15.6	10069	PASS
442	198	50	100	78.8	64483	PASS
443	442	15	24	19.7	12675	PASS