

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101118\
 Data File : BF109798.D
 Acq On : 11 Oct 2018 20:34
 Operator : JU/SJ
 Sample : J5296-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 100418-JETT-E-D-S

Quant Time: Oct 12 04:26:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 08 16:02:11 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.69	152	78558	20.00	ng	0.00
21) Naphthalene-d8	7.97	136	323251	20.00	ng	0.00
38) Acenaphthene-d10	9.72	164	144034	20.00	ng	0.00
63) Phenanthrene-d10	11.20	188	233272	20.00	ng	0.00
75) Chrysene-d12	13.83	240	203008	20.00	ng	0.00
86) Perylene-d12	15.23	264	232302	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.31	112	172624	39.00	ng	-0.01
7) Phenol-d6	6.34	99	156849	26.53	ng	-0.02
23) Nitrobenzene-d5	7.26	82	568476	96.94	ng	-0.01
41) 2,4,6-Tribromophenol	10.51	330	117141	74.64	ng	0.00
44) 2-Fluorobiphenyl	9.05	172	993535	95.00	ng	0.00
78) Terphenyl-d14	12.78	244	739302	70.50	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	6.46	77	8259	2.171	ng	# 78
19) n-Nitroso-di-n-propylamine	7.26	70	72918	17.587	ng	# 78
25) Isophorone	7.26	82	568476	58.379	ng	# 67
49) Dimethylphthalate	9.45	163	27098	2.565	ng	# 97
50) 2,6-Dinitrotoluene	9.72	165	17757	7.755	ng	# 21
56) 2,4-Dinitrotoluene	9.72	165	17757	6.214	ng	# 17
66) 4-Bromophenyl-phenylether	10.51	248	6767	2.525	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101118\
Data File : BF109798.D
Acq On : 11 Oct 2018 20:34
Operator : JU/SJ
Sample : J5296-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
100418-JETT-E-D-S

Quant Time: Oct 12 04:26:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 08 16:02:11 2018
Response via : Initial Calibration

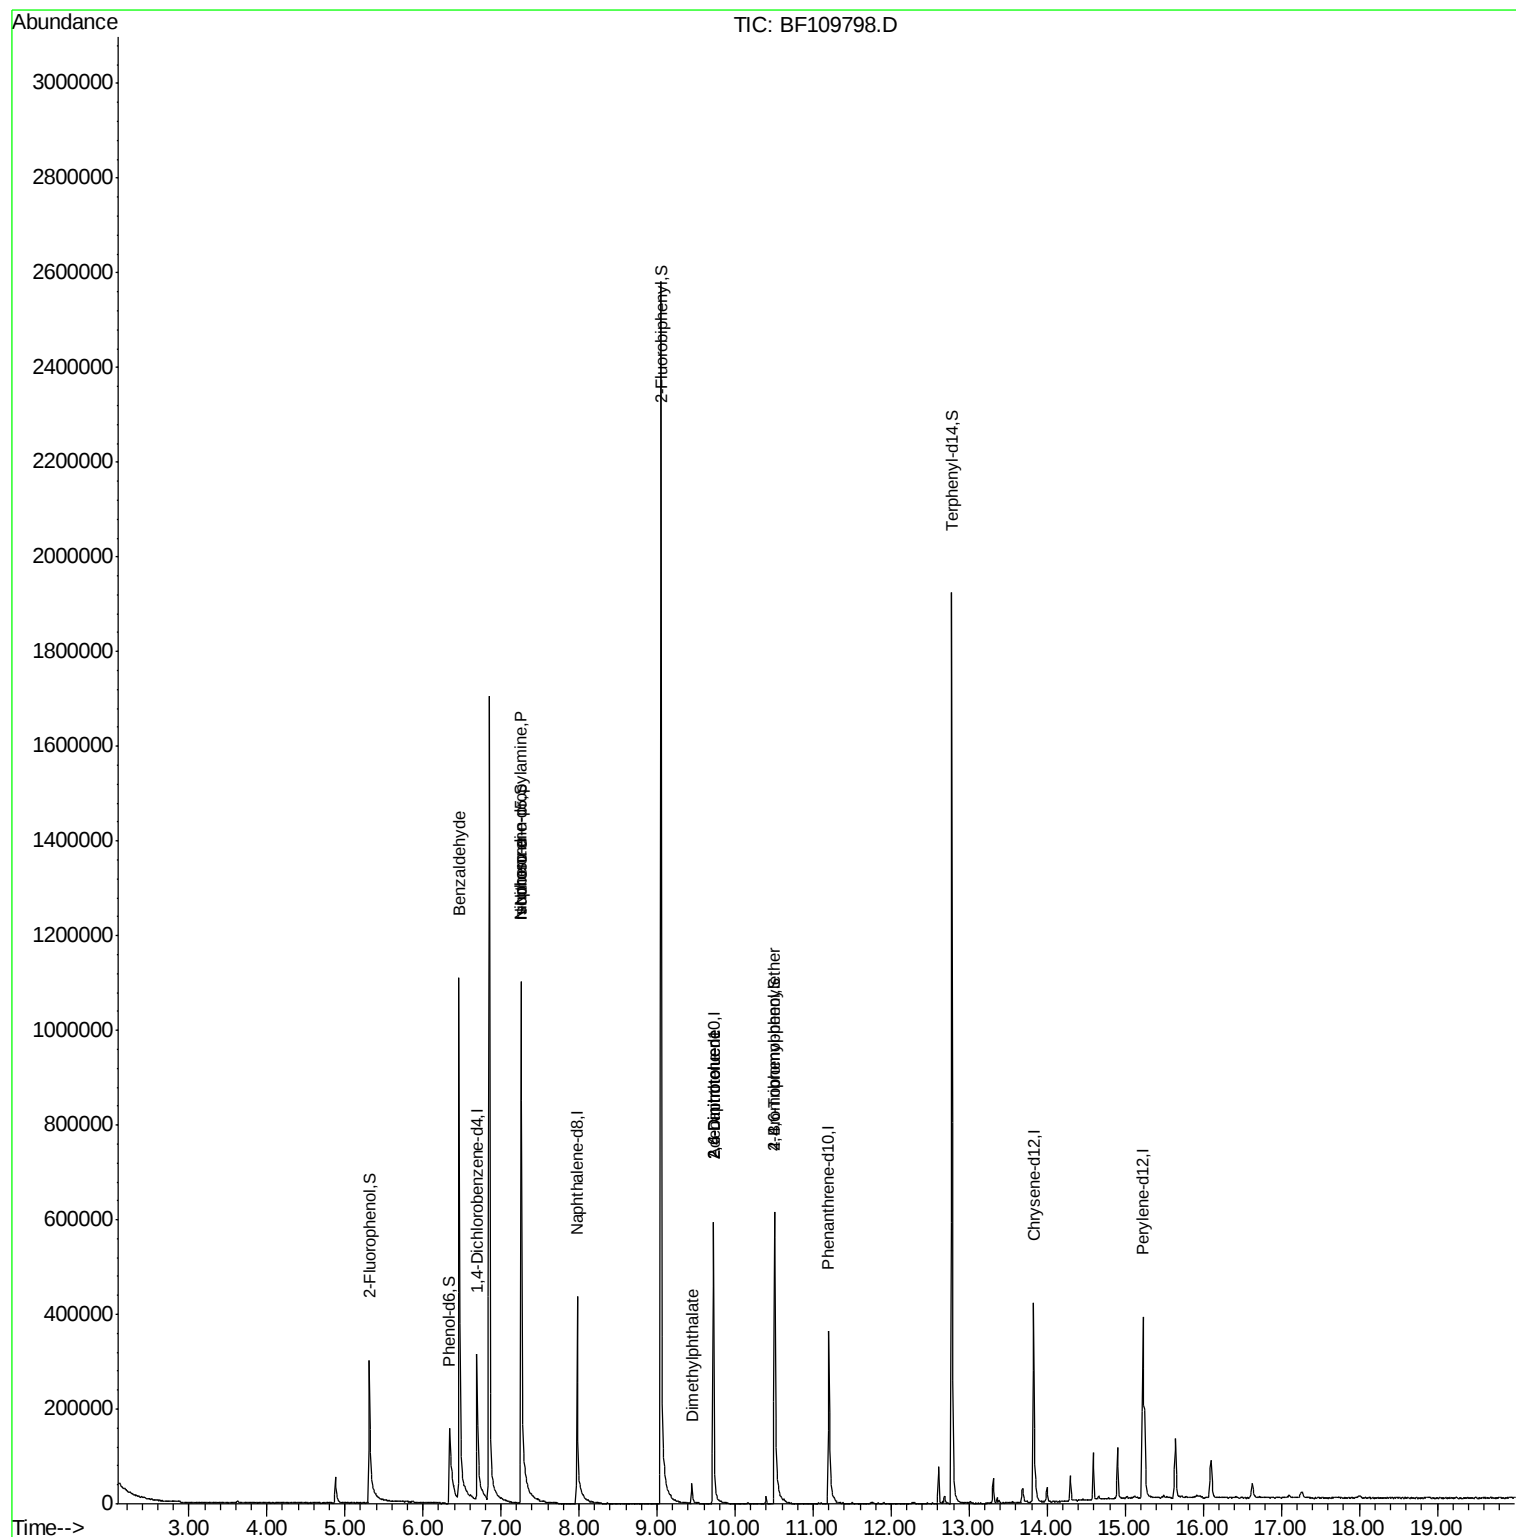


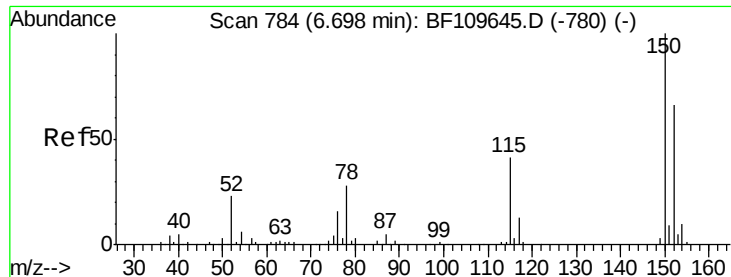




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.69 min Scan# 783
 Delta R.T. -0.01 min
 Lab File: BF109798.D
 Acq: 11 Oct 2018 20:34

Instrument :
 BNA_F
 ClientSampleId :
 100418-JETT-E-D-S

Tgt Ion:152 Resp: 78558
 Ion Ratio Lower Upper
 152 100
 150 154.5 122.7 184.1
 115 61.4 49.1 73.7

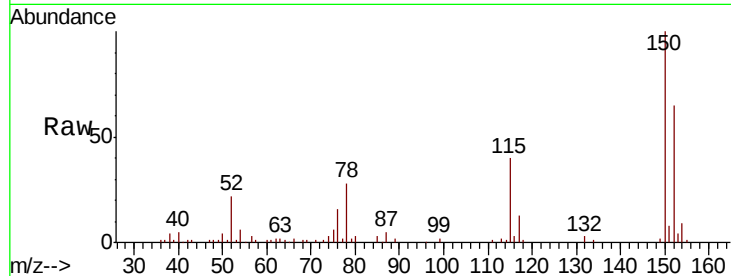


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

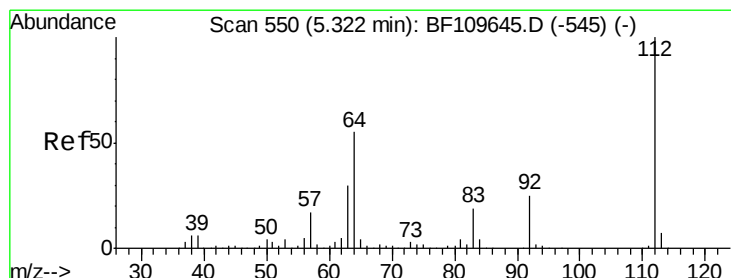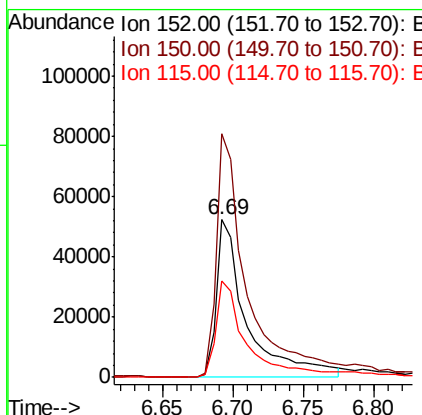
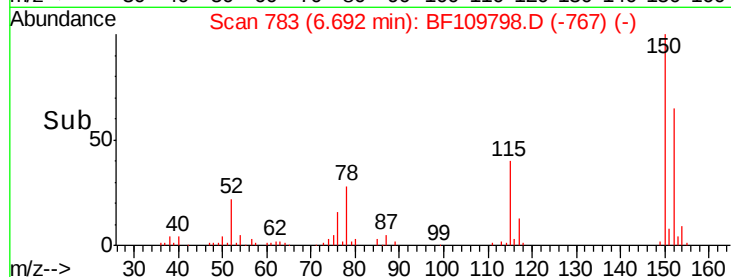



#5
 2-Fluorophenol
 Concen: 39.005 ng
 RT: 5.31 min Scan# 548
 Delta R.T. -0.01 min
 Lab File: BF109798.D
 Acq: 11 Oct 2018 20:34

Tgt Ion:112 Resp: 172624
 Ion Ratio Lower Upper
 112 100
 64 59.0 44.1 66.1
 63 30.5 23.7 35.5

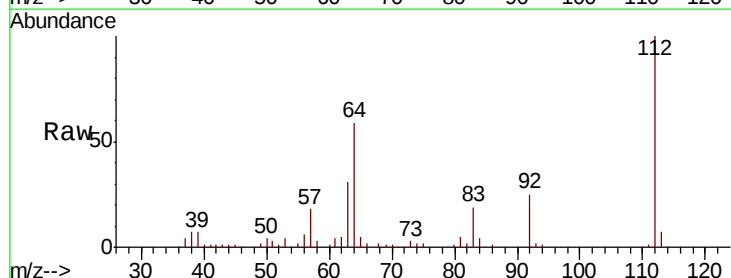

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

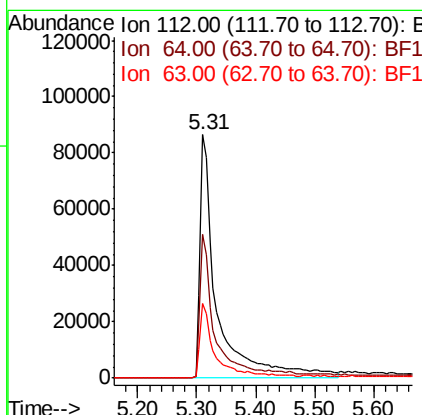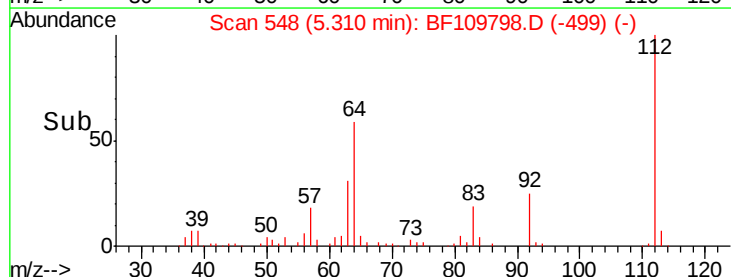

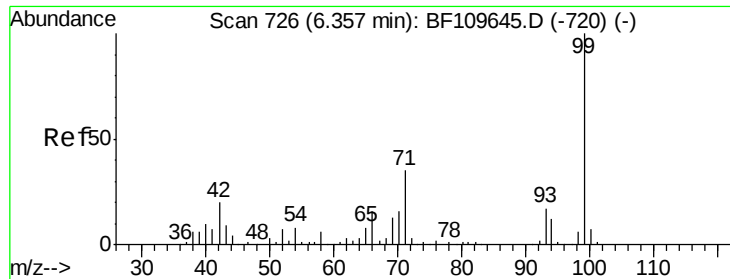

#7

Phenol-d6

Concen: 26.529 ng

RT: 6.34 min Scan# 723

Delta R.T. -0.02 min

Lab File: BF109798.D

Acq: 11 Oct 2018 20:34

Instrument :

BNA_F

ClientSampleId :

100418-JETT-E-D-S


Tgt Ion: 99 Resp: 156849

Ion Ratio Lower Upper

99 100

42 20.3 15.8 23.6




71 36.0 28.0 42.0

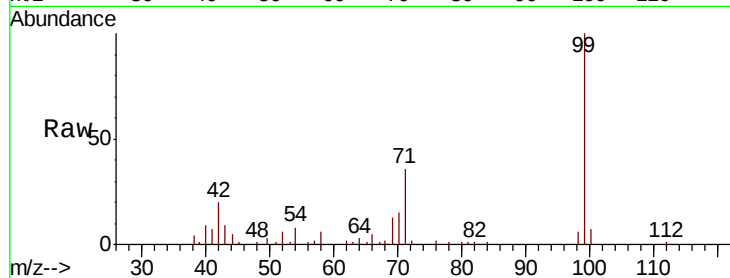

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

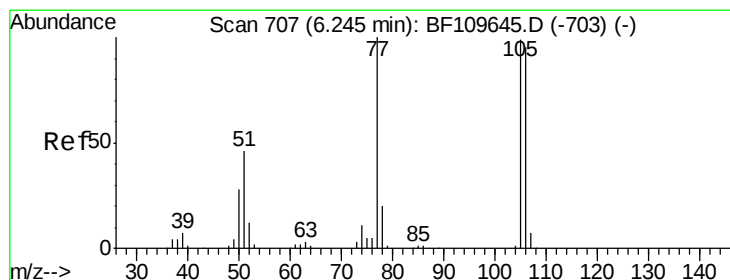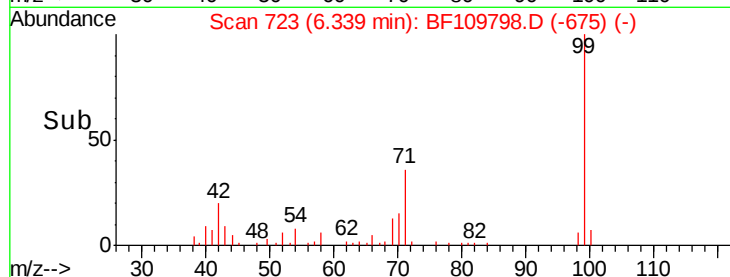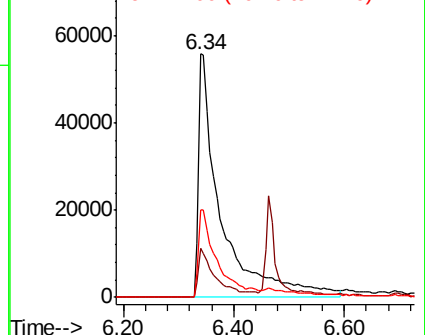

#9

Benzaldehyde

Concen: 2.171 ng

RT: 6.46 min Scan# 744

Delta R.T. 0.22 min

Lab File: BF109798.D

Acq: 11 Oct 2018 20:34


Tgt Ion: 77 Resp: 8259

Ion Ratio Lower Upper

77 100

105 80.5 78.6 118.6



106 70.1 74.8 114.8#

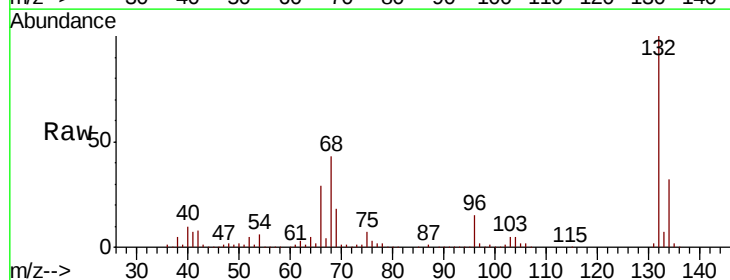


Abundance Ion 77.00 (76.70 to 77.70): BF1

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E



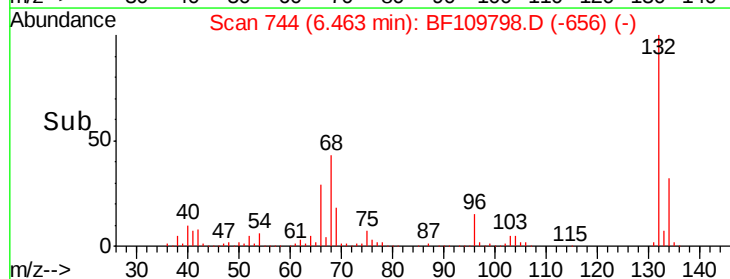
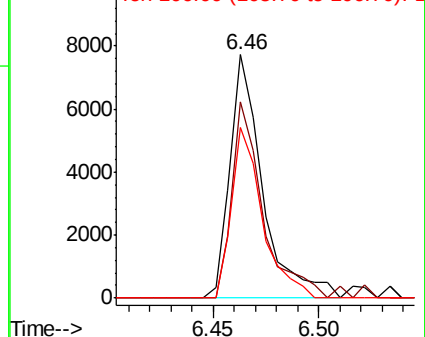


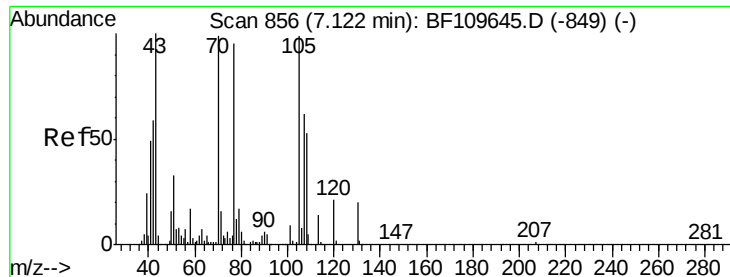

#19
n-Nitroso-di-n-propylamine
Concen: 17.587 ng
RT: 7.26 min Scan# 879
Delta R.T. 0.14 min
Lab File: BF109798.D
Acq: 11 Oct 2018 20:34




Instrument :
BNA_F
ClientSampleId :
100418-JETT-E-D-S


Tgt Ion: 70 Resp: 72918
Ion Ratio Lower Upper
70 100
42 48.2 47.4 71.2
101 0.0 7.3 10.9#
130 1.8 16.2 24.2#

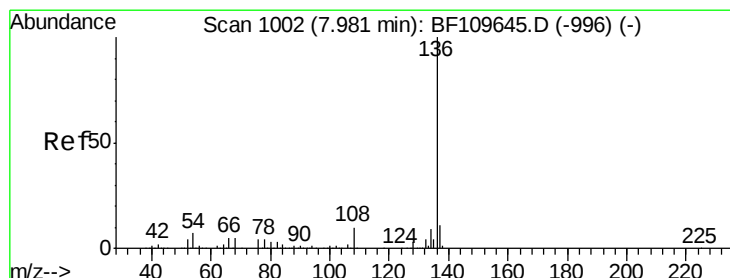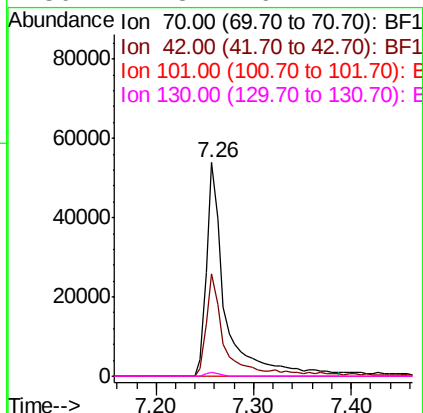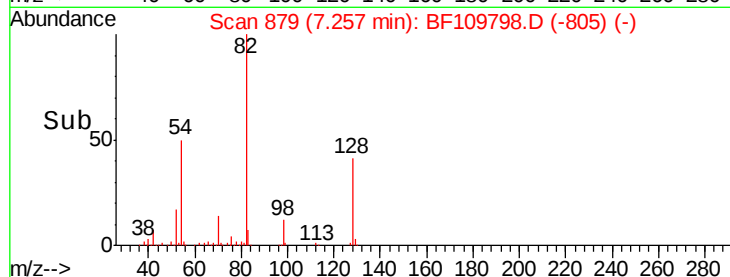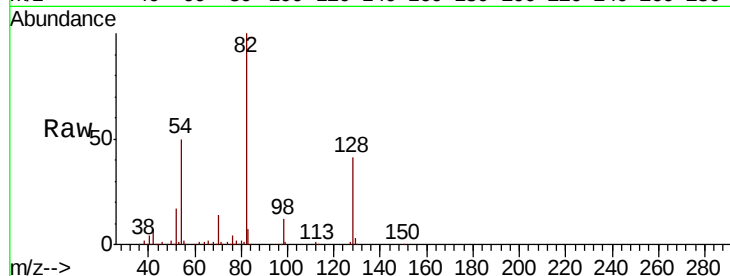

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.97 min Scan# 1001
Delta R.T. -0.01 min
Lab File: BF109798.D
Acq: 11 Oct 2018 20:34

Tgt Ion: 136 Resp: 323251
Ion Ratio Lower Upper
136 100
137 10.6 8.8 13.2
54 6.8 5.4 8.2
68 5.2 4.2 6.2


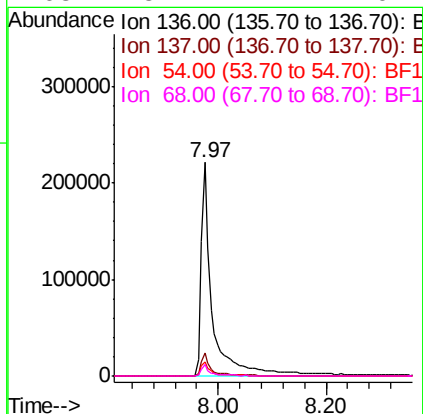
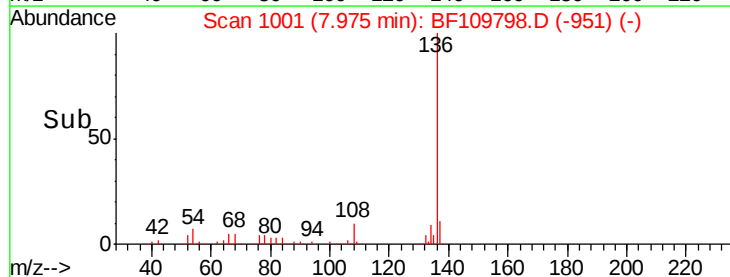
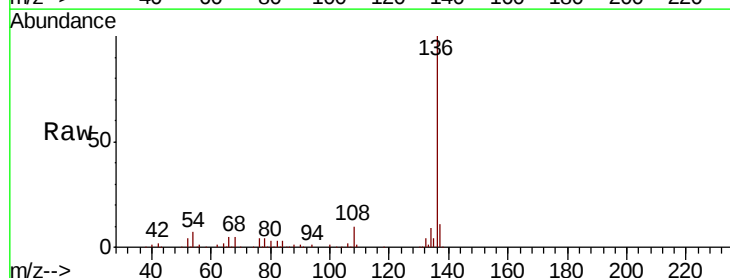


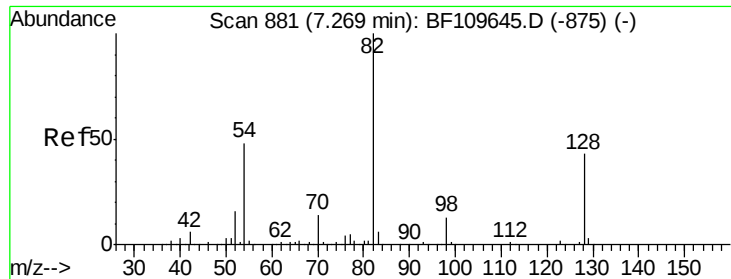

#23
Nitrobenzene-d5
Concen: 96.941 ng
RT: 7.26 min Scan# 879
Delta R.T. -0.01 min
Lab File: BF109798.D
Acq: 11 Oct 2018 20:34




Instrument :
BNA_F
ClientSampleId :
100418-JETT-E-D-S


Tgt Ion	Ratio	Lower	Upper
82	100		
128	41.2	34.2	51.2
54	49.8	38.6	58.0

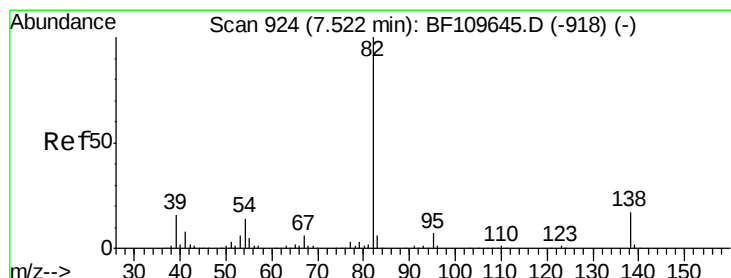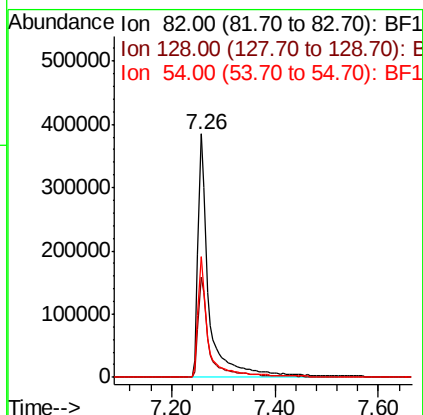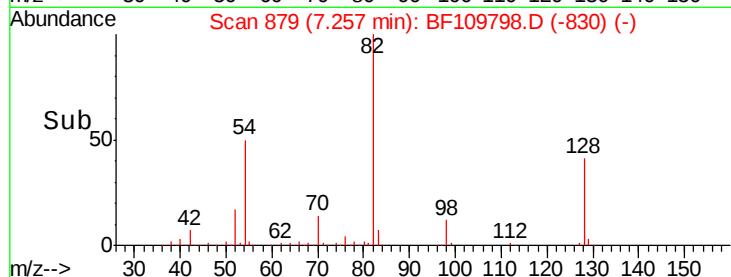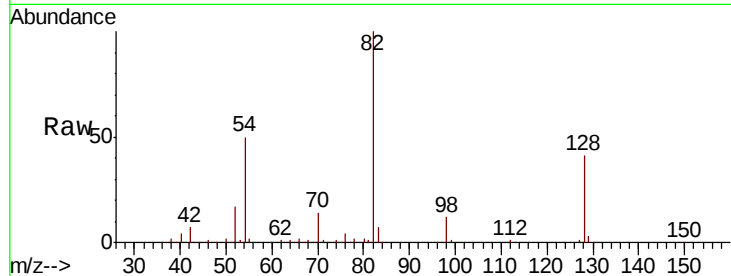

#25
Isophorone
Concen: 58.379 ng
RT: 7.26 min Scan# 879
Delta R.T. -0.26 min
Lab File: BF109798.D
Acq: 11 Oct 2018 20:34

Tgt Ion	Ratio	Lower	Upper
82	100		
95	0.0	5.7	8.5#
138	0.0	13.2	19.8#

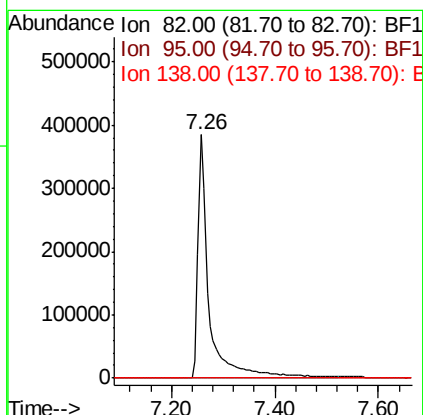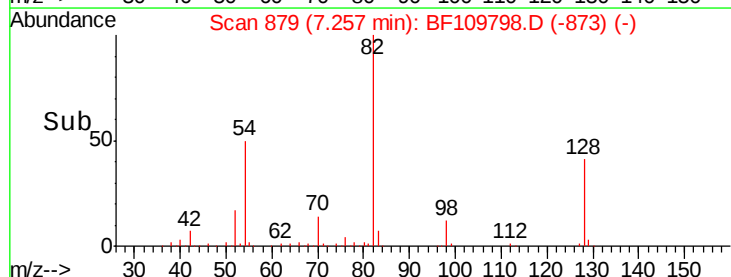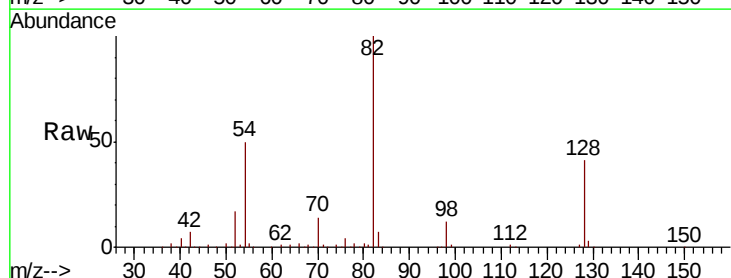

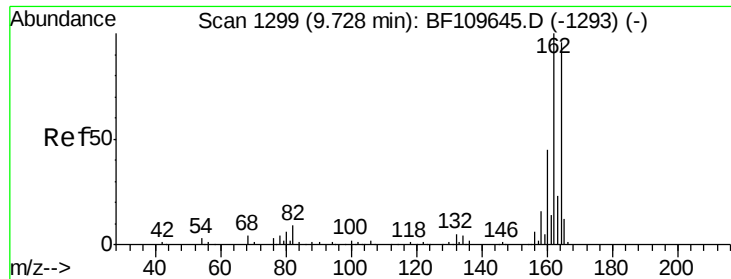

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.72 min Scan# 1298

Delta R.T. -0.01 min

Lab File: BF109798.D

Acq: 11 Oct 2018 20:34

Instrument :

BNA_F

ClientSampleId :

100418-JETT-E-D-S


Tgt Ion:164 Resp: 144034

Ion Ratio Lower Upper




164 100

162 105.4 83.0 124.6

160 48.2 37.0 55.6

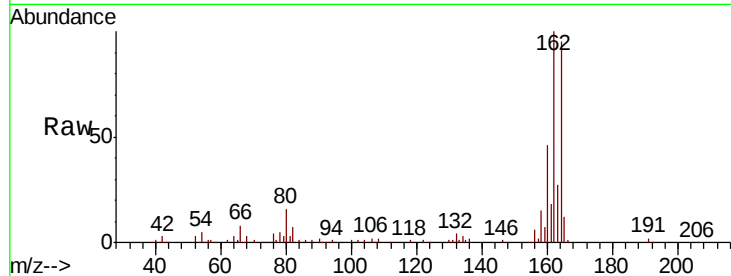

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

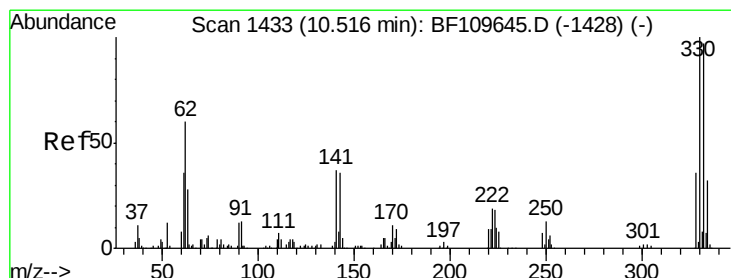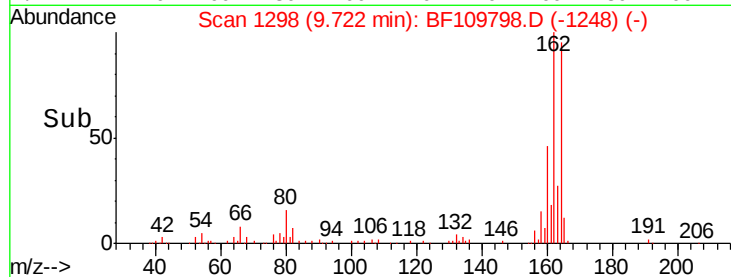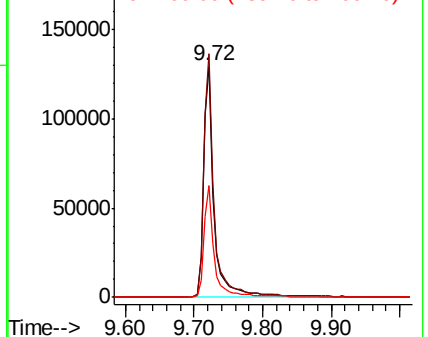

#41

2,4,6-Tribromophenol

Concen: 74.640 ng

RT: 10.51 min Scan# 1432

Delta R.T. -0.01 min

Lab File: BF109798.D

Acq: 11 Oct 2018 20:34


Tgt Ion:330 Resp: 117141

Ion Ratio Lower Upper



330 100


332 98.3 77.1 115.7

141 35.5 27.0 40.4

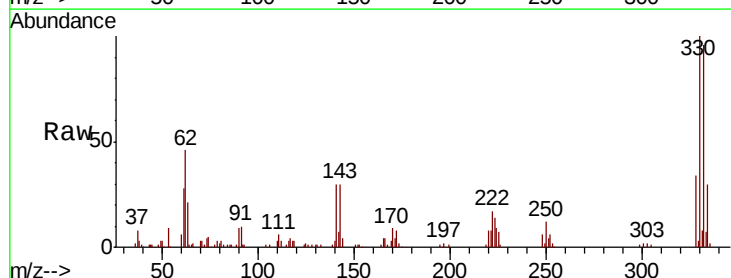

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

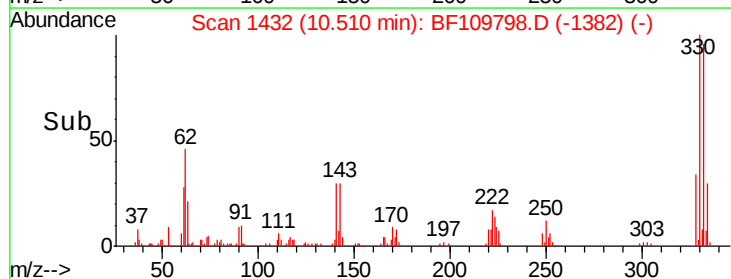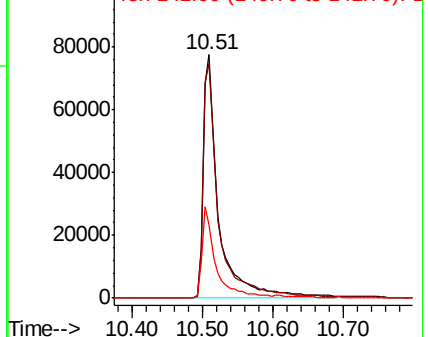


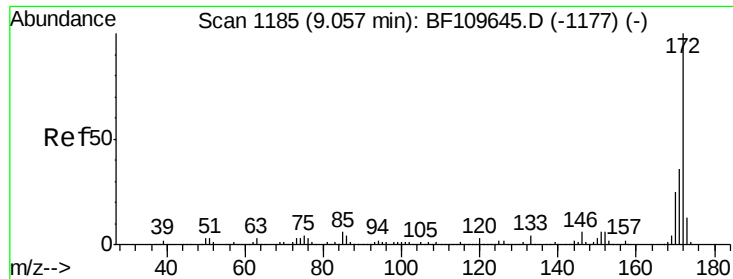




#44
2-Fluorobiphenyl
Concen: 95.002 ng
RT: 9.05 min Scan# 1184
Delta R.T. -0.01 min
Lab File: BF109798.D
Acq: 11 Oct 2018 20:34

Instrument :
BNA_F
ClientSampleId :
100418-JETT-E-D-S

Tgt Ion:172 Resp: 993535
Ion Ratio Lower Upper
172 100
171 35.9 28.6 43.0
170 23.9 19.7 29.5

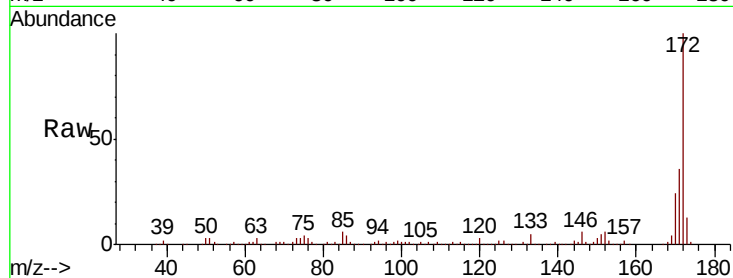


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

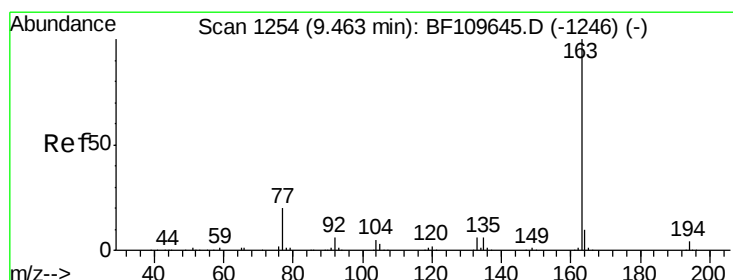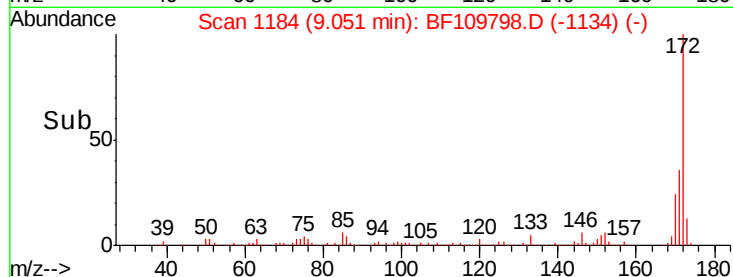
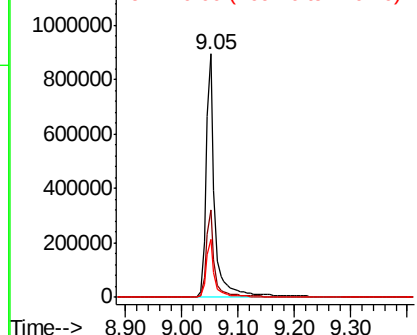



#49
Dimethylphthalate
Concen: 2.565 ng
RT: 9.45 min Scan# 1251
Delta R.T. -0.02 min
Lab File: BF109798.D
Acq: 11 Oct 2018 20:34

Tgt Ion:163 Resp: 27098
Ion Ratio Lower Upper
163 100
194 3.9 3.2 4.8
164 11.6 8.1 12.1

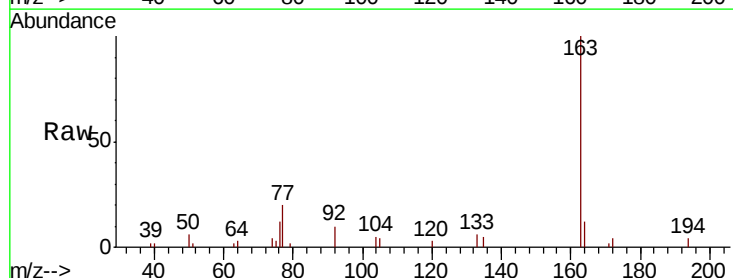

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E



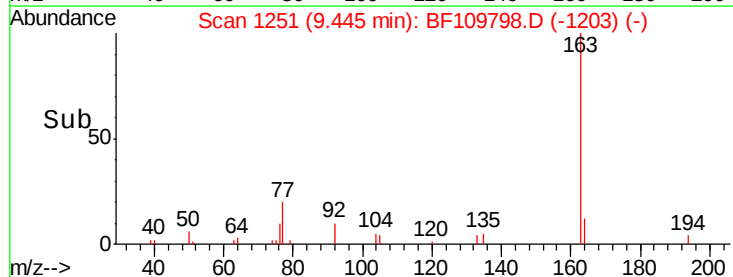
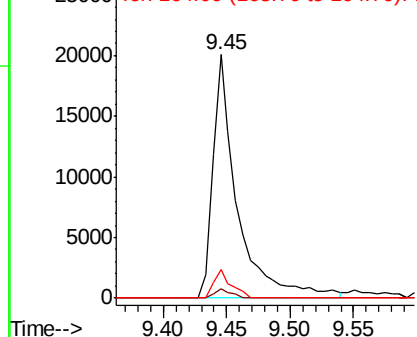


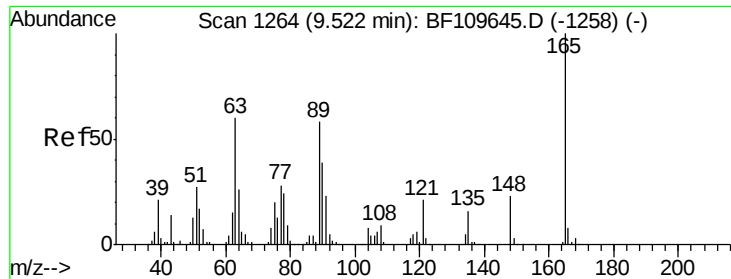

#50
 2,6-Dinitrotoluene
 Concen: 7.755 ng
 RT: 9.72 min Scan# 1298
 Delta R.T. 0.20 min
 Lab File: BF109798.D
 Acq: 11 Oct 2018 20:34




Instrument :
 BNA_F
 ClientSampleId :
 100418-JETT-E-D-S


Tgt Ion:165 Resp: 17757
 Ion Ratio Lower Upper
 165 100
 63 0.0 48.9 73.3#
 89 0.0 46.6 69.8#

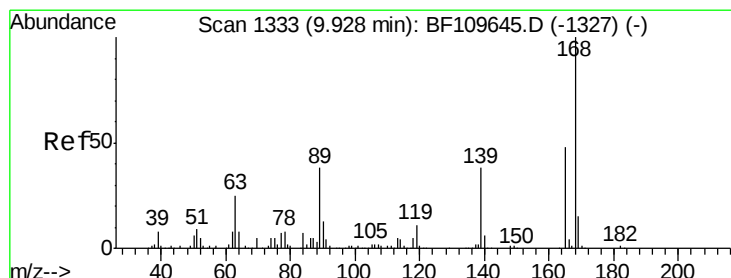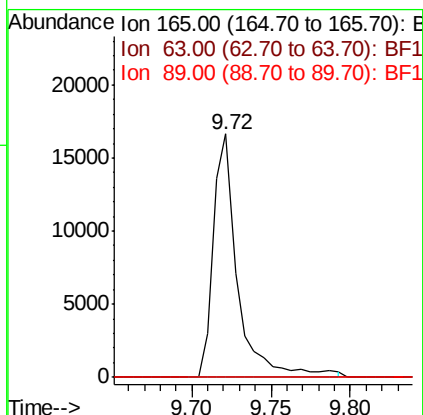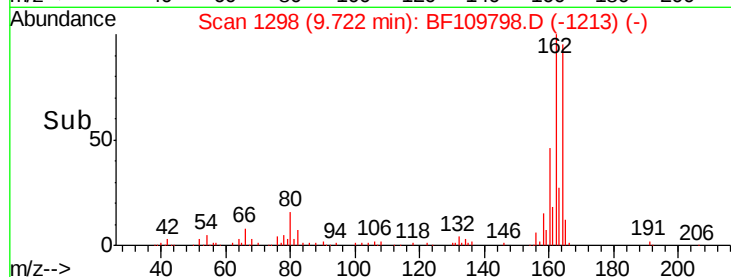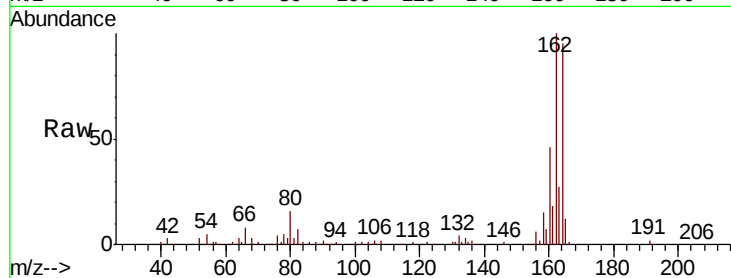

#56
 2,4-Dinitrotoluene
 Concen: 6.214 ng
 RT: 9.72 min Scan# 1298
 Delta R.T. -0.21 min
 Lab File: BF109798.D
 Acq: 11 Oct 2018 20:34

Tgt Ion:165 Resp: 17757
 Ion Ratio Lower Upper
 165 100
 63 0.0 44.8 67.2#
 89 0.0 62.2 93.4#
 182 0.0 2.1 3.1#


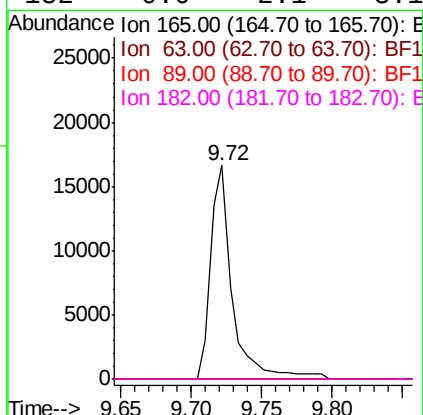
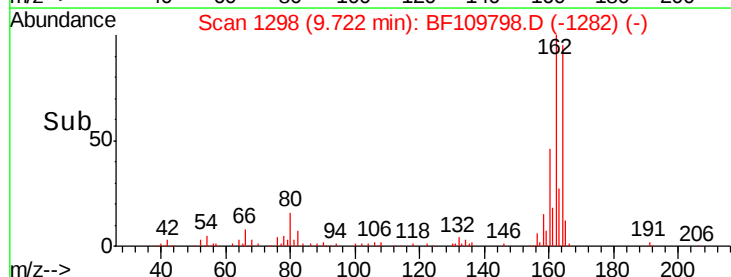
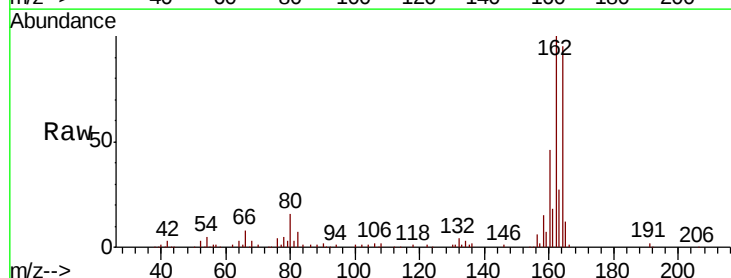


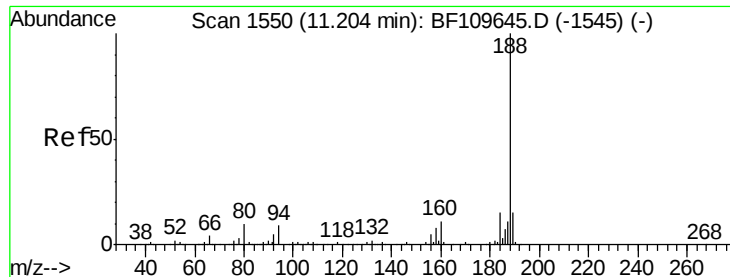

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.20 min Scan# 1549
Delta R.T. -0.01 min
Lab File: BF109798.D
Acq: 11 Oct 2018 20:34




Instrument :
BNA_F
ClientSampleId :
100418-JETT-E-D-S


Tgt Ion:188 Resp: 233272
Ion Ratio Lower Upper
188 100
94 9.3 7.2 10.8
80 10.0 7.9 11.9

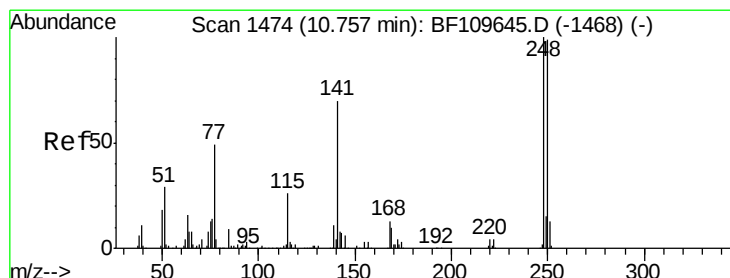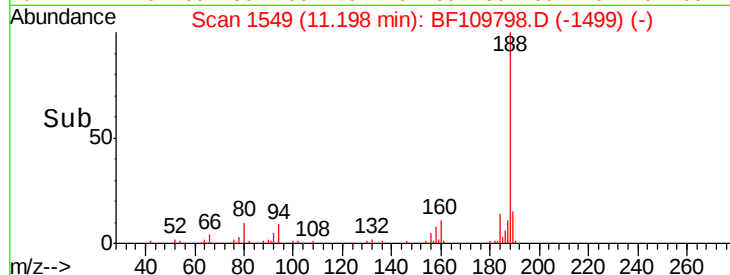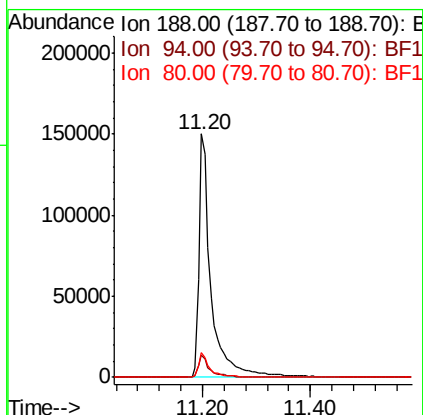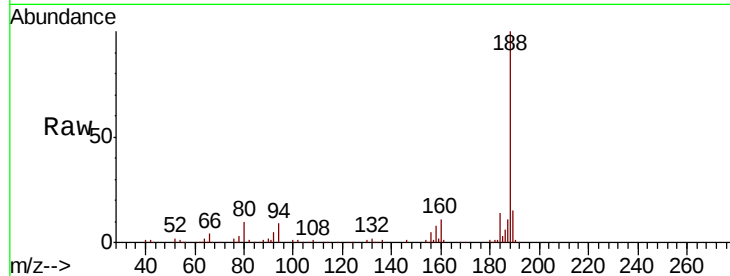

#66
4-Bromophenyl-phenylether
Concen: 2.525 ng
RT: 10.51 min Scan# 1432
Delta R.T. -0.25 min
Lab File: BF109798.D
Acq: 11 Oct 2018 20:34

Tgt Ion:248 Resp: 6767
Ion Ratio Lower Upper
248 100
250 199.6 79.4 119.2#
141 502.4 55.9 83.9#


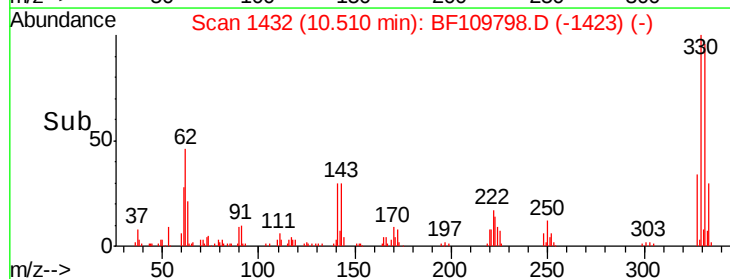
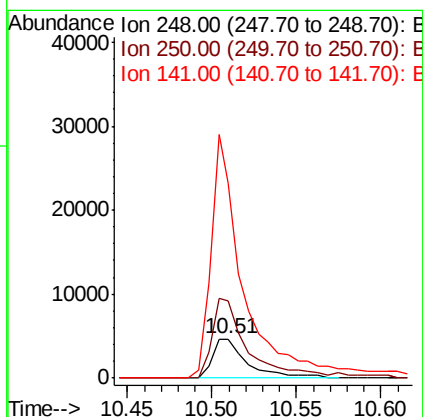
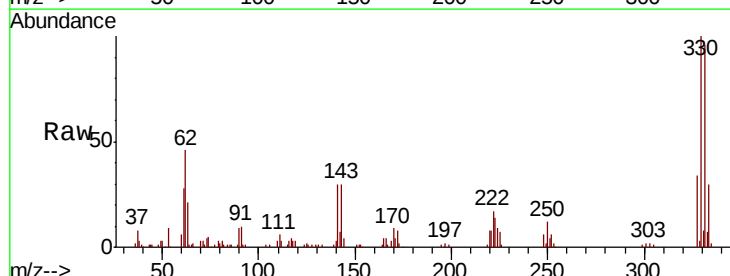


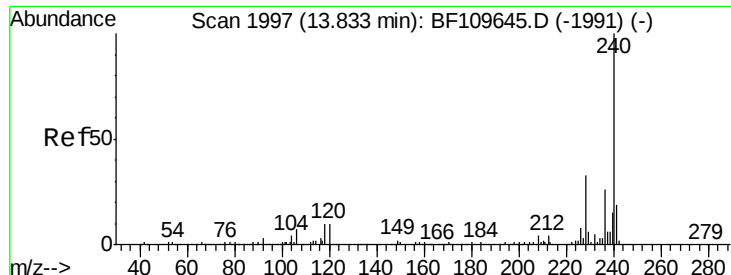

#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.83 min Scan# 1996
Delta R.T. -0.01 min
Lab File: BF109798.D
Acq: 11 Oct 2018 20:34




Instrument :
BNA_F
ClientSampleId :
100418-JETT-E-D-S


Tgt Ion:240 Resp: 203008
Ion Ratio Lower Upper
240 100
120 10.2 8.3 12.5
236 24.3 21.2 31.8

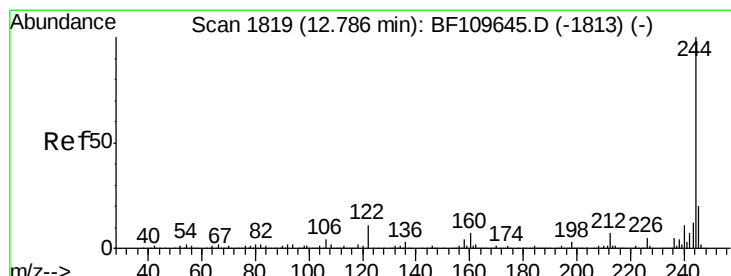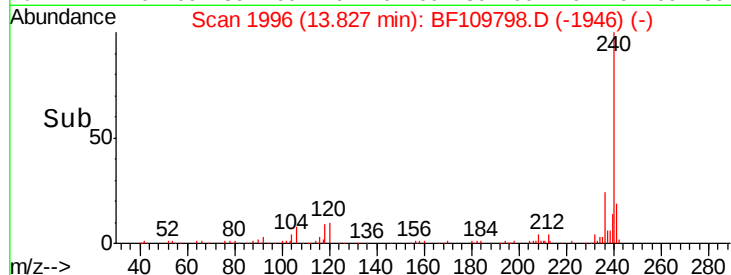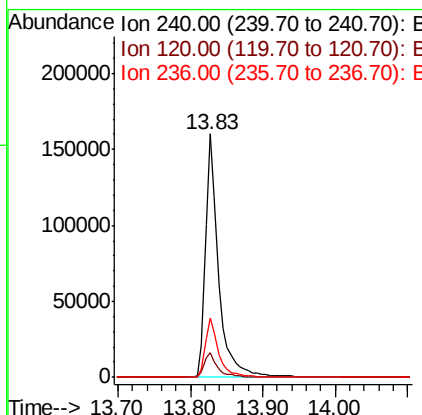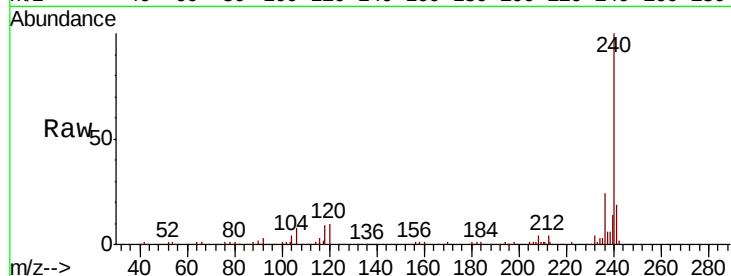

#78
Terphenyl-d14
Concen: 70.498 ng
RT: 12.78 min Scan# 1818
Delta R.T. -0.01 min
Lab File: BF109798.D
Acq: 11 Oct 2018 20:34

Tgt Ion:244 Resp: 739302
Ion Ratio Lower Upper
244 100
212 7.2 5.8 8.8
122 10.5 8.7 13.1

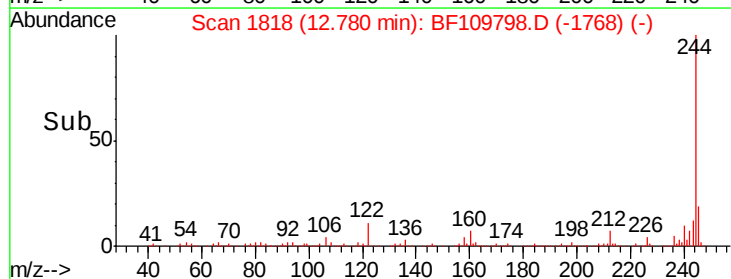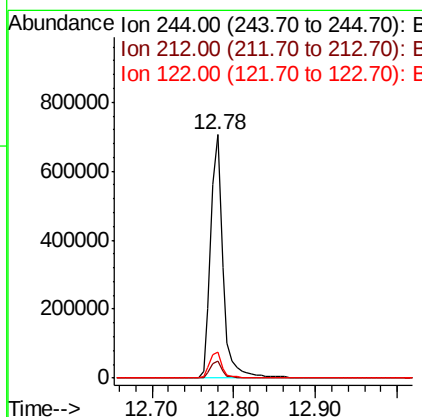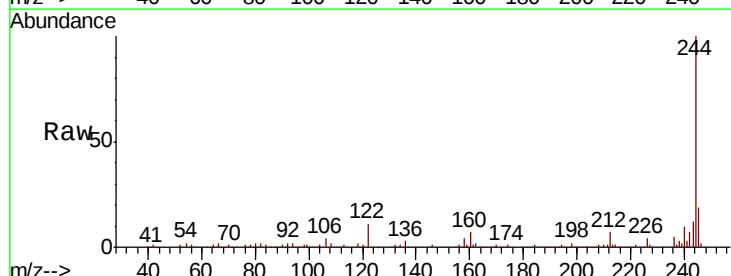

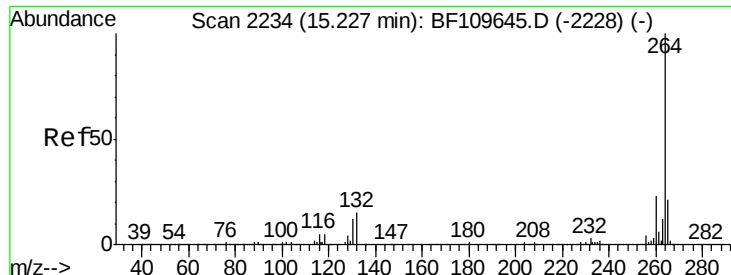

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.23 min Scan# 2234
Delta R.T. -0.00 min
Lab File: BF109798.D
Acq: 11 Oct 2018 20:34

Instrument :
BNA_F
ClientSampleId :
100418-JETT-E-D-S

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.1	18.7	28.1
265	21.1	16.7	25.1

