
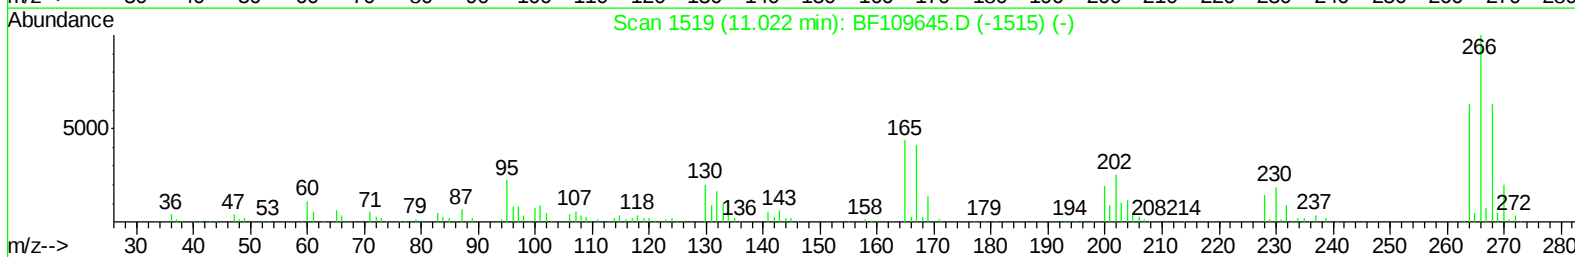
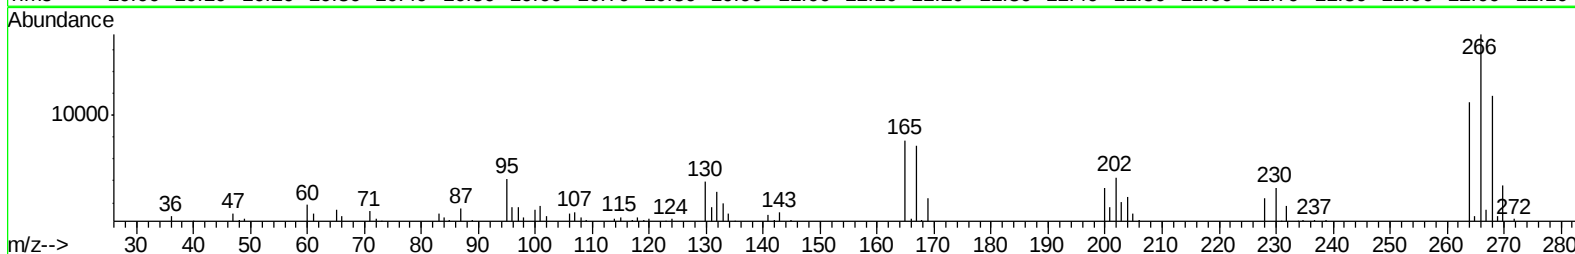


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101118\
Data File : BF109810.D
Acq On : 12 Oct 2018 2:42
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 08:58:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 08 16:02:11 2018
Response via : Initial Calibration

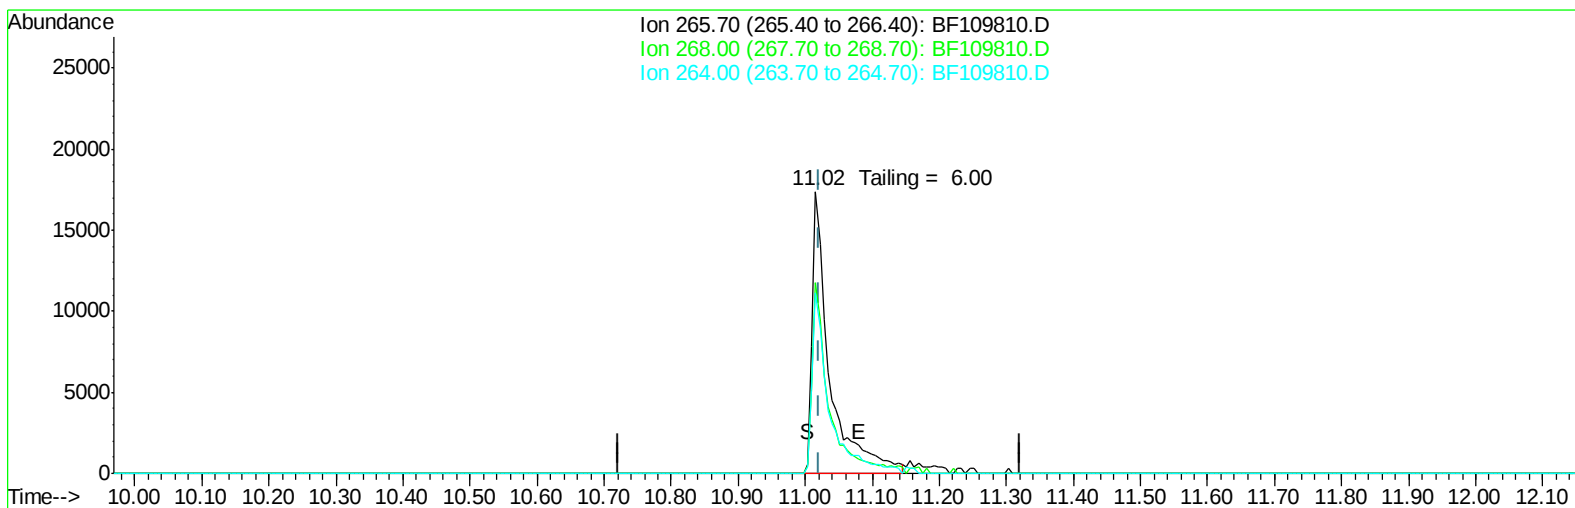

TIC: BF109810.D

(69) Pentachlorophenol (C)




11.016min (-0.006) 0.00ng

response 30895

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	67.91
264.00	63.20	64.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101118\
Data File : BF109810.D
Acq On : 12 Oct 2018 2:42
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 08:58:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 08 16:02:11 2018
Response via : Initial Calibration

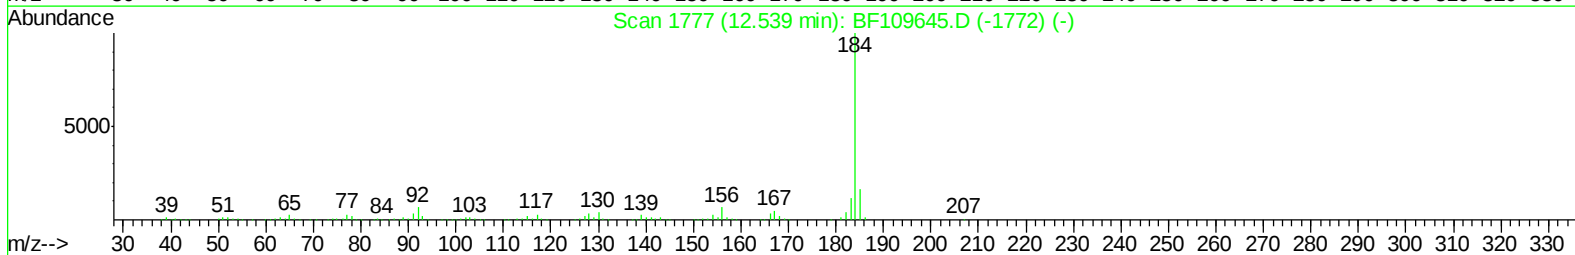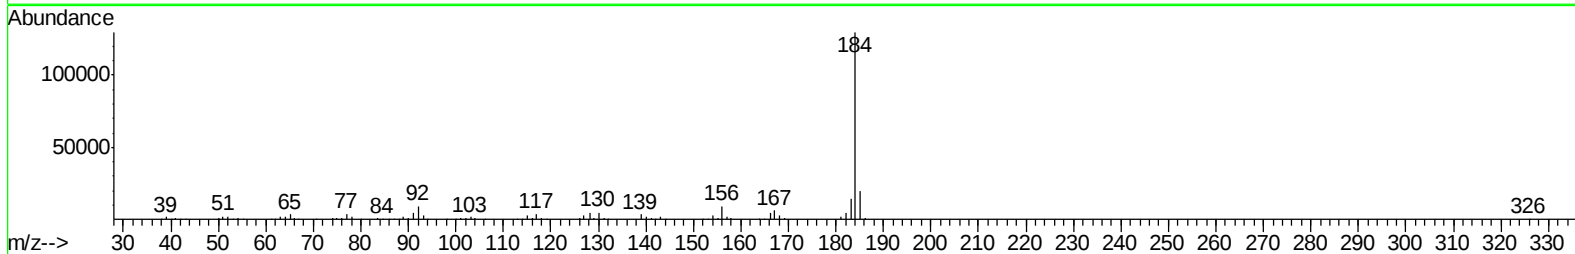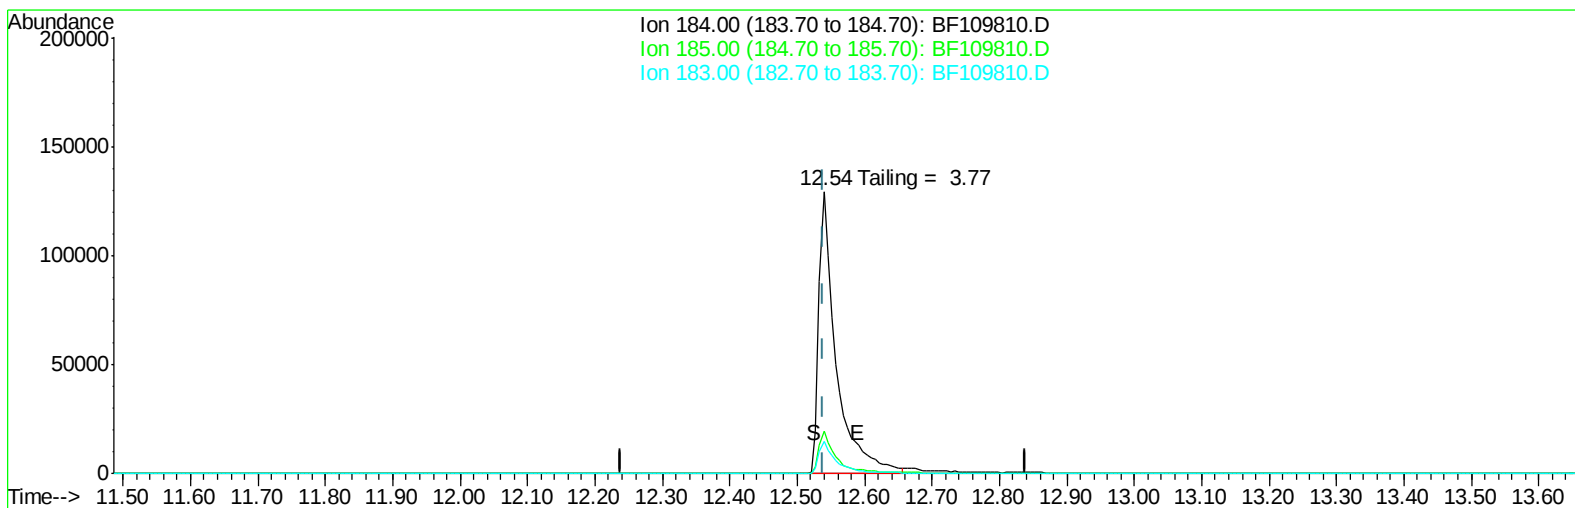

TIC: BF109810.D

(76) Benzidine

12.539min (-0.000) 0.00ng

response 227500

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	15.09
183.00	11.80	11.17
0.00	0.00	0.00