

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101118\
 Data File : BF109812.D
 Acq On : 12 Oct 2018 3:51
 Operator : JU/SJ
 Sample : J5296-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 100418-JETT-E-U-S

Quant Time: Oct 12 06:40:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF100818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 08 16:02:11 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.69	152	69878	20.00	ng	0.00
21) Naphthalene-d8	7.97	136	256599	20.00	ng	0.00
38) Acenaphthene-d10	9.72	164	101813	20.00	ng	0.00
63) Phenanthrene-d10	11.20	188	202180	20.00	ng	0.00
75) Chrysene-d12	13.83	240	228304	20.00	ng	0.00
86) Perylene-d12	15.23	264	165593	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.31	112	138736	35.24	ng	-0.01
7) Phenol-d6	6.35	99	119573	22.74	ng	-0.01
23) Nitrobenzene-d5	7.26	82	481644	103.47	ng	-0.01
41) 2,4,6-Tribromophenol	10.51	330	103396	93.20	ng	0.00
44) 2-Fluorobiphenyl	9.05	172	798079	107.96	ng	0.00
78) Terphenyl-d14	12.78	244	856047	72.59	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.45	163	16721	2.239	ng	Qvalue # 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101118\
Data File : BF109812.D
Acq On : 12 Oct 2018 3:51
Operator : JU/SJ
Sample : J5296-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
100418-JETT-E-U-S

Quant Time: Oct 12 06:40:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF100818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 08 16:02:11 2018
Response via : Initial Calibration

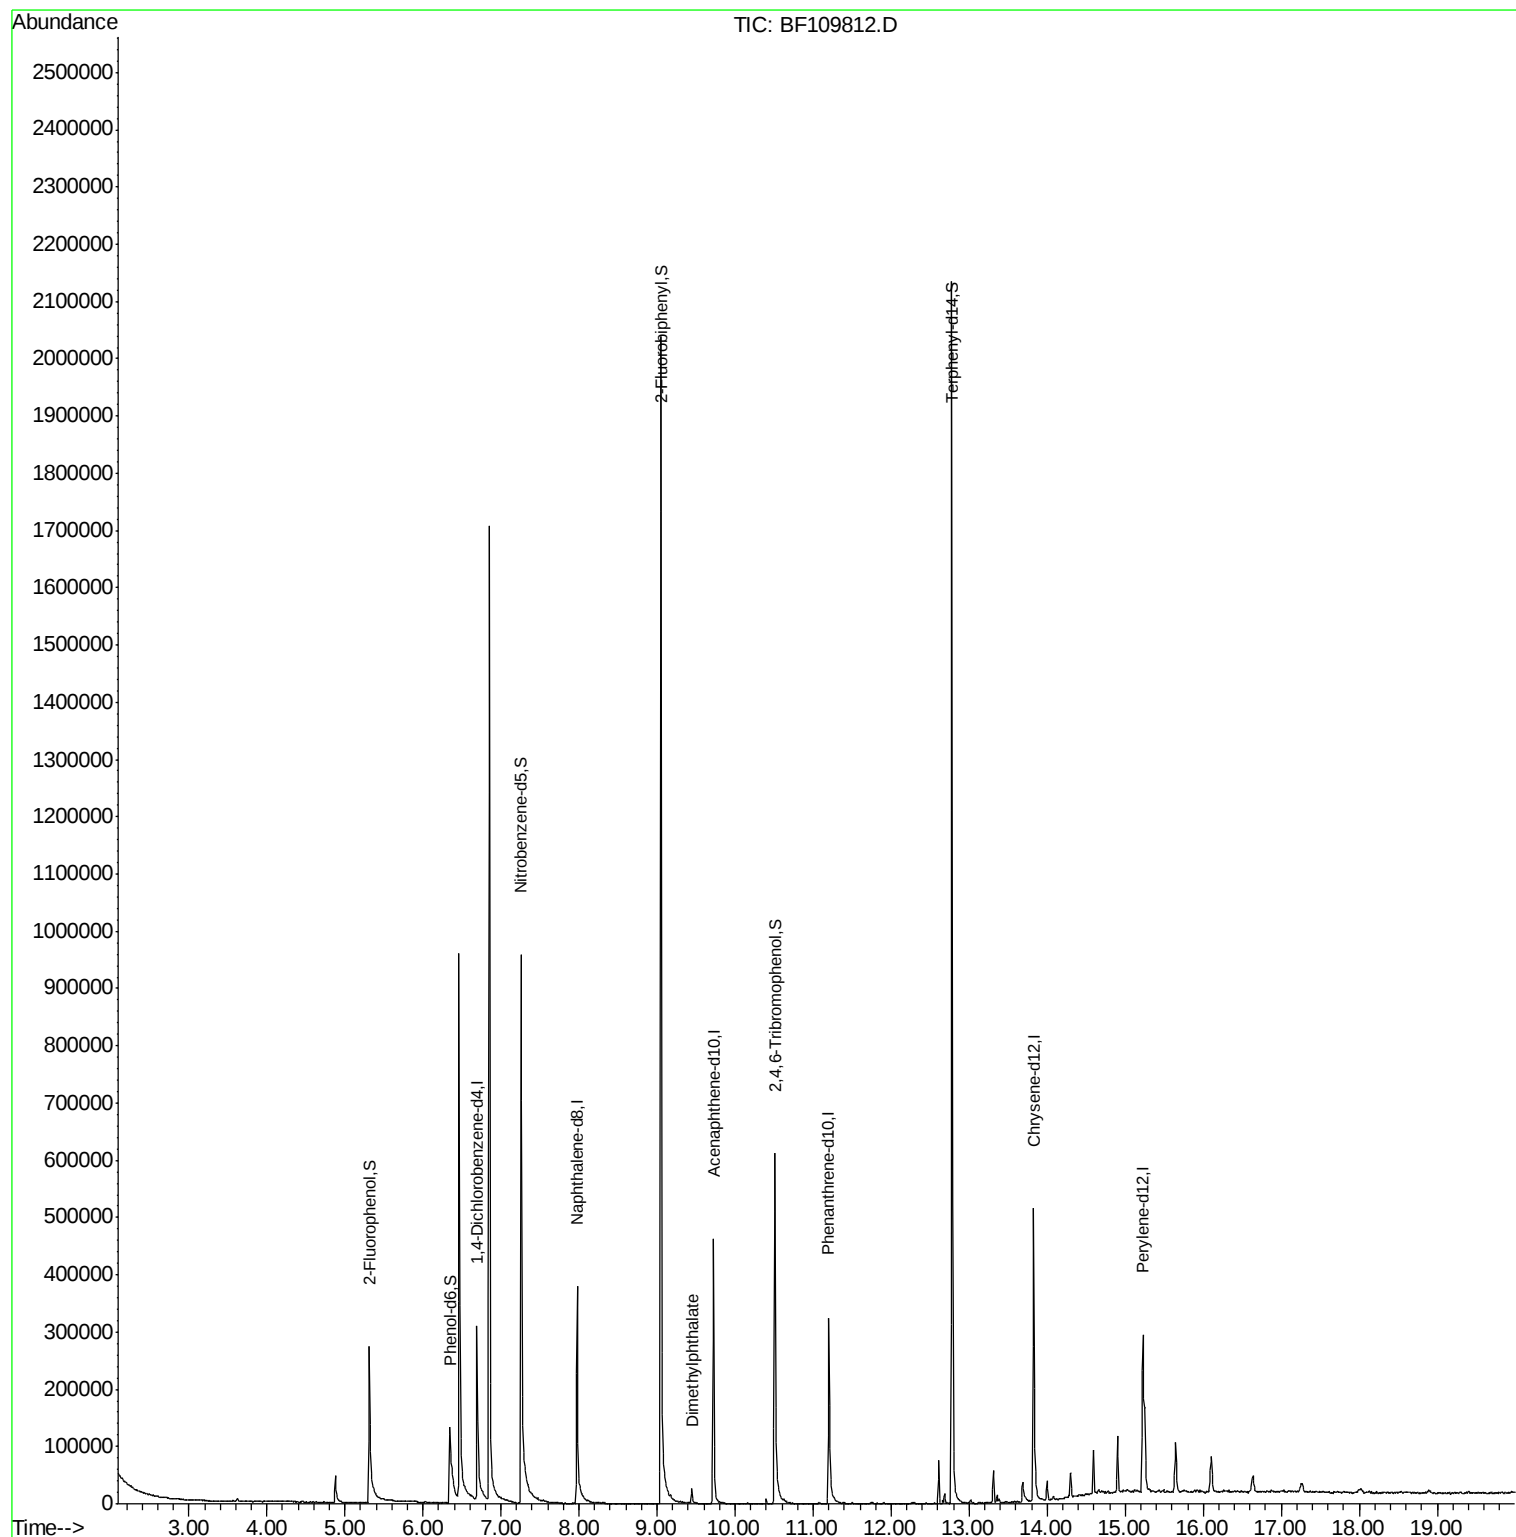

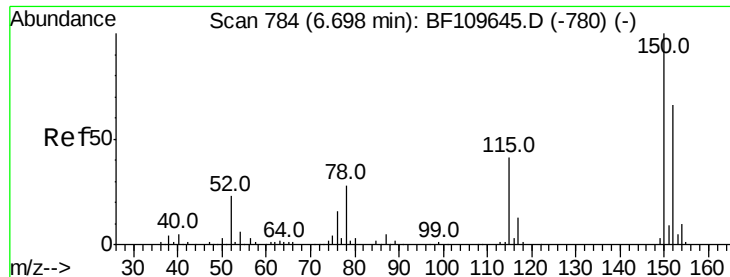


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.69 min Scan# 783
 Delta R.T. -0.01 min
 Lab File: BF109812.D
 Acq: 12 Oct 2018 3:51

Instrument :
 BNA_F
 ClientSampleId :
 100418-JETT-E-U-S

Tot Ion:152 Resp: 69878
 Ion Ratio Lower Upper
 152 100
 150 156.0 122.7 184.1
 115 62.8 49.1 73.7

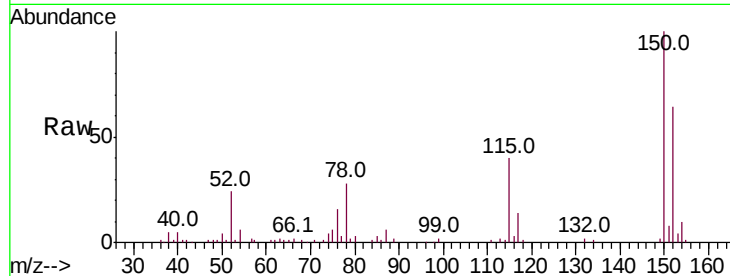


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

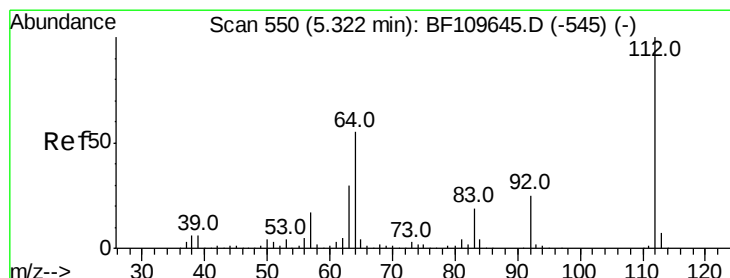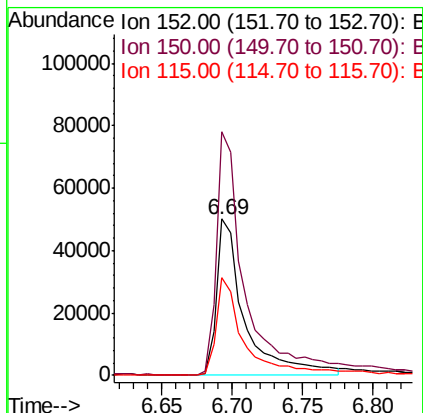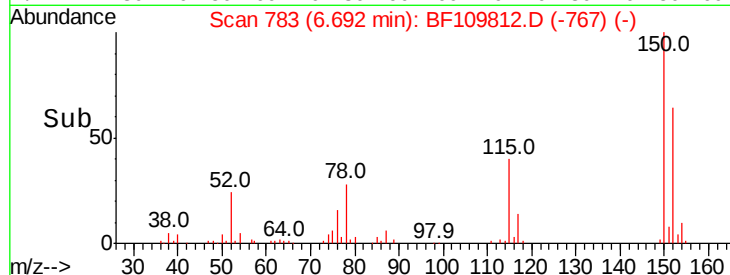



#5


2-Fluorophenol
 Concen: 35.242 ng
 RT: 5.31 min Scan# 548
 Delta R.T. -0.01 min
 Lab File: BF109812.D
 Acq: 12 Oct 2018 3:51

Tgt Ion:112 Resp: 138736
 Ion Ratio Lower Upper
 112 100
 64 58.7 44.1 66.1
 63 30.9 23.7 35.5

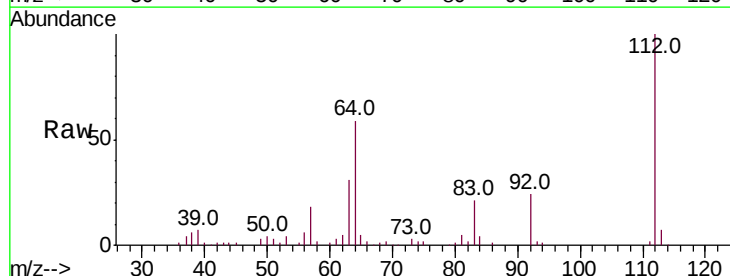

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

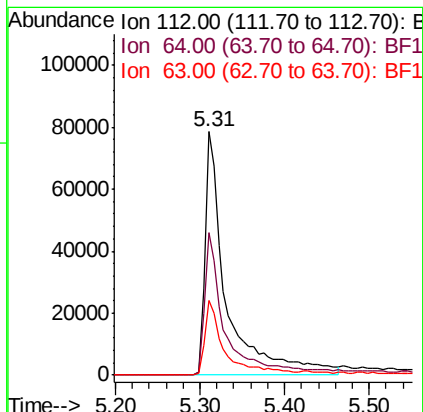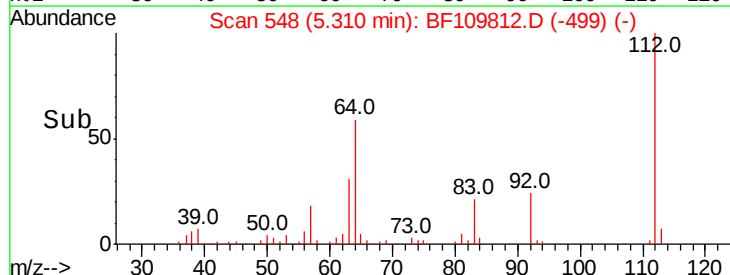

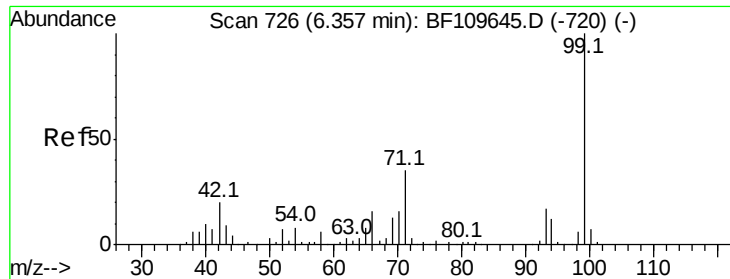

#7

Phenol-d6

Concen: 22.737 ng

RT: 6.35 min Scan# 724

Delta R.T. -0.01 min

Lab File: BF109812.D

Acq: 12 Oct 2018 3:51

Instrument :

BNA_F

ClientSampleId :

100418-JETT-E-U-S





Tot Ion: 99 Resp: 119573

Ion Ratio Lower Upper

99 100

42 19.0 15.8 23.6

71 36.3 28.0 42.0

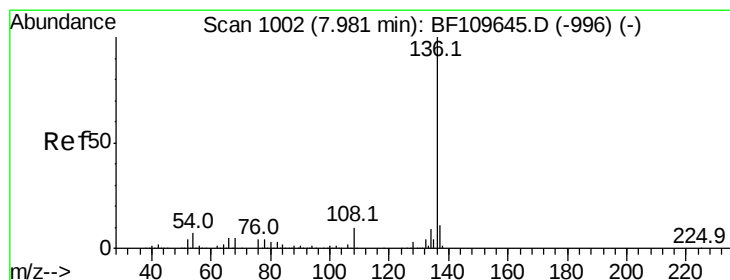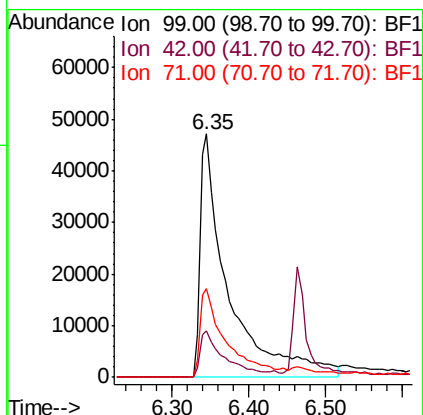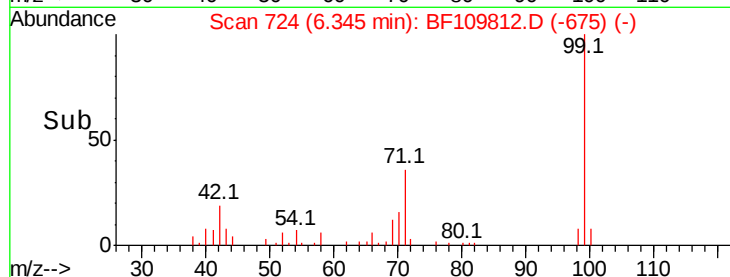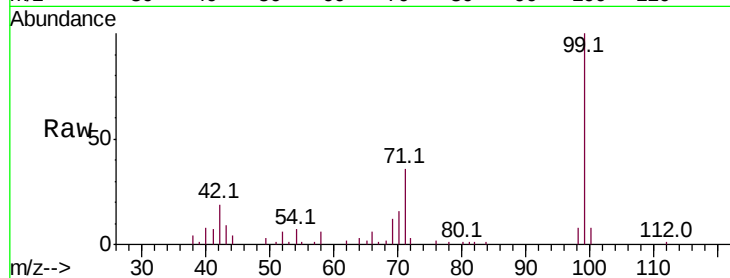

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.97 min Scan# 1001

Delta R.T. -0.01 min

Lab File: BF109812.D

Acq: 12 Oct 2018 3:51

Tgt Ion: 136 Resp: 256599




Ion Ratio Lower Upper


136 100

137 11.0 8.8 13.2

54 6.7 5.4 8.2

68 5.2 4.2 6.2


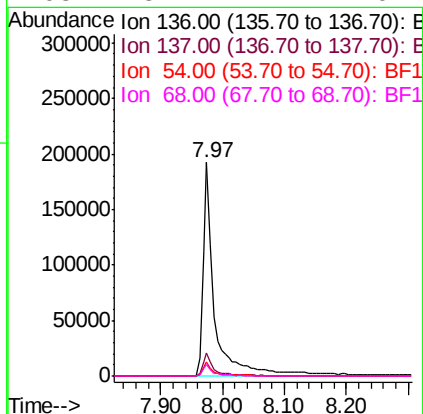
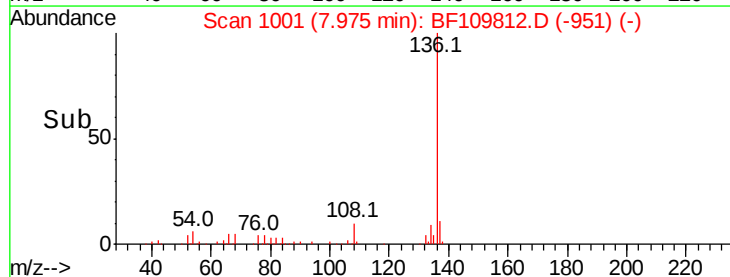
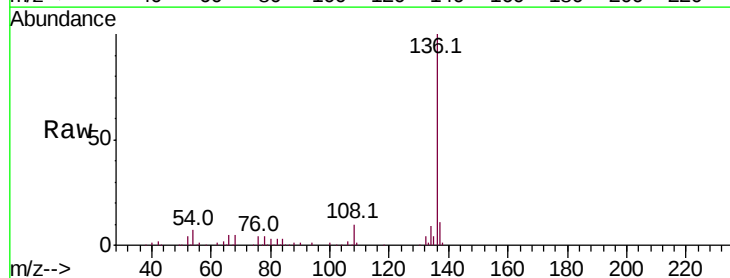


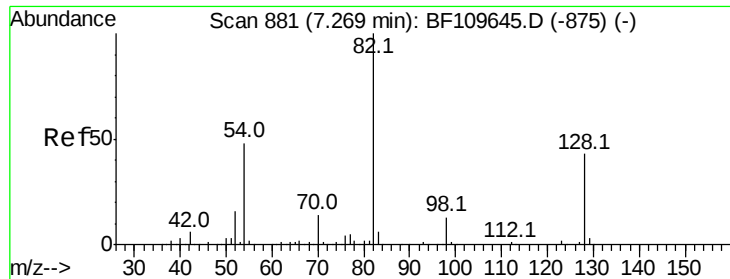

#23
 Nitrobenzene-d5
 Concen: 103.468 ng
 RT: 7.26 min Scan# 879
 Delta R.T. -0.01 min
 Lab File: BF109812.D
 Acq: 12 Oct 2018 3:51




Instrument :
 BNA_F
 ClientSampleId :
 100418-JETT-E-U-S


Tot Ion: 82 Resp: 481644
 Ion Ratio Lower Upper
 82 100
 128 42.1 34.2 51.2
 54 49.5 38.6 58.0

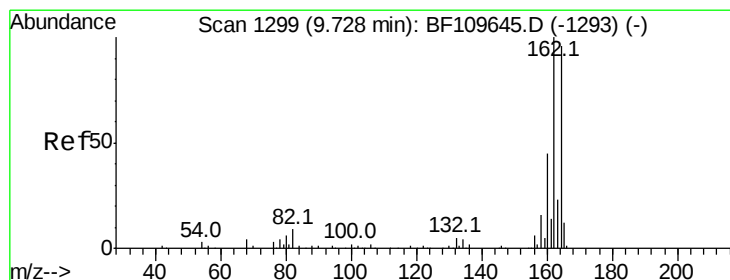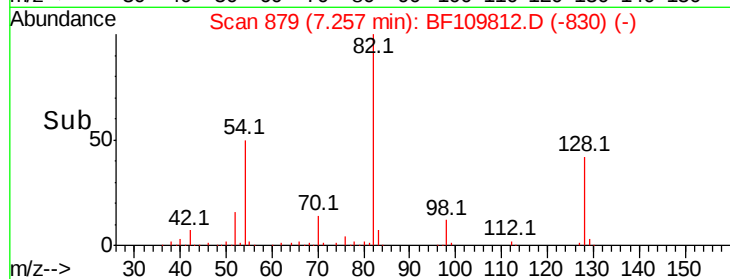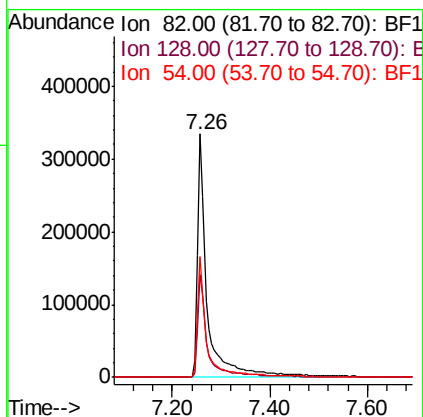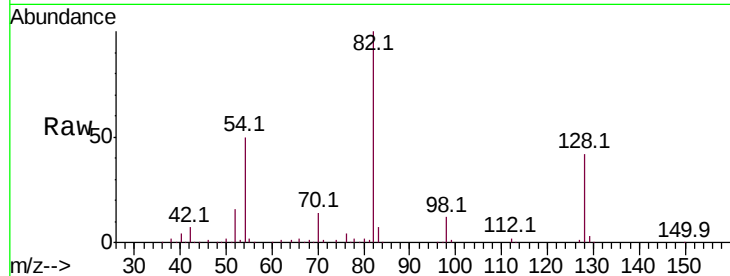

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.72 min Scan# 1298
 Delta R.T. -0.01 min
 Lab File: BF109812.D
 Acq: 12 Oct 2018 3:51

Tgt Ion:164 Resp: 101813
 Ion Ratio Lower Upper
 164 100
 162 103.3 83.0 124.6
 160 47.4 37.0 55.6


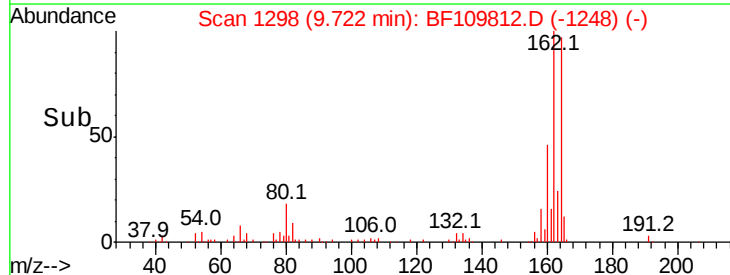
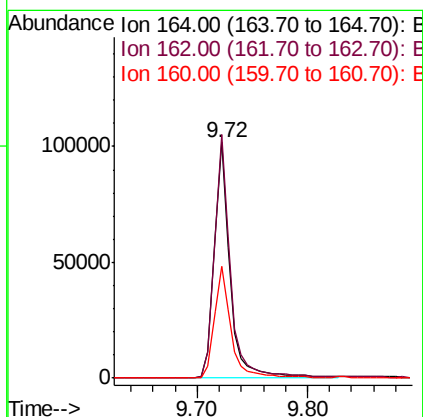
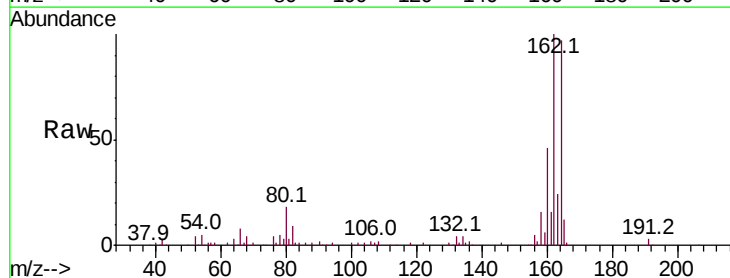


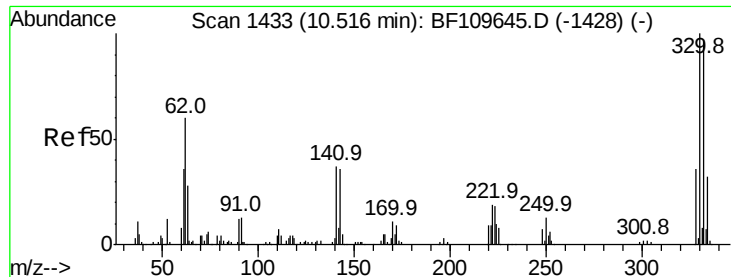

#41
 2,4,6-Tribromophenol
 Concen: 93.203 ng
 RT: 10.51 min Scan# 1432
 Delta R.T. -0.01 min
 Lab File: BF109812.D
 Acq: 12 Oct 2018 3:51




Instrument :
 BNA_F
 ClientSampleId :
 100418-JETT-E-U-S


Tot Ion	Ratio	Lower	Upper
330	100		
332	98.3	77.1	115.7
141	36.0	27.0	40.4

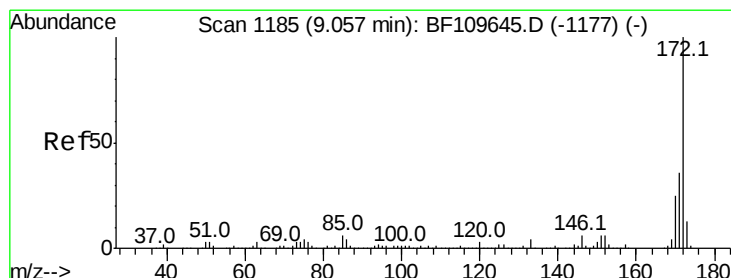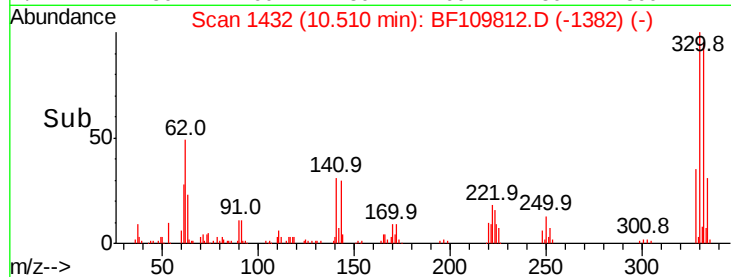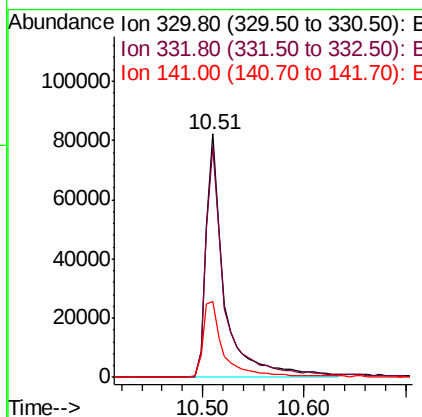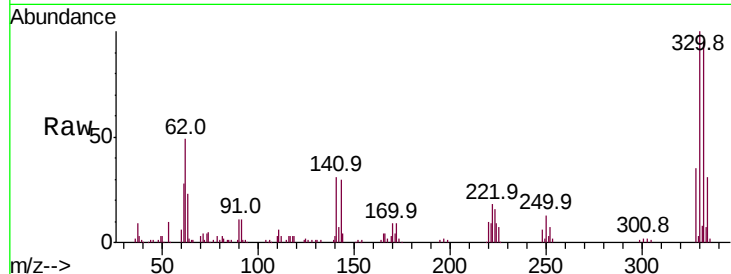

#44
 2-Fluorobiphenyl
 Concen: 107.958 ng
 RT: 9.05 min Scan# 1184
 Delta R.T. -0.01 min
 Lab File: BF109812.D
 Acq: 12 Oct 2018 3:51

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	28.6	43.0
170	24.1	19.7	29.5

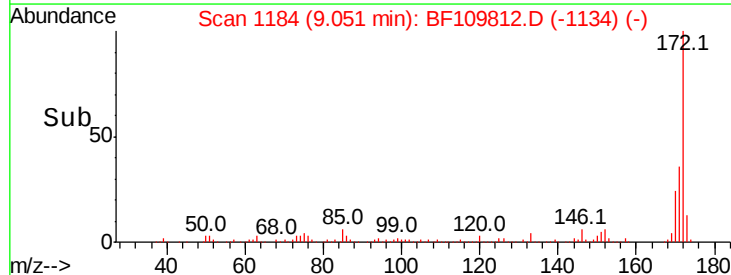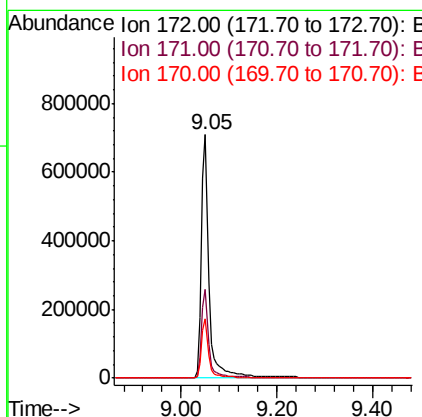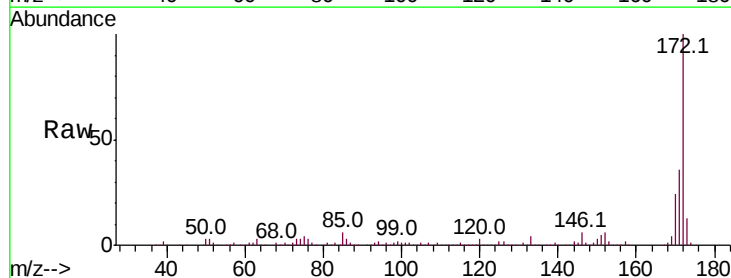

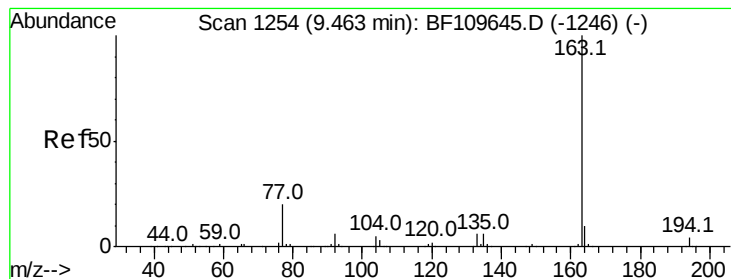

#49

Dimethylphthalate

Concen: 2.239 ng

RT: 9.45 min Scan# 1251

Delta R.T. -0.02 min

Lab File: BF109812.D

Acq: 12 Oct 2018 3:51

Instrument :

BNA_F

ClientSampleId :

100418-JETT-E-U-S


Tot Ion:163 Resp: 16721

Ion Ratio Lower Upper




163 100

194 3.0 3.2 4.8#

164 11.2 8.1 12.1

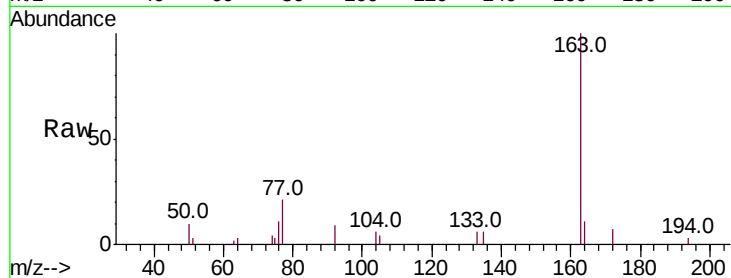

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

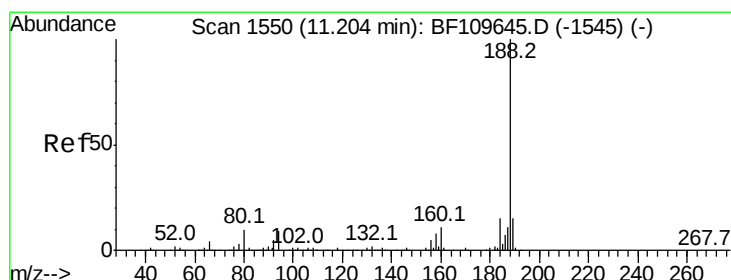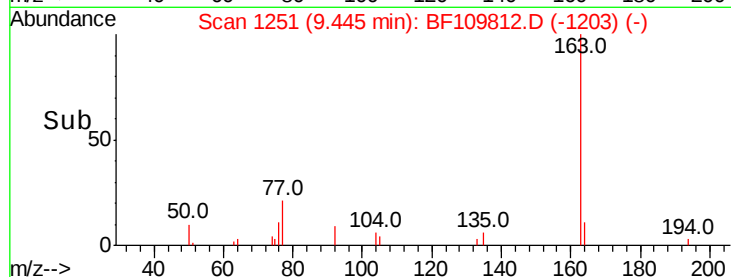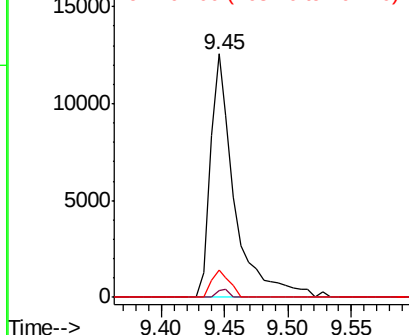

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.20 min Scan# 1549

Delta R.T. -0.01 min

Lab File: BF109812.D

Acq: 12 Oct 2018 3:51


Tgt Ion:188 Resp: 202180

Ion Ratio Lower Upper



188 100


94 8.8 7.2 10.8

80 9.6 7.9 11.9

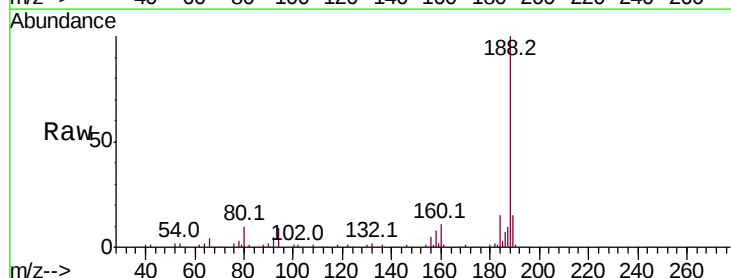

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

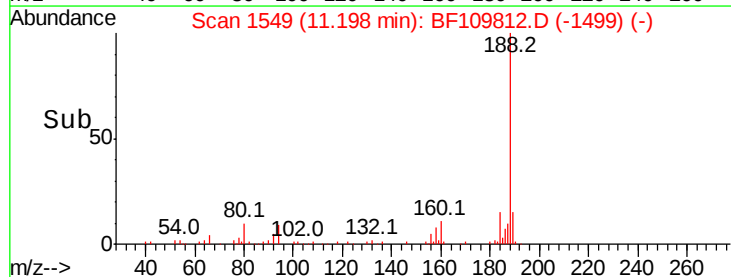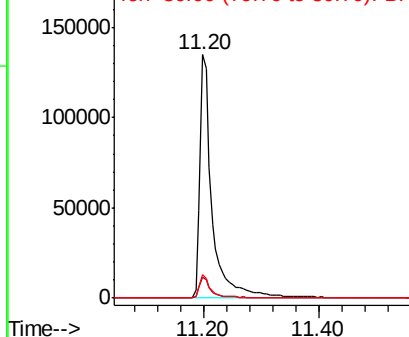

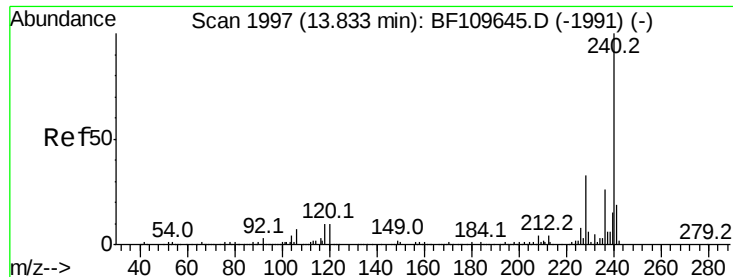

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.83 min Scan# 1996

Delta R.T. -0.01 min

Lab File: BF109812.D

Acq: 12 Oct 2018 3:51

Instrument :

BNA_F

ClientSampleID :

100418-JETT-E-U-S


Tot Ion:240 Resp: 228304

Ion Ratio Lower Upper

240 100

120 11.2 8.3 12.5




236 26.1 21.2 31.8

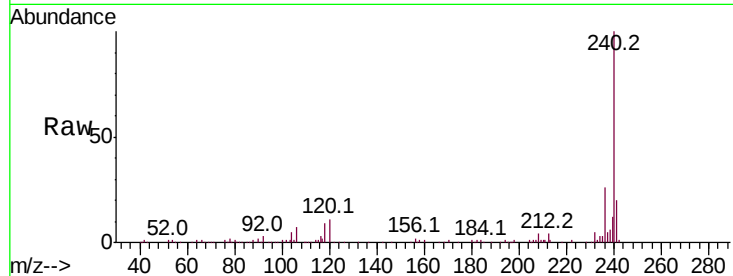

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

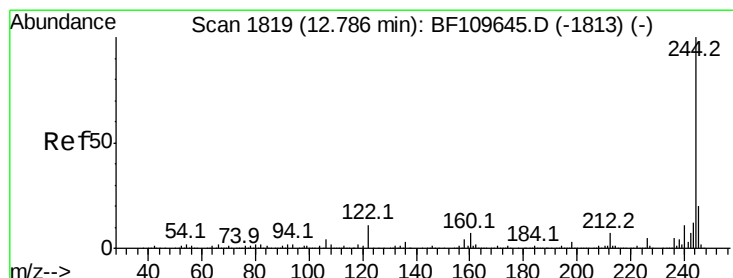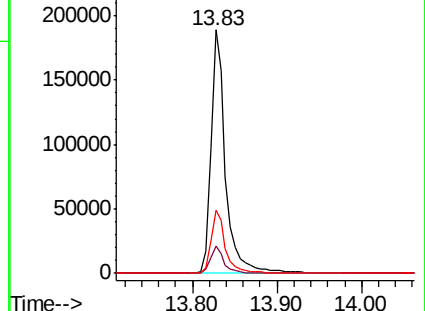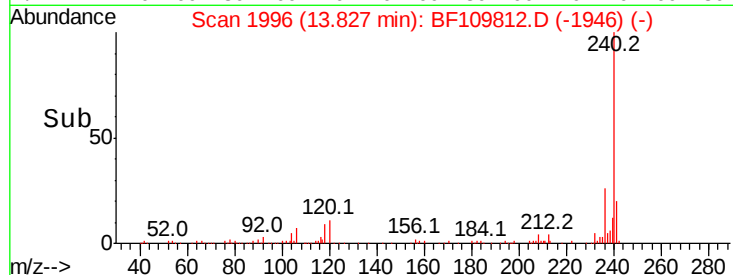

#78

Terphenyl-d14

Concen: 72.586 ng

RT: 12.78 min Scan# 1818

Delta R.T. -0.01 min

Lab File: BF109812.D

Acq: 12 Oct 2018 3:51


Tgt Ion:244 Resp: 856047

Ion Ratio Lower Upper

244 100

212 7.4 5.8 8.8



122 12.2 8.7 13.1

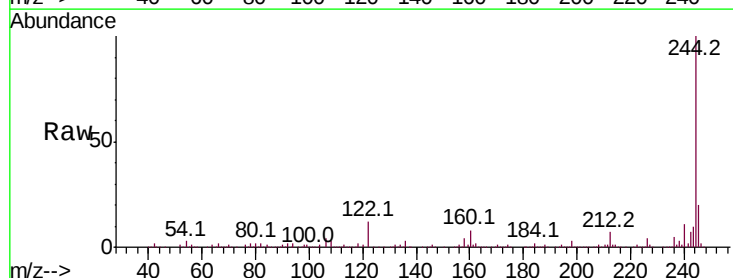


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

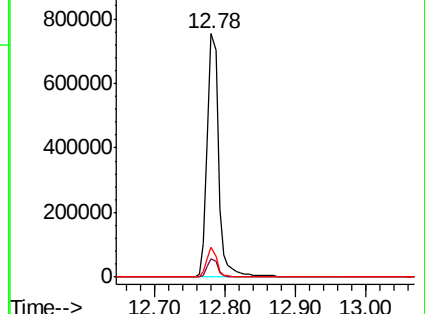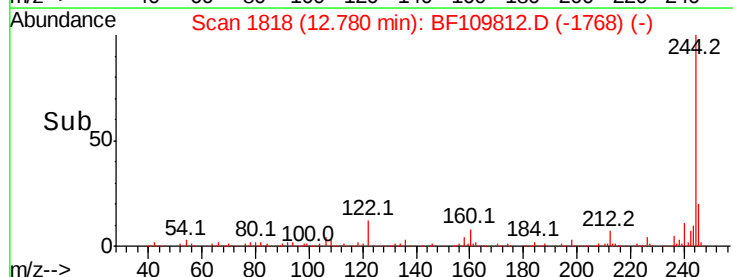

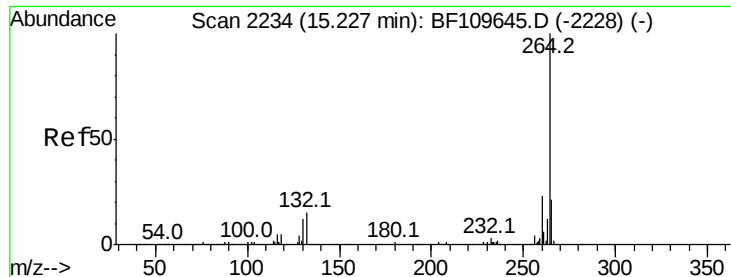

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.23 min Scan# 2234
Delta R.T. 0.00 min
Lab File: BF109812.D
Acq: 12 Oct 2018 3:51

Instrument :
BNA_F
ClientSampleId :
100418-JETT-E-U-S

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.4	18.7	28.1
265	21.3	16.7	25.1

