


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101118\
 Data File : BF109784.D
 Acq On : 11 Oct 2018 13:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 08 16:02:11 2018

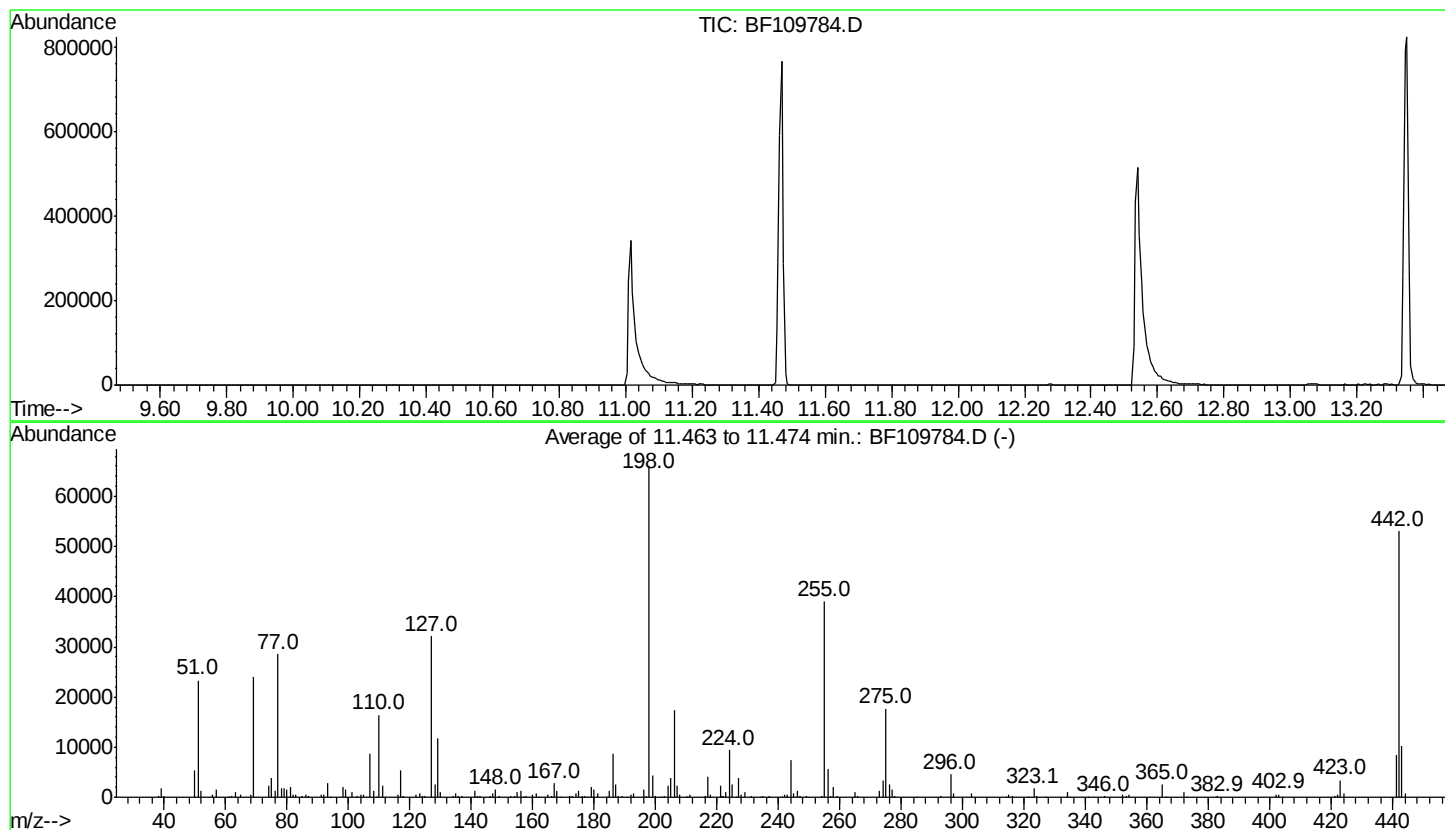

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	23245	PASS
68	69	0.00	2	1.7	404	PASS
69	198	0.00	100	36.4	24081	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.5	32048	PASS
197	198	0.00	2	0.5	320	PASS
198	198	100	100	100.0	66128	PASS
199	198	5	9	6.7	4430	PASS
275	198	10	60	26.6	17618	PASS
365	198	1	100	3.7	2475	PASS
441	198	0.01	100	12.9	8526	PASS
442	198	50	100	80.3	53074	PASS
443	442	15	24	19.1	10123	PASS