

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101122\
 Data File : BF130619.D
 Acq On : 11 Oct 2022 15:30
 Operator : CG\JU
 Sample : PB148225BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB148225BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.793	457	460	469	rBV	28028	41412	1.16%	0.206%
2	5.198	524	529	548	rBV	2255542	2364185	65.97%	11.733%
3	6.234	700	705	708	rBV	2148026	2327464	64.94%	11.551%
4	6.587	761	765	776	rVB	713111	572820	15.98%	2.843%
5	7.157	857	862	865	rBV	1630001	1544549	43.10%	7.665%
6	7.869	978	983	986	rBV	859131	779623	21.75%	3.869%
7	8.945	1160	1166	1169	rBV	3310117	3180390	88.74%	15.783%
8	9.616	1275	1280	1283	rBV	1167100	921555	25.71%	4.573%
9	10.404	1410	1414	1418	rBV	2139462	2059038	57.45%	10.218%
10	11.092	1528	1531	1535	rBV	1059886	969482	27.05%	4.811%
11	12.686	1797	1802	1805	rBV	4032435	3583951	100.00%	17.786%
12	13.727	1975	1979	1982	rBV	912858	832505	23.23%	4.131%
13	15.098	2208	2212	2216	rBV	620033	659850	18.41%	3.275%
14	15.504	2276	2281	2286	rBV	40243	60237	1.68%	0.299%
15	15.586	2287	2295	2296	rBV3	25352	45431	1.27%	0.225%
16	15.939	2350	2355	2362	rVB2	38035	62087	1.73%	0.308%
17	16.451	2436	2442	2449	rVB3	27685	53447	1.49%	0.265%
18	17.045	2536	2543	2553	rBV3	23054	52415	1.46%	0.260%
19	17.756	2656	2664	2671	rBV4	15744	39764	1.11%	0.197%




Sum of corrected areas: 20150205

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101122\
Data File : BF130619.D
Acq On : 11 Oct 2022 15:30
Operator : CG\JU
Sample : PB148225BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148225BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

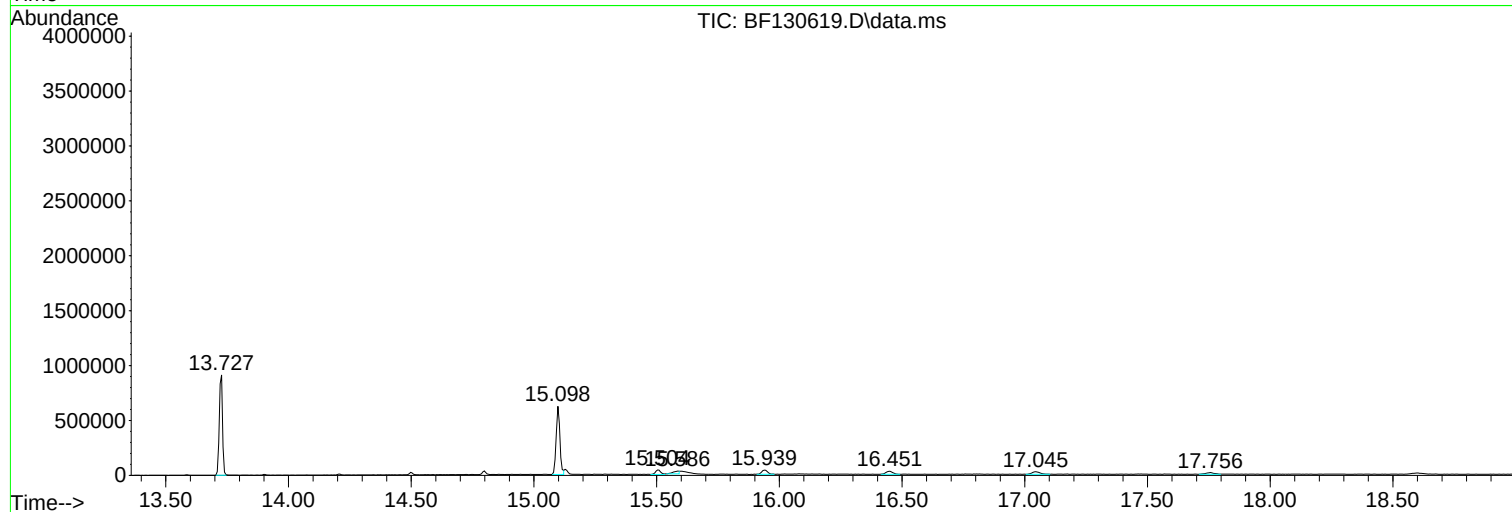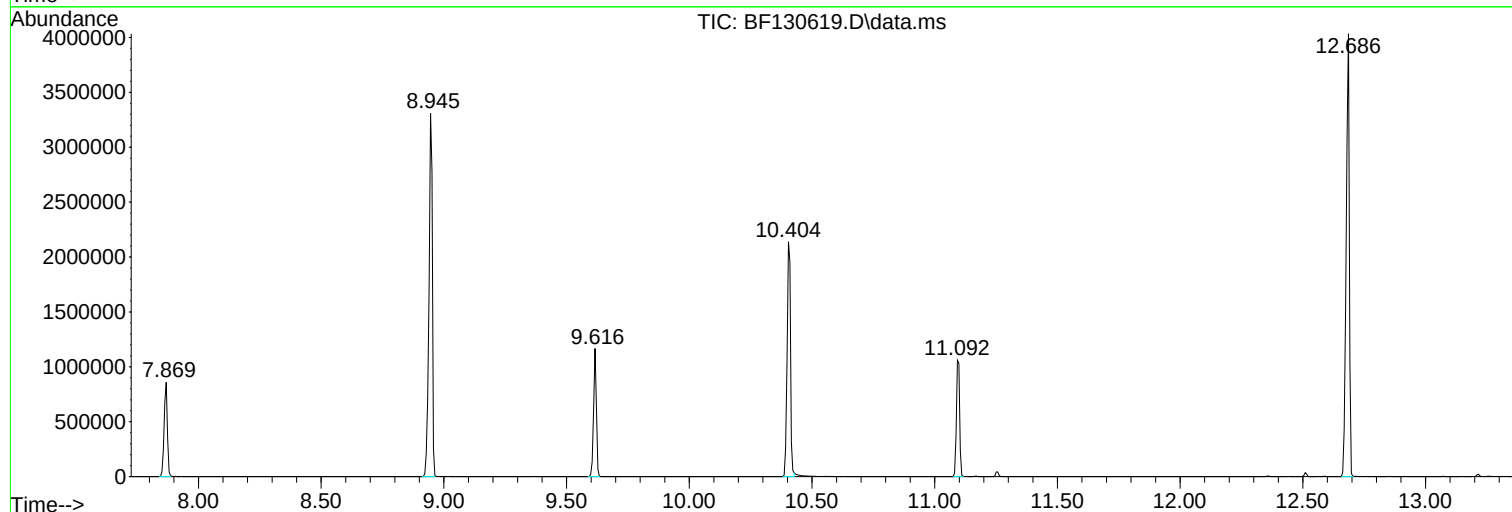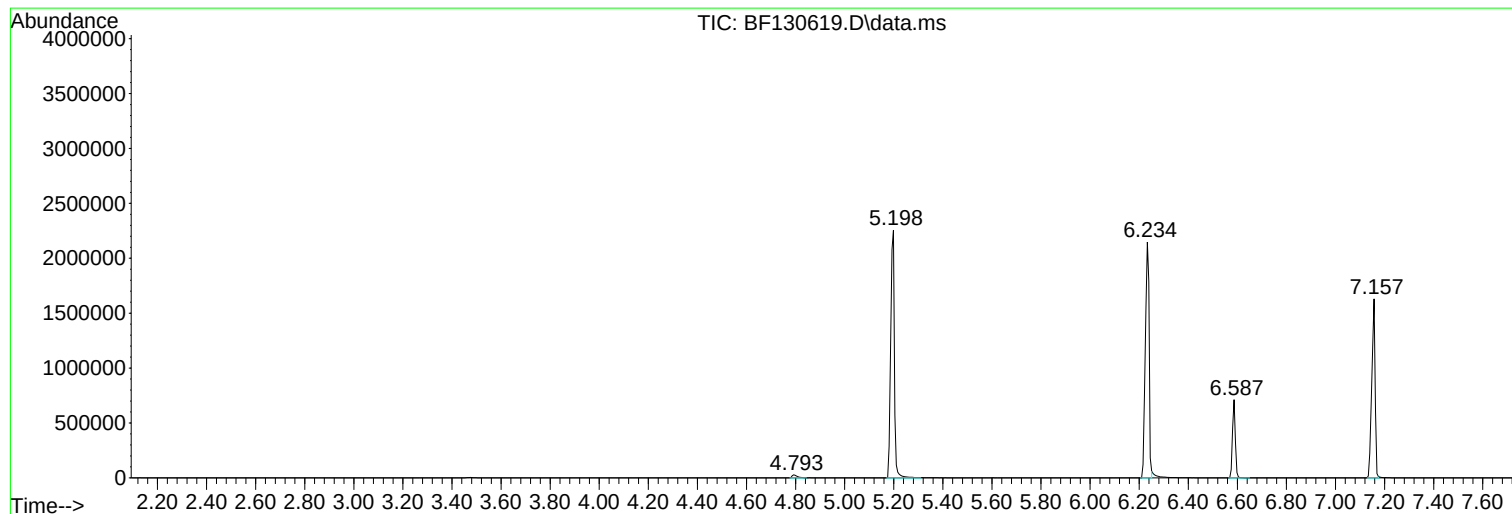

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101122\
Data File : BF130619.D
Acq On : 11 Oct 2022 15:30
Operator : CG\JU
Sample : PB148225BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148225BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101122\
Data File : BF130619.D
Acq On : 11 Oct 2022 15:30
Operator : CG\JU
Sample : PB148225BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148225BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------