
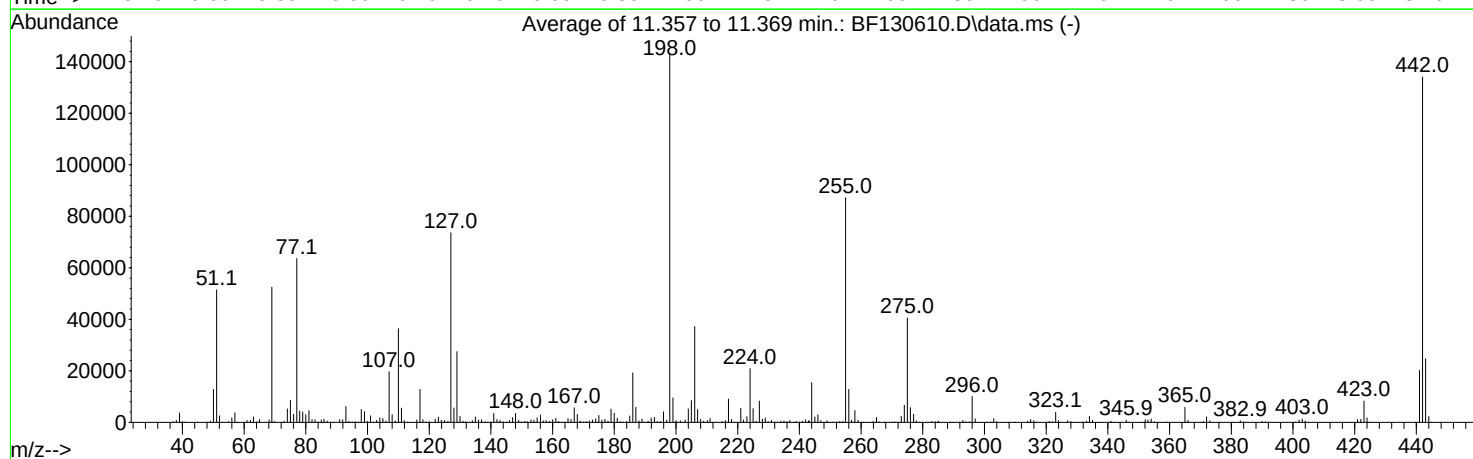


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101122\
 Data File : BF130610.D
 Acq On : 11 Oct 2022 10:07
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 12 06:52:52 2022

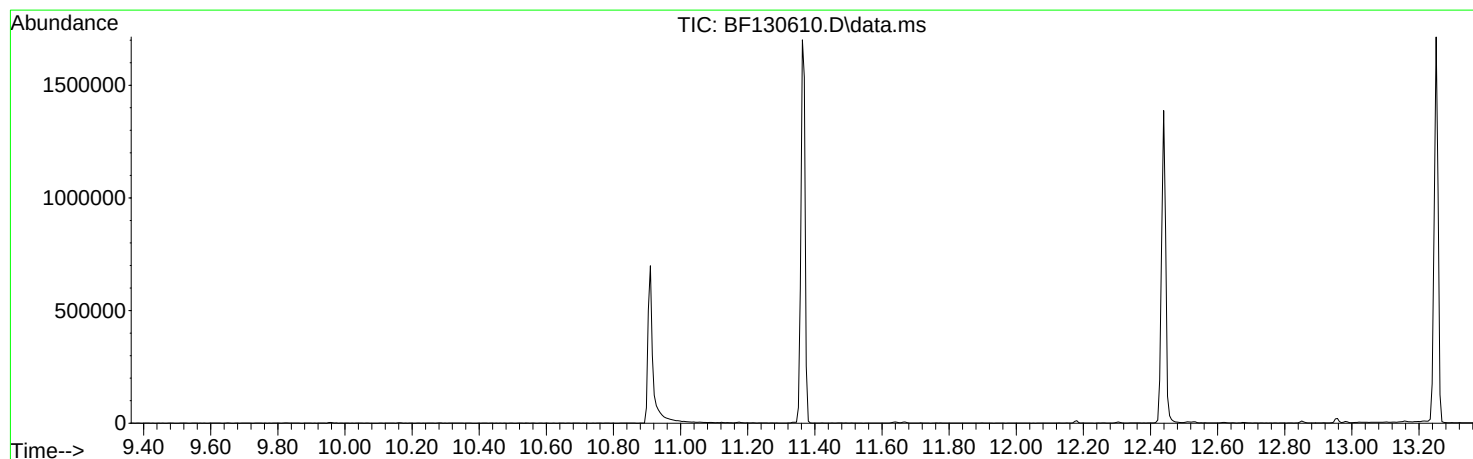




AutoFind: Scans 1576, 1577, 1578; Background Corrected with Scan 1571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	51411	PASS
68	69	0.00	2	1.9	993	PASS
69	198	0.00	100	36.7	52464	PASS
70	69	0.00	2	0.6	318	PASS
127	198	10	80	51.5	73608	PASS
197	198	0.00	2	0.7	961	PASS
198	198	100	100	100.0	142813	PASS
199	198	5	9	6.7	9508	PASS
275	198	10	60	28.4	40514	PASS
365	198	1	100	4.1	5873	PASS
441	198	0.01	100	14.2	20217	PASS
442	442	50	100	100.0	134040	PASS
443	442	15	24	18.4	24708	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101122\
 Data File : BF130610.D
 Acq On : 11 Oct 2022 10:07
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 12 07:47:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 12 06:52:52 2022
 Response via : Initial Calibration

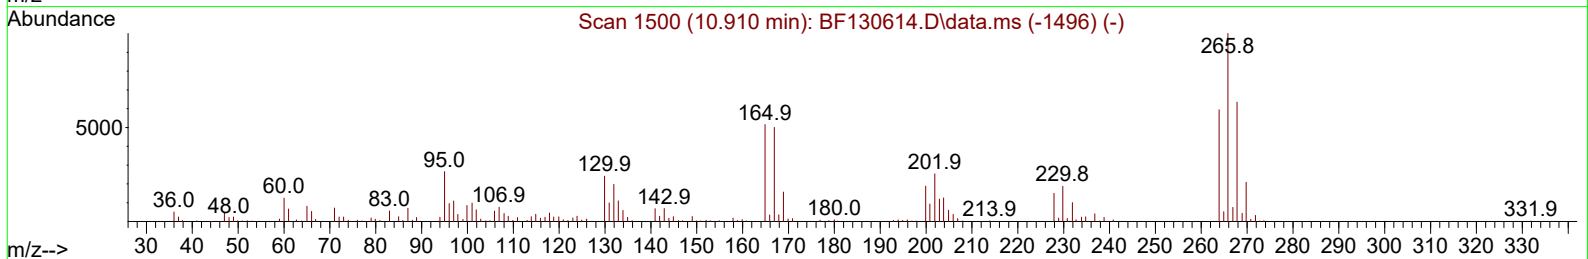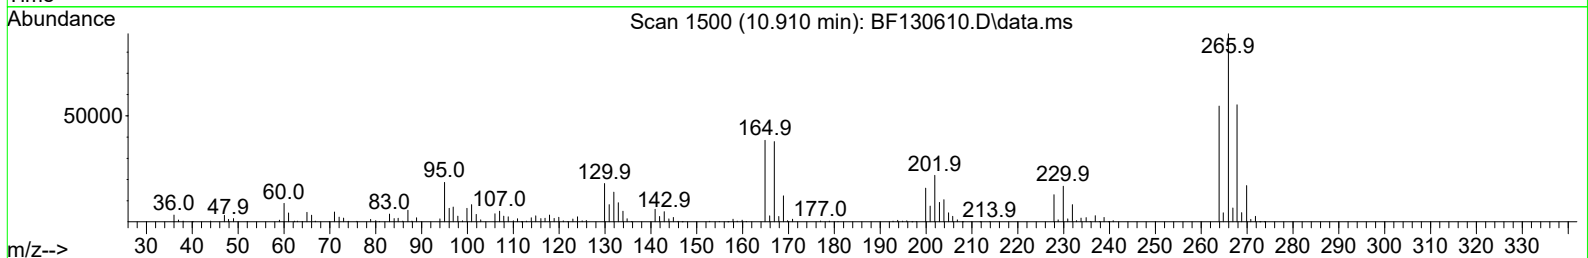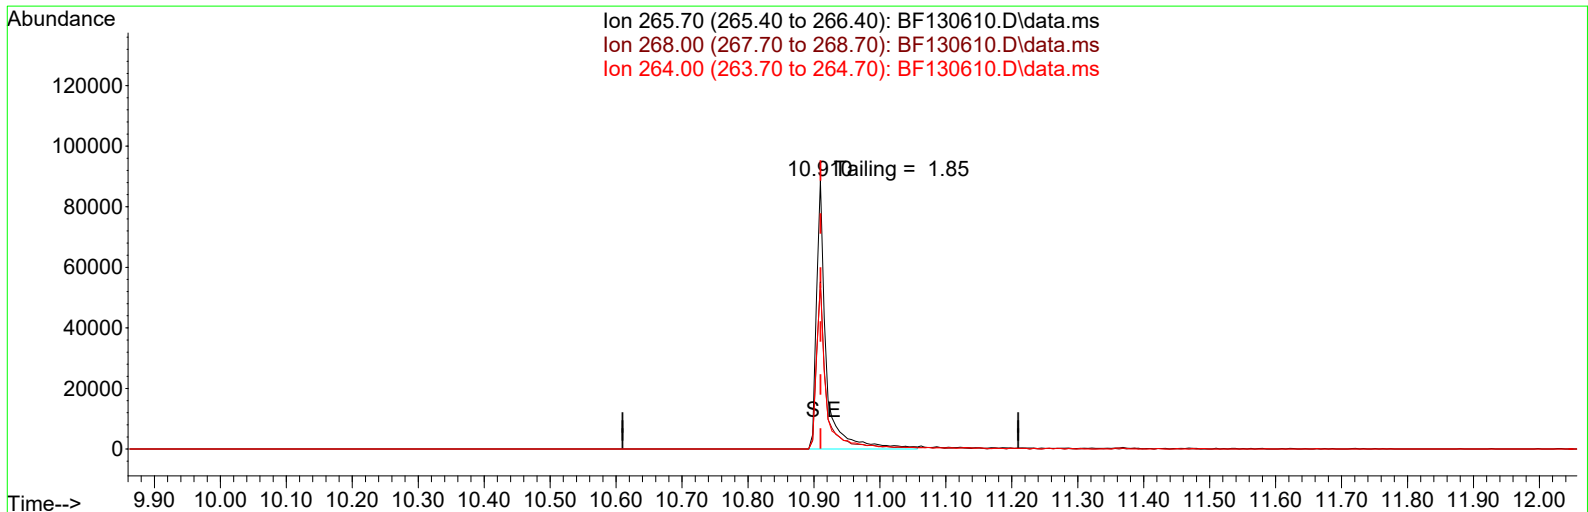

TIC: BF130610.D\data.ms

(70) Pentachlorophenol (C)

10.910min (-0.000) 261057.87 ng




response 92270

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	62.28
264.00	59.40	61.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101122\
Data File : BF130610.D
Acq On : 11 Oct 2022 10:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 12 07:47:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 12 06:52:52 2022
Response via : Initial Calibration

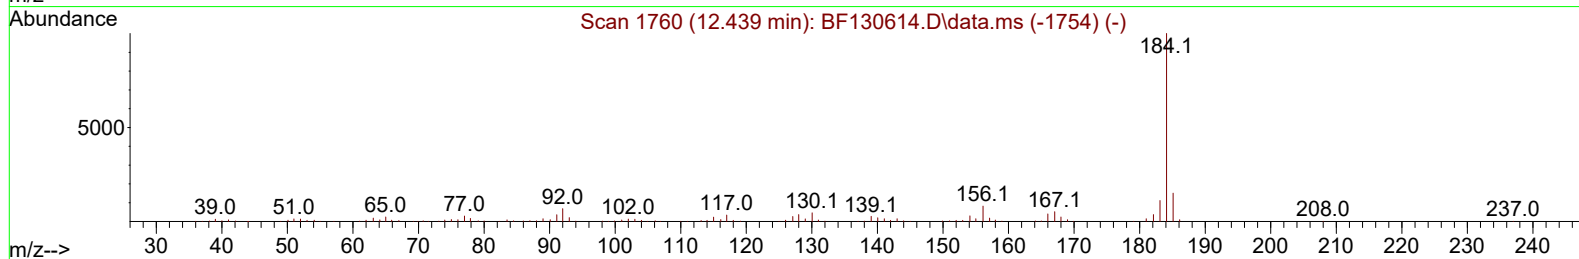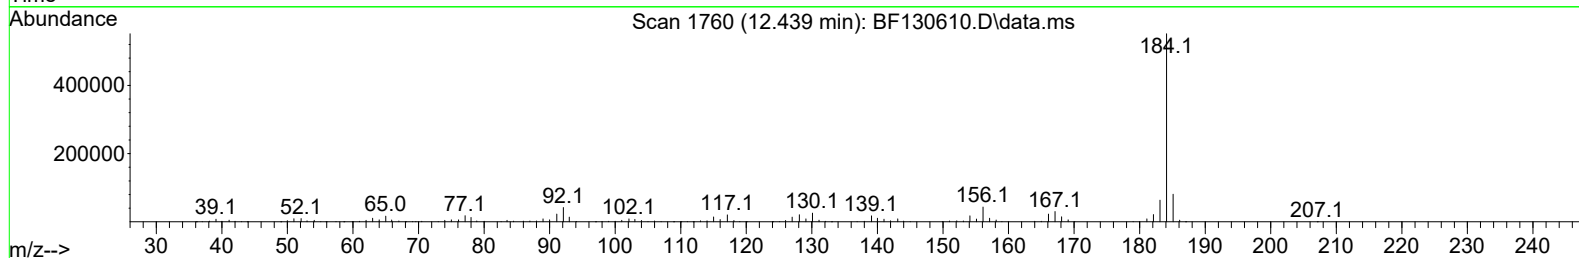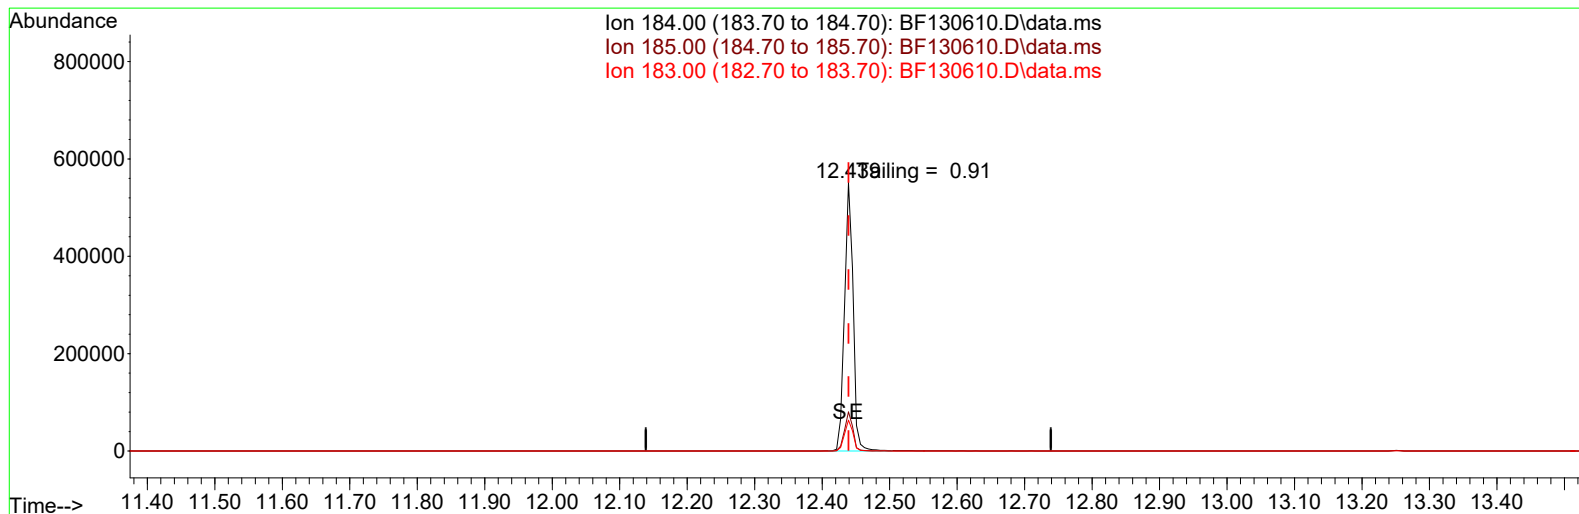

TIC: BF130610.D\data.ms

(77) Benzidine

12.439min (0.000) 121477.35 ng

response 491280

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.65
183.00	11.20	11.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/11/2022	BNA_F	<u>BF130610.D</u>
Compound Name	Response	Retention Time
DDT	269089	13.251
DDD	5798	12.957
DDE	734	12.616
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6532	275621	2.37

Instrument :
BNA_F
ClientSampleId :
DFTPP