


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101124\
Data File : BF139762.D
Acq On : 11 Oct 2024 09:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 02 04:58:47 2024

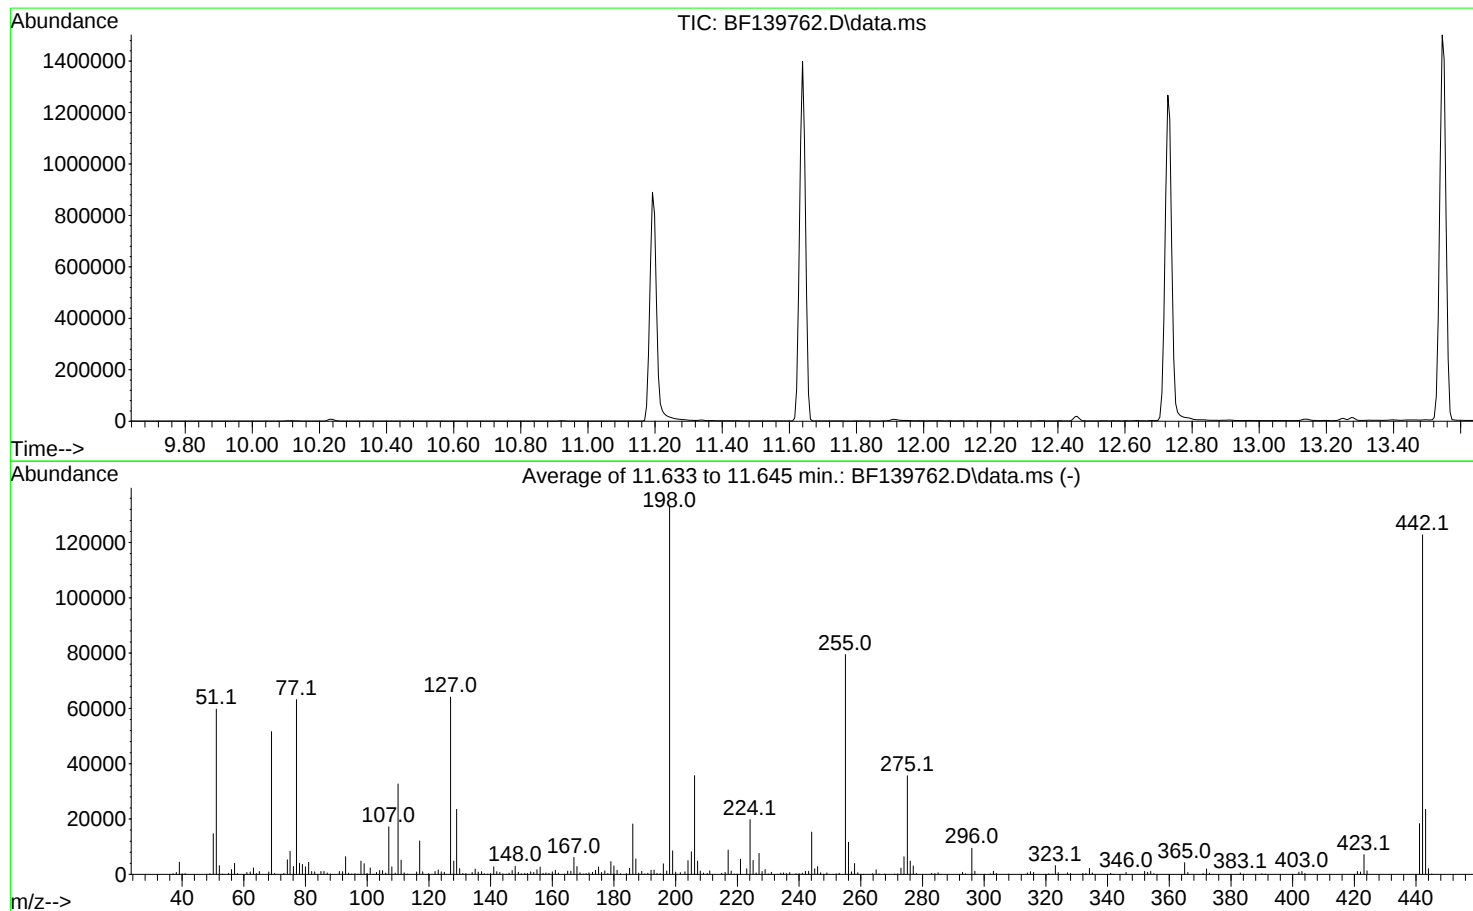




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	59749	PASS
68	69	0.00	2	1.7	901	PASS
69	198	0.00	100	38.8	51587	PASS
70	69	0.00	2	0.7	341	PASS
127	198	10	80	48.2	64091	PASS
197	198	0.00	2	0.9	1196	PASS
198	198	100	100	100.0	133021	PASS
199	198	5	9	6.4	8511	PASS
275	198	10	60	26.8	35621	PASS
365	198	1	100	3.2	4228	PASS
441	198	0.01	100	13.8	18361	PASS
442	442	50	100	100.0	122760	PASS
443	442	15	24	19.2	23525	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101124\
Data File : BF139762.D
Acq On : 11 Oct 2024 09:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 11 12:36:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

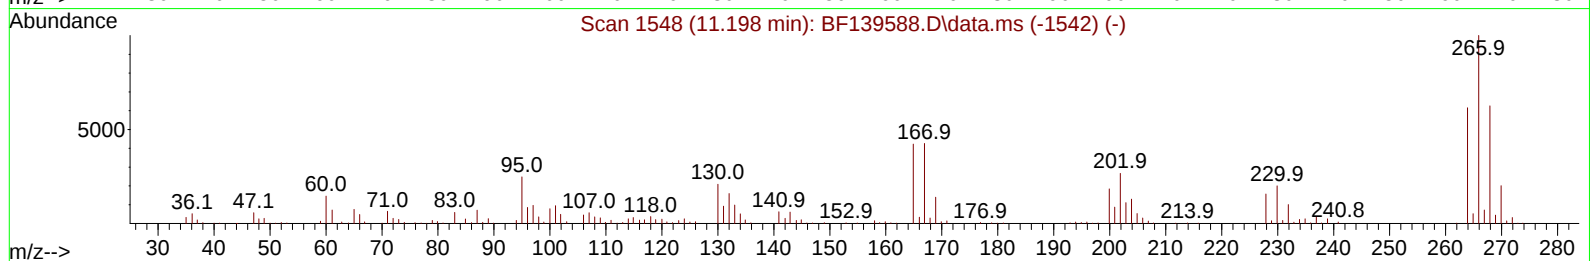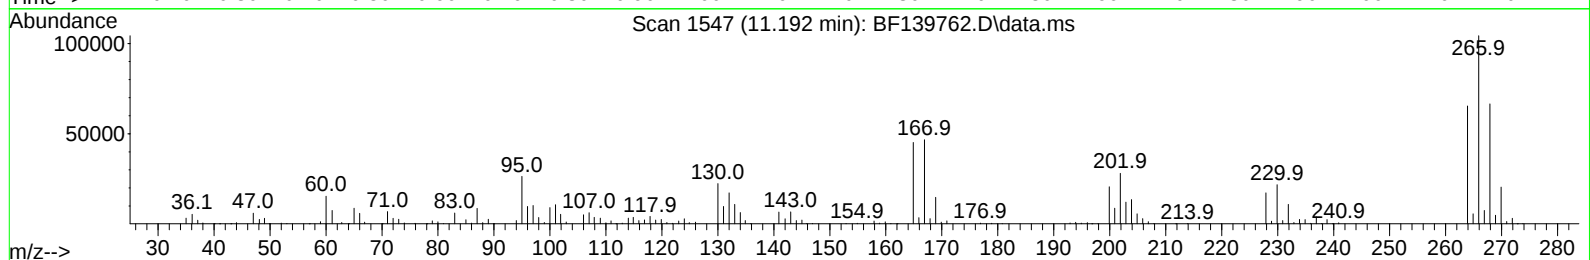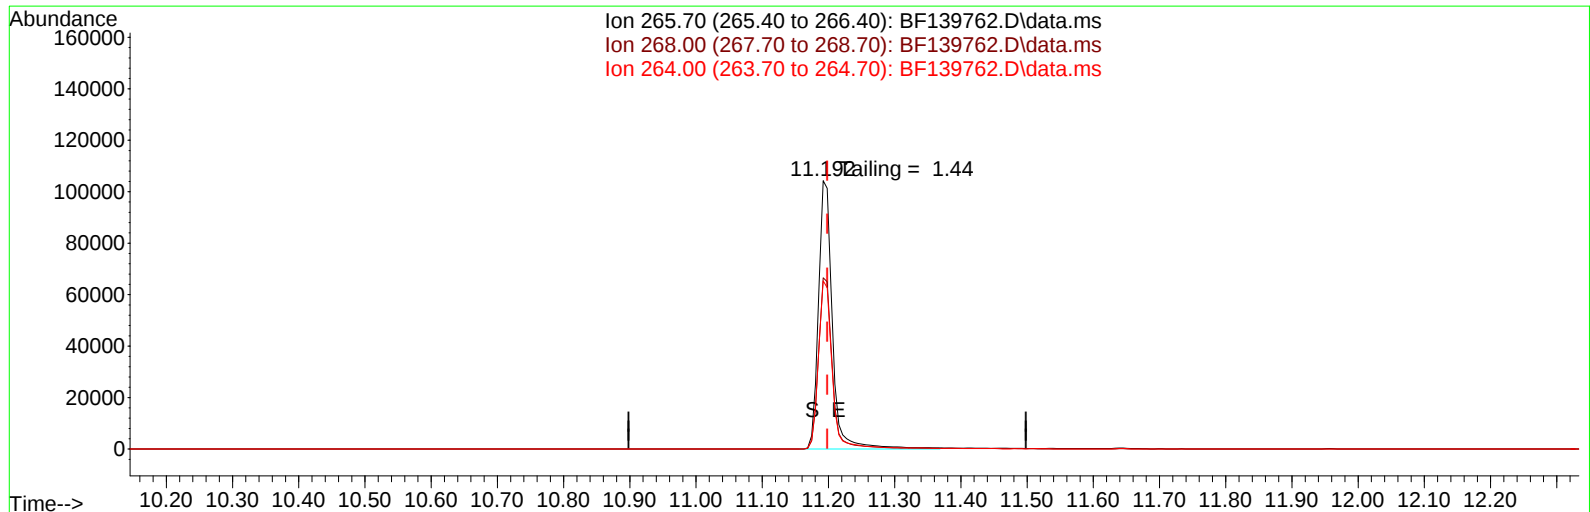

TIC: BF139762.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 351901.64 ng




response 152575

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	63.78
264.00	61.60	62.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101124\
Data File : BF139762.D
Acq On : 11 Oct 2024 09:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 11 12:36:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

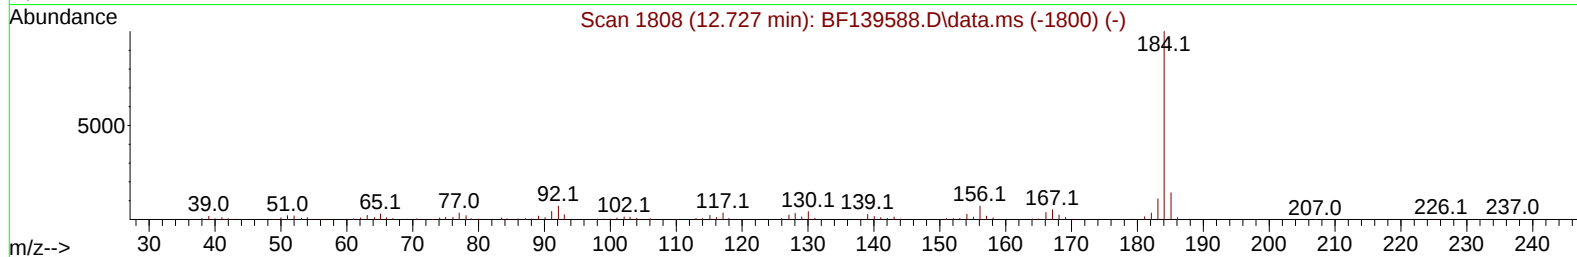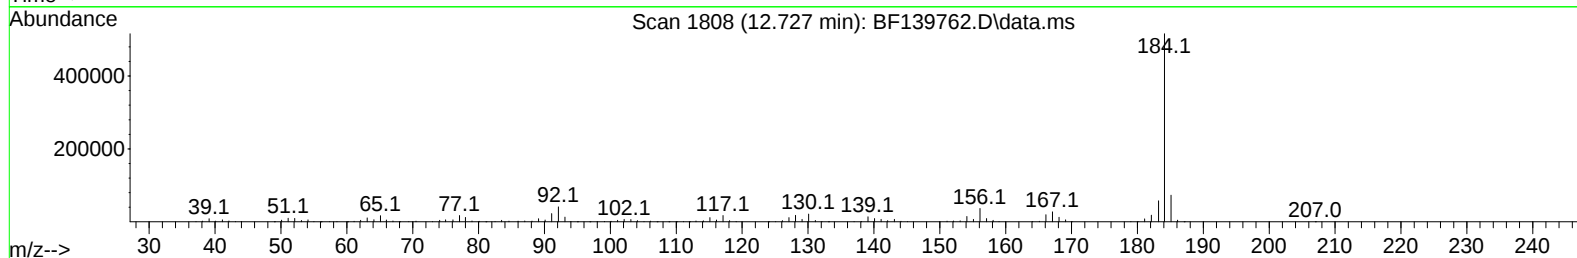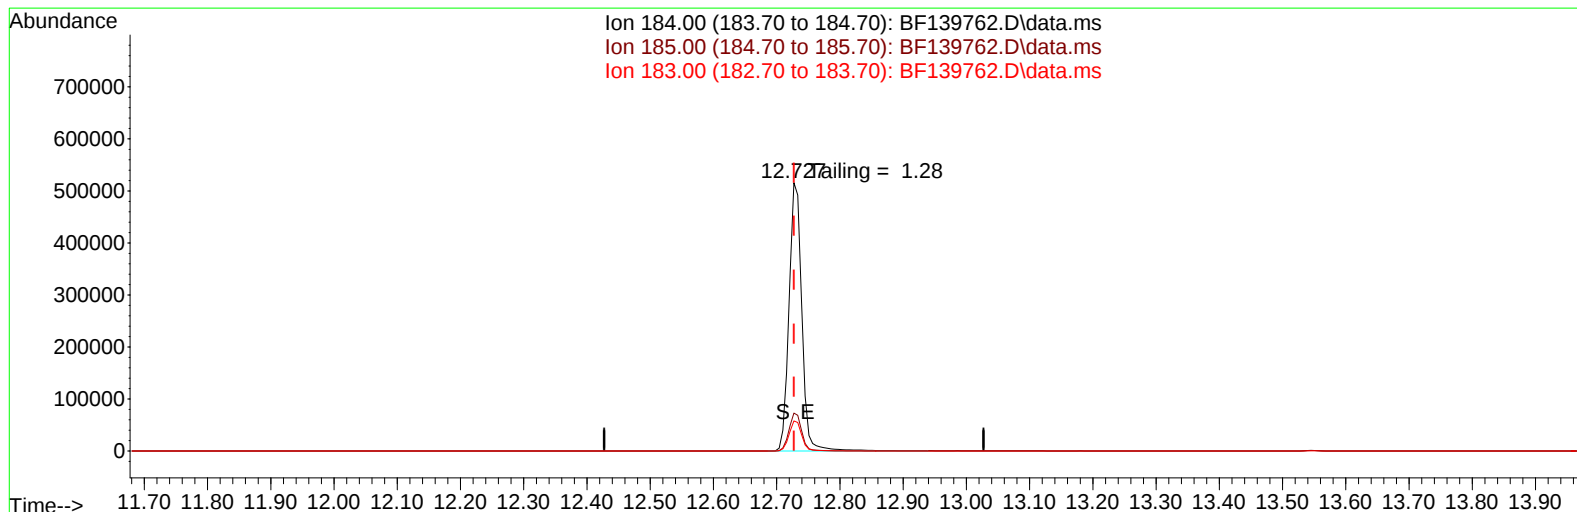

TIC: BF139762.D\data.ms

(77) Benzidine

12.727min (-0.000) 765669.40 ng

response 729297

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.15
183.00	11.00	11.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/11/2024	BNA_F	<u>BF139762.D</u>
Compound Name	Response	Retention Time
DDT	380349	13.545
DDD	6681	13.28
DDE	758	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7439	387788	1.92

Instrument :
BNA_F
ClientSampleId :
DFTPP