
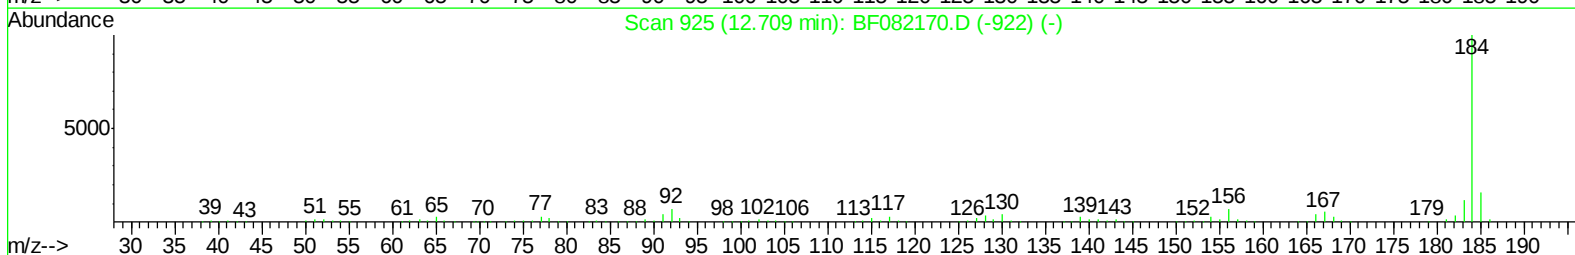
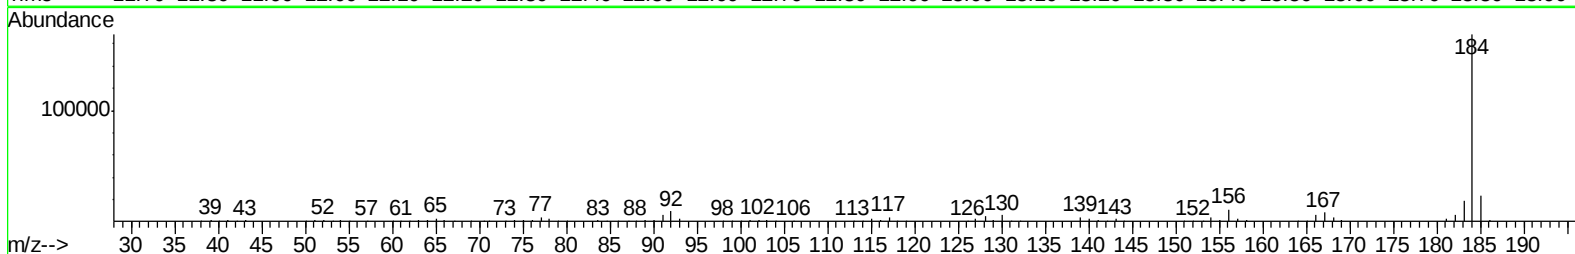


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101215\
 Data File : BF082216.D
 Acq On : 12 Oct 2015 11:38
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 02:56:20 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 13 02:05:16 2015
 Response via : Initial Calibration

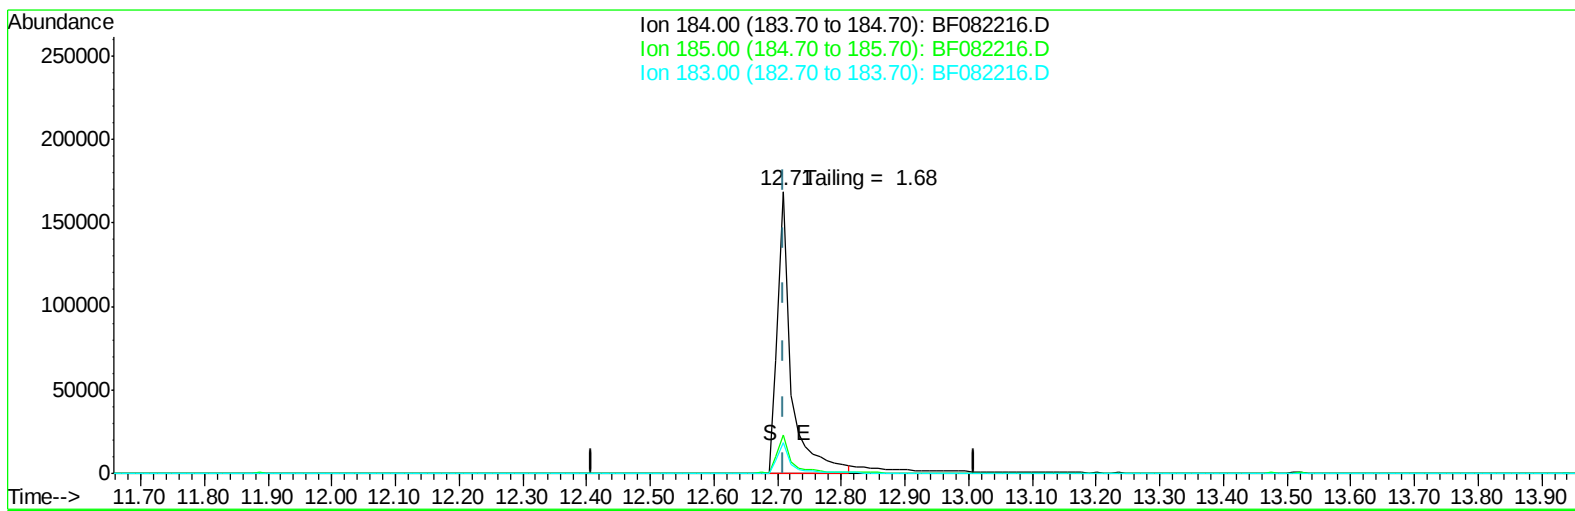

TIC: BF082216.D

(76) Benzidine




12.709min (-0.000) 0.00ng

response 273704

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	13.80
183.00	11.40	11.11
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101215\
Data File : BF082216.D
Acq On : 12 Oct 2015 11:38
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 02:56:20 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 13 02:05:16 2015
Response via : Initial Calibration

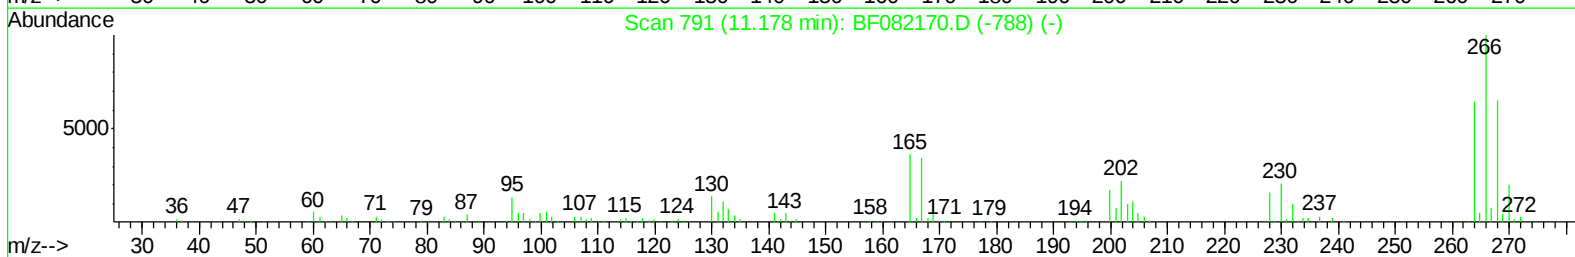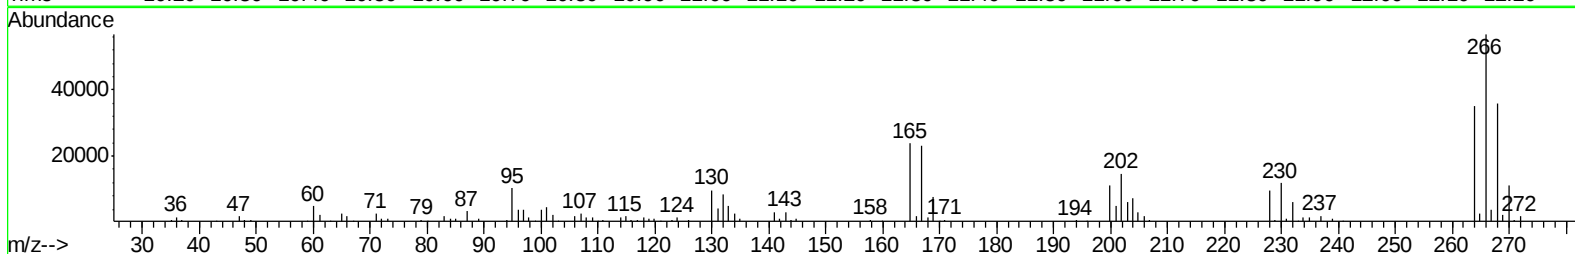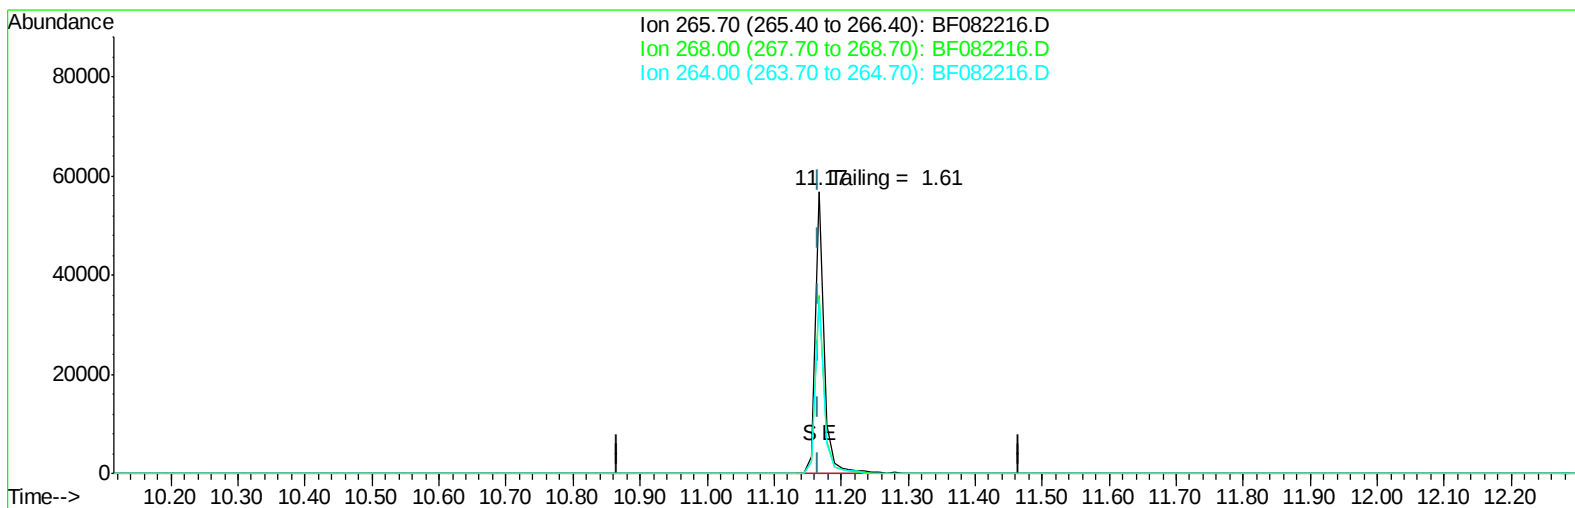

TIC: BF082216.D

(69) Pentachlorophenol (C)

11.166min (-0.000) 0.00ng

response 52151

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.22
264.00	64.20	61.81
0.00	0.00	0.00