

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101216\
 Data File : U3S6.D
 Acq On : 12 Oct 2016 22:27
 Operator : UM/SJ
 Sample : U3S6
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Oct 13 00:54:56 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 16:14:43 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	194641	20.00	ng	0.00
21) Naphthalene-d8	8.23	136	838685	20.00	ng	-0.01
38) Acenaphthene-d10	9.99	164	438975	20.00	ng	-0.01
63) Phenanthrene-d10	11.48	188	765790	20.00	ng	0.00
75) Chrysene-d12	14.12	240	575034	20.00	ng	-0.01
86) Perylene-d12	15.60	264	389025	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.57	112	1595340	127.51	ng	0.01
7) Phenol-d6	6.59	99	2137940	135.41	ng	0.00
23) Nitrobenzene-d5	7.51	82	1342679	86.83	ng	0.00
41) 2,4,6-Tribromophenol	10.78	330	567363	130.38	ng	-0.01
44) 2-Fluorobiphenyl	9.31	172	2380388	91.13	ng	-0.01
78) Terphenyl-d14	13.07	244	2372773	100.84	ng	-0.01


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101216\
Data File : U3S6.D
Acq On : 12 Oct 2016 22:27
Operator : UM/SJ
Sample : U3S6
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Oct 13 00:54:56 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 16:14:43 2016
Response via : Initial Calibration

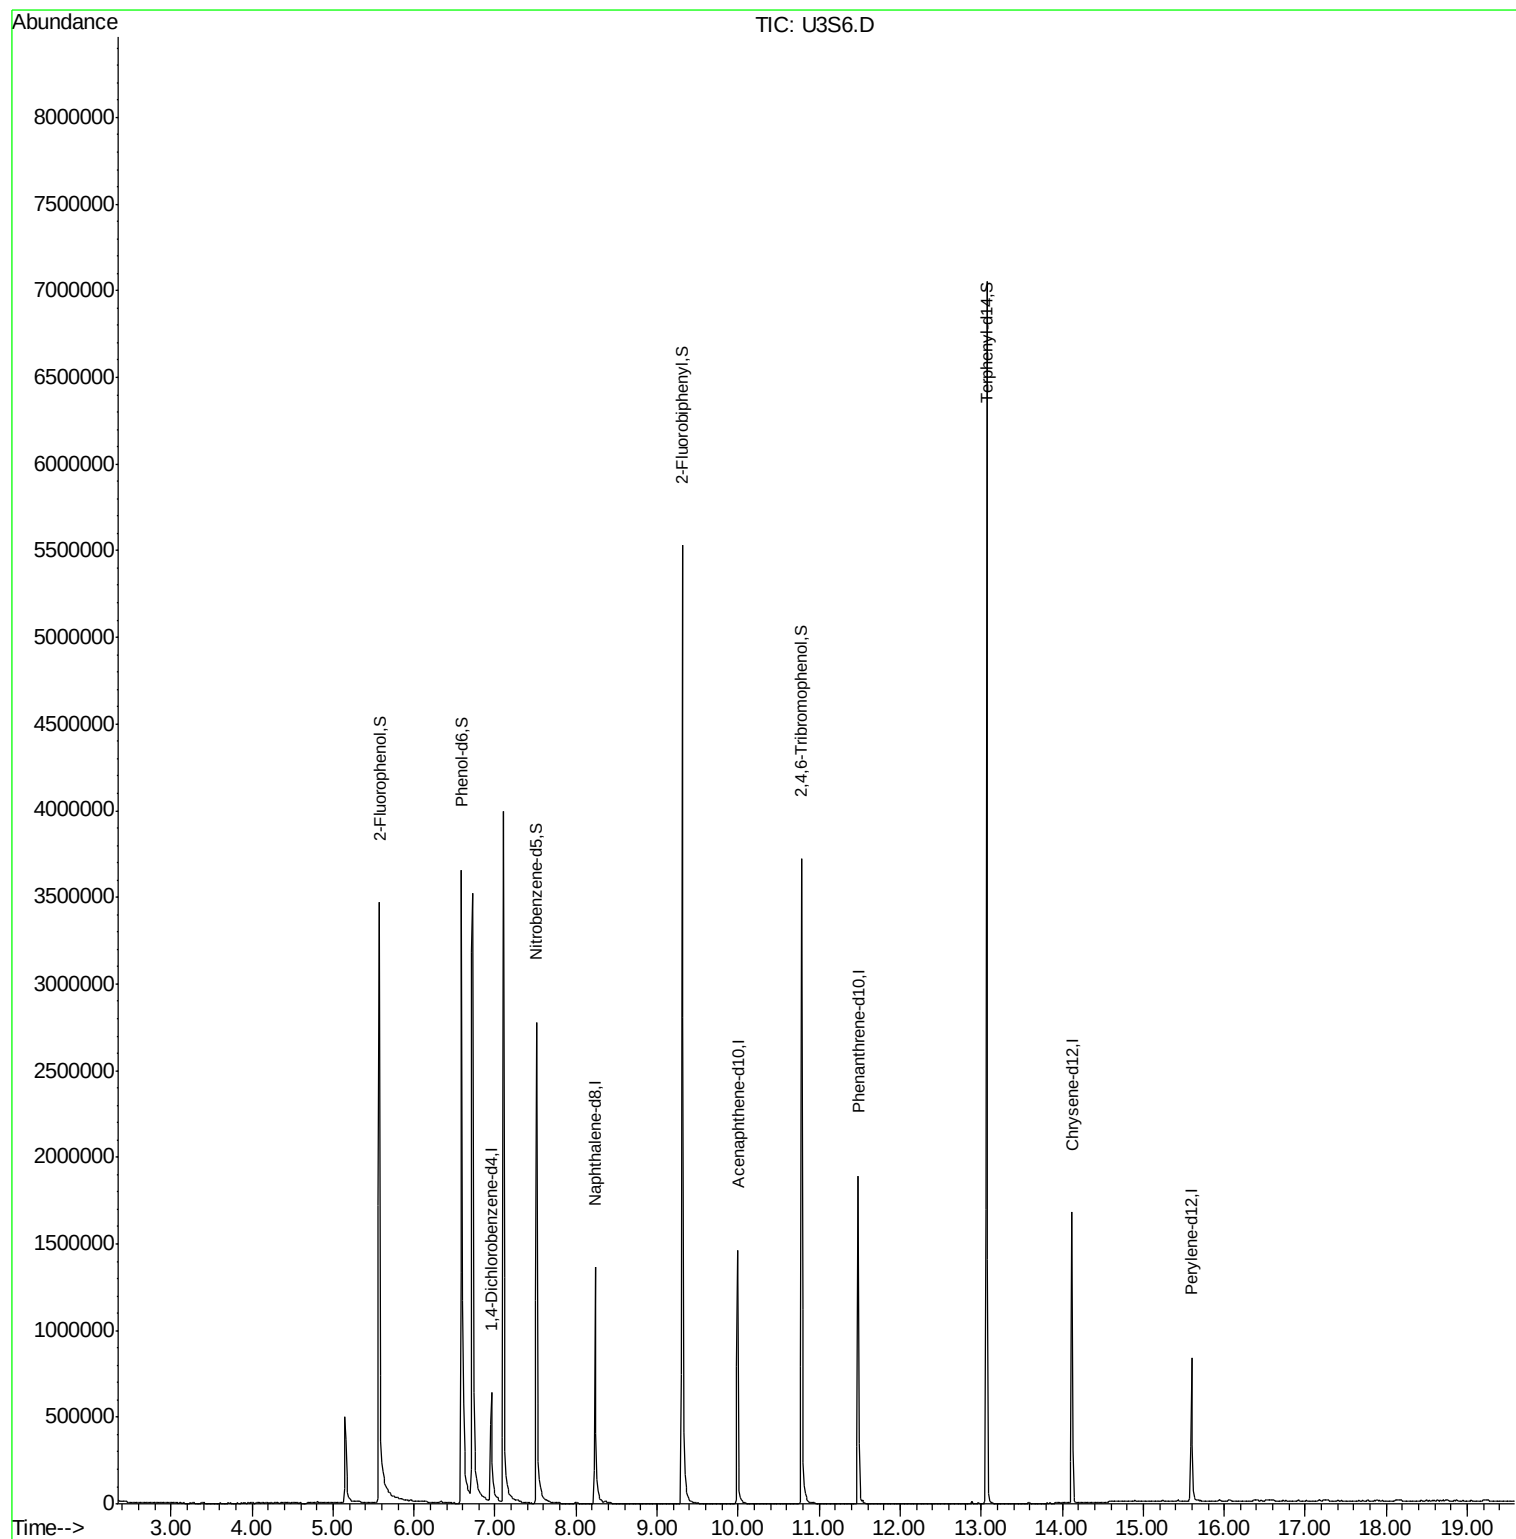

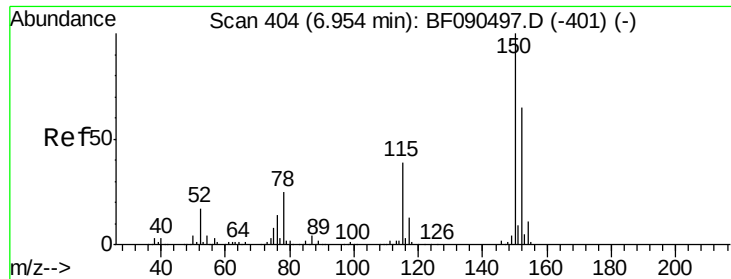


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.95 min Scan# 404
Delta R.T. -0.00 min
Lab File: U3S6.D
Acq: 12 Oct 2016 22:27

Instrument :
BNA_F
ClientSampleId :

Tgt Ion	Ratio	Lower	Upper
152	100		
150	155.5	124.6	186.8
115	55.5	46.2	69.4

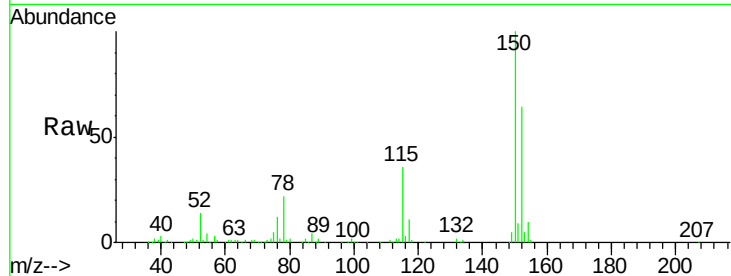


Abundance Ion 152.00 (151.70 to 152.70): U
Ion 150.00 (149.70 to 150.70): U
Ion 115.00 (114.70 to 115.70): U

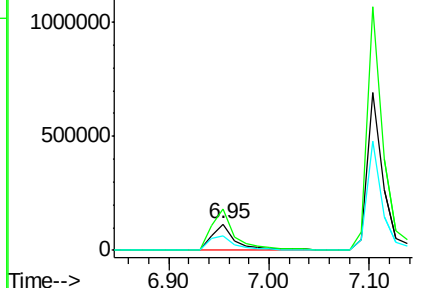



#5




2-Fluorophenol
Concen: 127.51 ng
RT: 5.57 min Scan# 283
Delta R.T. 0.01 min
Lab File: U3S6.D
Acq: 12 Oct 2016 22:27

Tgt Ion	Ratio	Lower	Upper
112	100		
64	52.7	57.9	86.9#
63	26.1	29.6	44.4#



Abundance Ion 112.00 (111.70 to 112.70): U
Ion 64.00 (63.70 to 64.70): U3S
Ion 63.00 (62.70 to 63.70): U3S

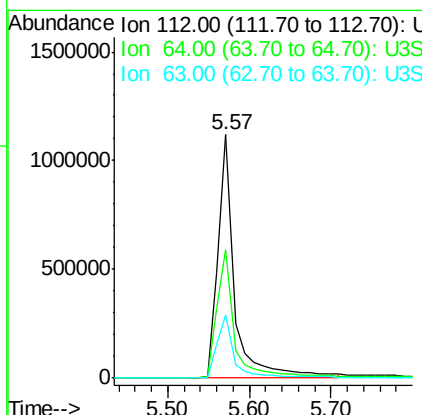

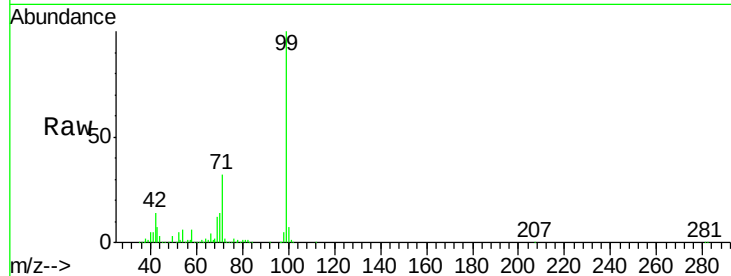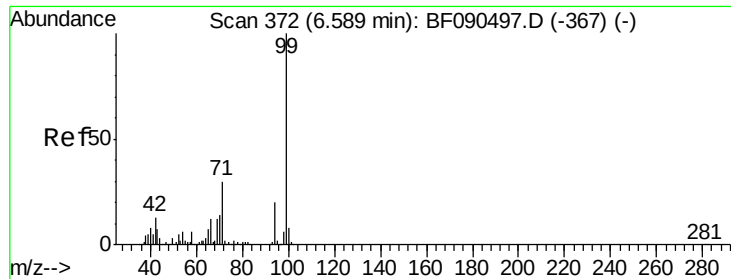

#7

Phenol-d6

Concen: 135.41 ng

RT: 6.59 min Scan# 372

Delta R.T. -0.00 min

Lab File: U3S6.D

Acq: 12 Oct 2016 22:27

Instrument :

BNA_F

ClientSampleId :





Tgt Ion: 99 Resp: 2137940

Ion Ratio Lower Upper

99 100

42 13.8 20.0 30.0#

71 32.0 27.9 41.9

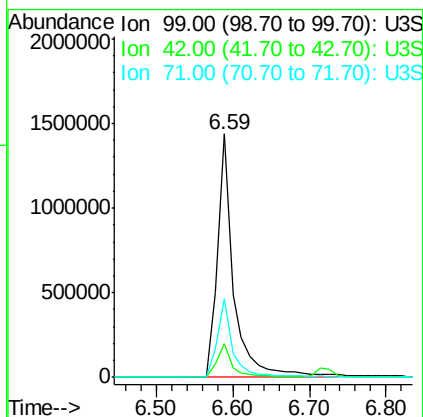

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.23 min Scan# 516

Delta R.T. -0.01 min

Lab File: U3S6.D

Acq: 12 Oct 2016 22:27

Tgt Ion: 136 Resp: 838685


Ion Ratio Lower Upper


136 100

137 11.1 9.0 13.6

54 7.2 6.6 10.0

68 6.7 5.0 7.6

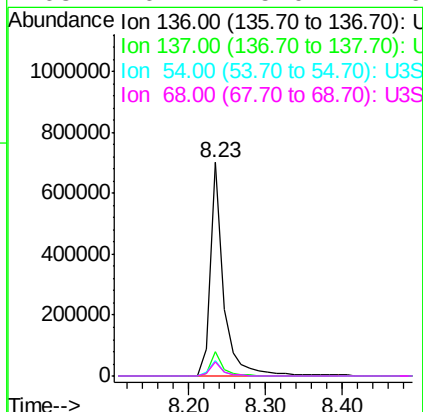



#23

Nitrobenzene-d5

Concen: 86.83 ng

RT: 7.51 min Scan# 453

Delta R.T. -0.00 min


Lab File: U3S6.D

Acq: 12 Oct 2016 22:27

Instrument :
BNA_F
ClientSampleId :

Tgt Ion: 82 Resp: 1342679




Ion	Ratio	Lower	Upper
82	100		
128	49.5	40.0	60.0
54	41.2	42.6	64.0

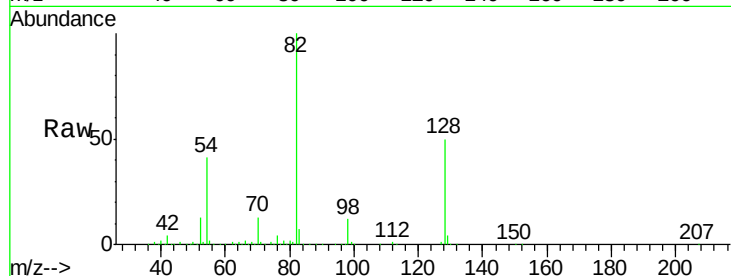

Abundance Ion 82.00 (81.70 to 82.70): U3S6.D (-436) (-)

Ion 128.00 (127.70 to 128.70): U3S6.D (-436) (-)

Ion 54.00 (53.70 to 54.70): U3S6.D (-436) (-)

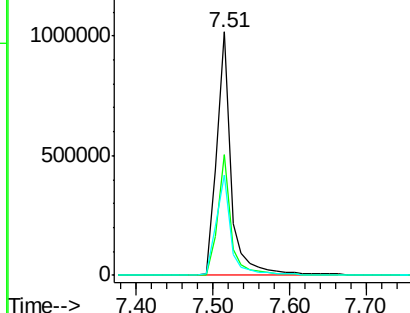

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.99 min Scan# 670


Delta R.T. -0.01 min

Lab File: U3S6.D

Acq: 12 Oct 2016 22:27

Tgt Ion: 164 Resp: 438975



Ion	Ratio	Lower	Upper
164	100		
162	103.1	80.1	120.1
160	45.9	36.3	54.5




Abundance Ion 164.00 (163.70 to 164.70): U3S6.D (-654) (-)

Ion 162.00 (161.70 to 162.70): U3S6.D (-654) (-)

Ion 160.00 (159.70 to 160.70): U3S6.D (-654) (-)



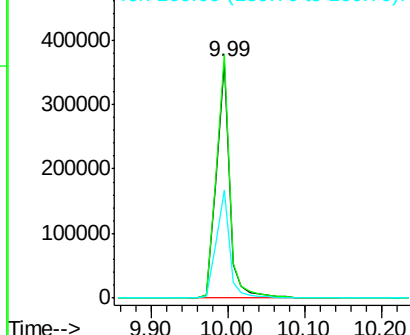



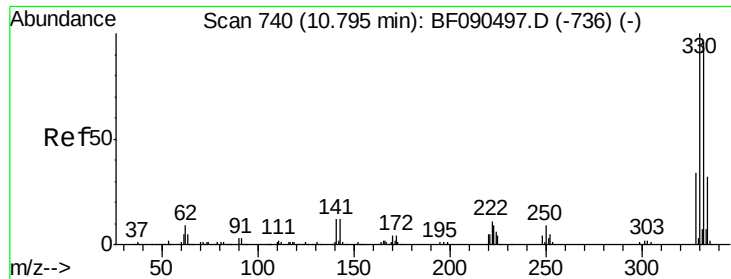

#41
 2,4,6-Tribromophenol
 Concen: 130.38 ng
 RT: 10.78 min Scan# 739
 Delta R.T. -0.01 min
 Lab File: U3S6.D
 Acq: 12 Oct 2016 22:27




Instrument :
 BNA_F
 ClientSampled :


Tgt Ion:330 Resp: 567363
 Ion Ratio Lower Upper
 330 100
 332 95.6 75.4 113.0
 141 33.9 26.9 40.3

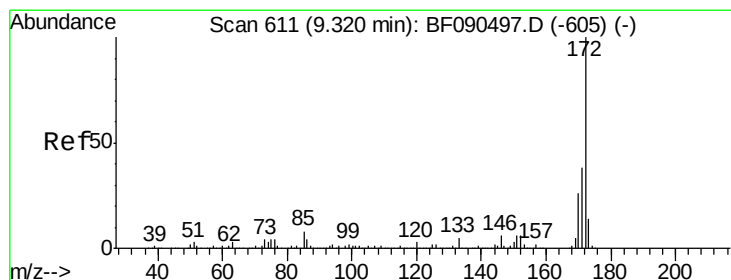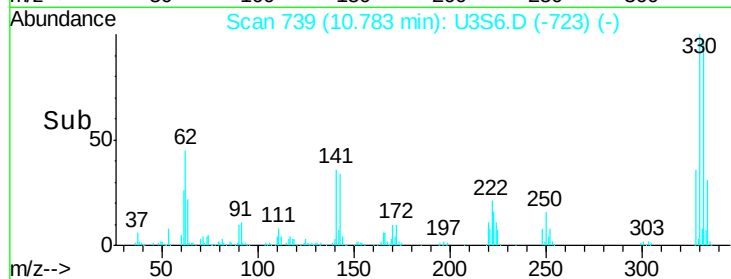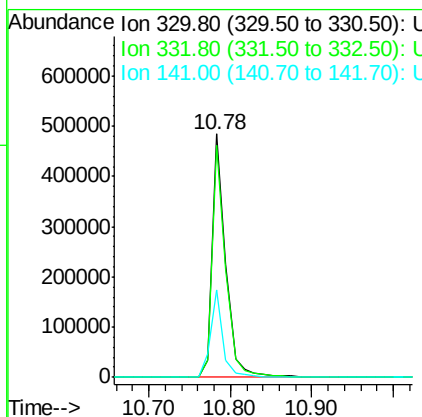

#44
 2-Fluorobiphenyl
 Concen: 91.13 ng
 RT: 9.31 min Scan# 610
 Delta R.T. -0.01 min
 Lab File: U3S6.D
 Acq: 12 Oct 2016 22:27

Tgt Ion:172 Resp: 2380388
 Ion Ratio Lower Upper
 172 100
 171 36.9 31.8 47.8
 170 25.2 21.7 32.5

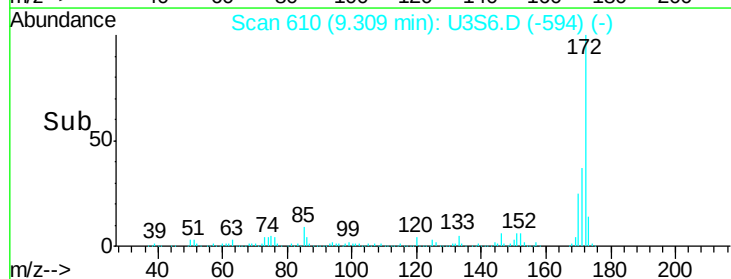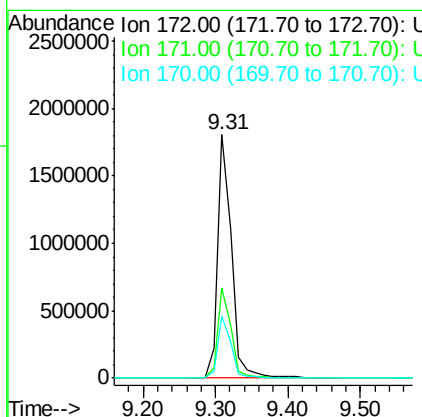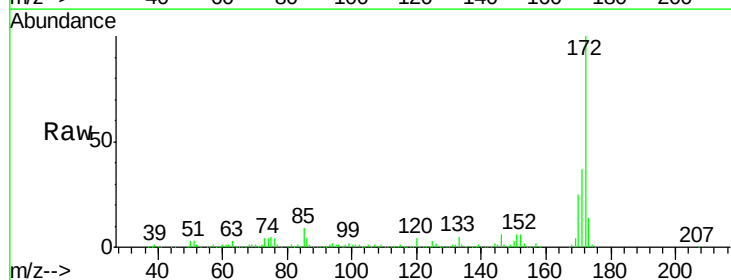

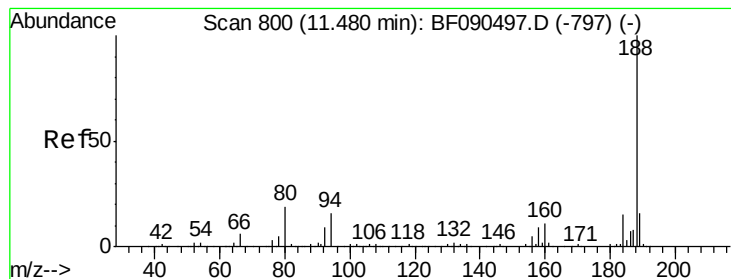

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.48 min Scan# 800

Delta R.T. -0.00 min

Lab File: U3S6.D

Acq: 12 Oct 2016 22:27

Instrument :

BNA_F

ClientSampled :


Tgt Ion:188 Resp: 765790

Ion Ratio Lower Upper

188 100

94 9.8 8.2 12.2




80 10.6 8.8 13.2



Abundance Ion 188.00 (187.70 to 188.70): U

Ion 94.00 (93.70 to 94.70): U3S

Ion 80.00 (79.70 to 80.70): U3S

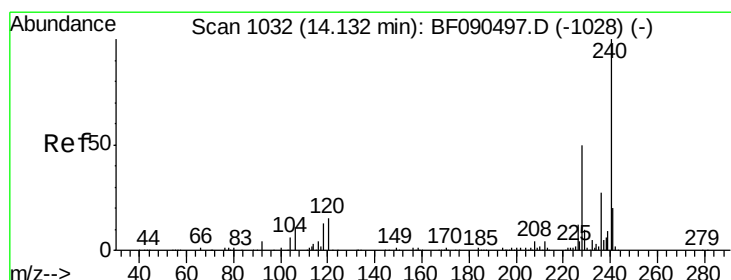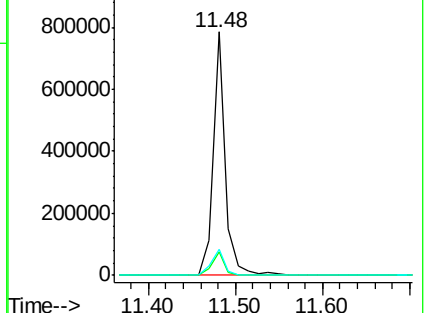

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.12 min Scan# 1031

Delta R.T. -0.01 min

Lab File: U3S6.D

Acq: 12 Oct 2016 22:27


Tgt Ion:240 Resp: 575034

Ion Ratio Lower Upper

240 100

120 13.2 8.6 13.0#



236 26.5 21.6 32.4




Abundance Ion 240.00 (239.70 to 240.70): U

Ion 120.00 (119.70 to 120.70): U

Ion 236.00 (235.70 to 236.70): U

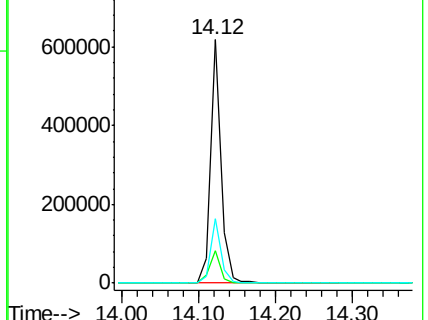



#78

Terphenyl-d14

Concen: 100.84 ng

RT: 13.07 min Scan# 939

Delta R.T. -0.01 min

Lab File: U3S6.D

Acq: 12 Oct 2016 22:27

Instrument :

BNA_F

ClientSampleId :





Tgt Ion:244 Resp: 2372773

Ion Ratio Lower Upper

244 100

212 7.4 6.8 10.2

122 13.5 13.3 19.9

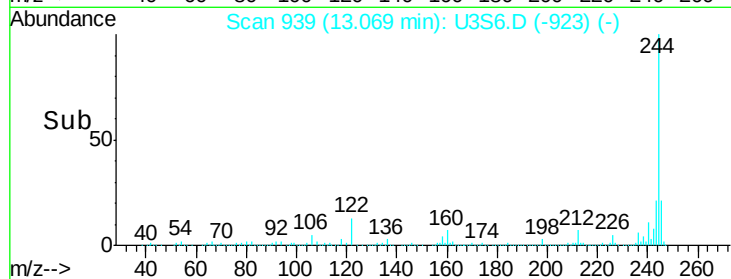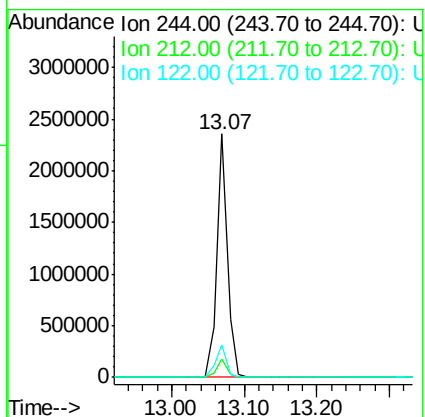

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.60 min Scan# 1160

Delta R.T. -0.01 min

Lab File: U3S6.D

Acq: 12 Oct 2016 22:27

Tgt Ion:264 Resp: 389025

Ion Ratio Lower Upper

264 100

260 24.5 19.3 28.9

265 21.9 17.4 26.0

