
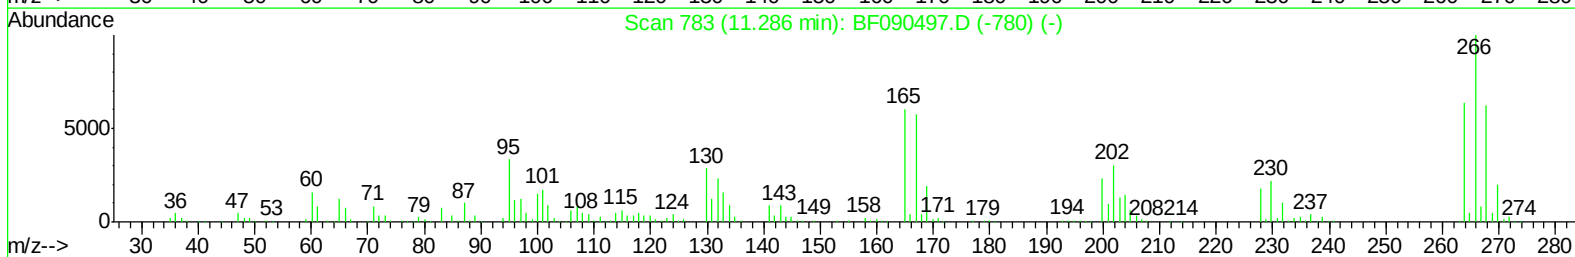
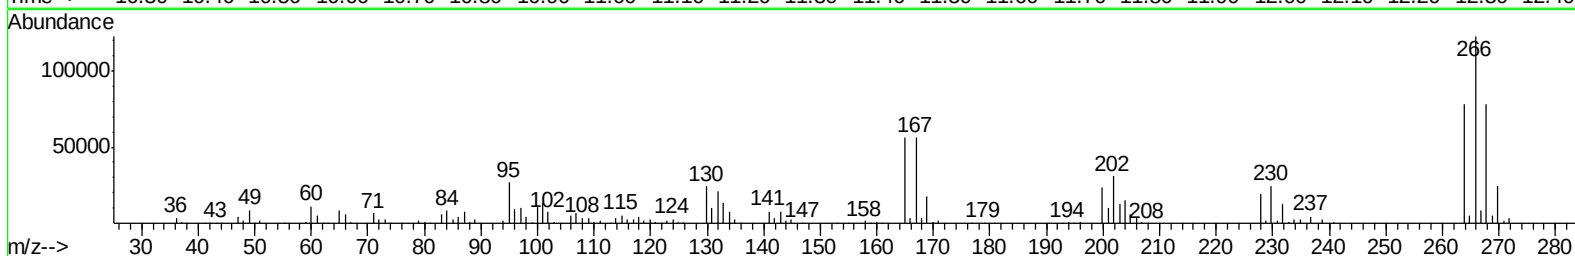


Data Path : Z:\HPCHEM1\BNA_F\Data\BF101216\
Data File : BF090526.D
Acq On : 12 Oct 2016 10:31
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 05:20:54 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 11 16:14:43 2016
Response via : Initial Calibration

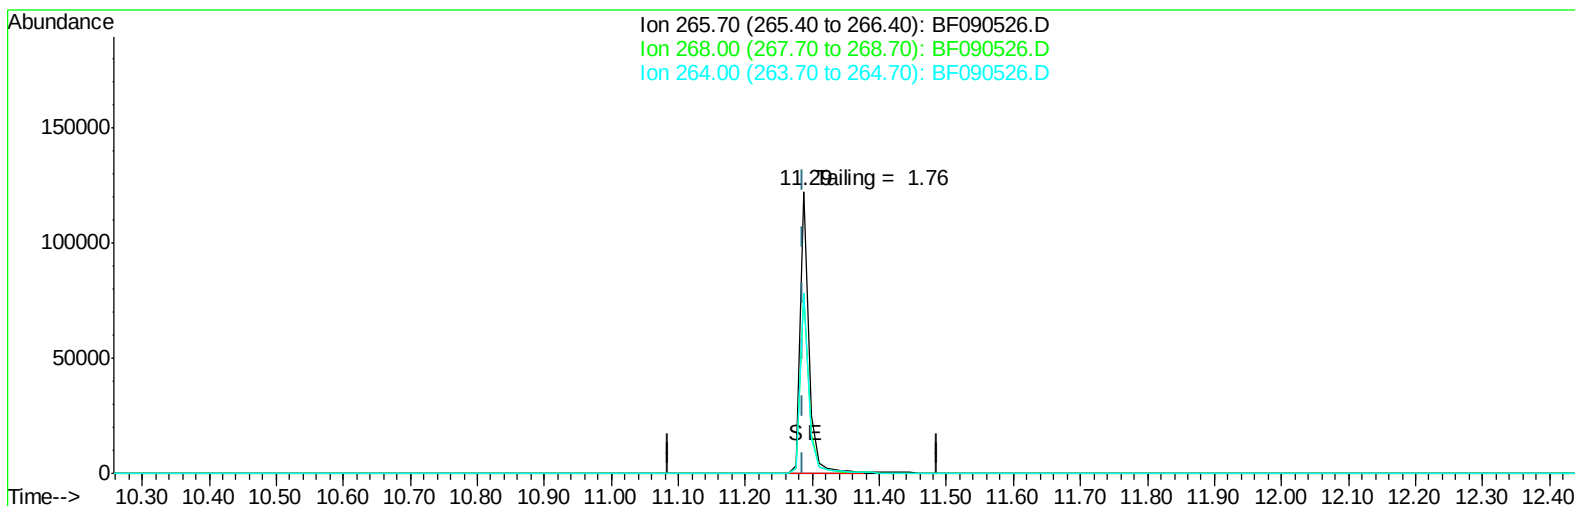

TIC: BF090526.D

(69) Pentachlorophenol (C)




11.286min (+0.000) 32590.28ng

response 113227

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	63.72
264.00	64.40	64.10
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF101216\
 Data File : BF090526.D
 Acq On : 12 Oct 2016 10:31
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 05:20:54 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 11 16:14:43 2016
 Response via : Initial Calibration

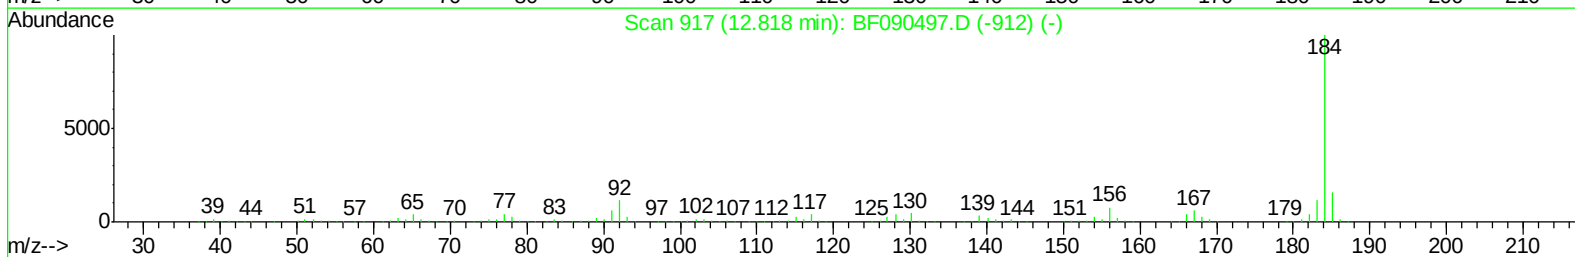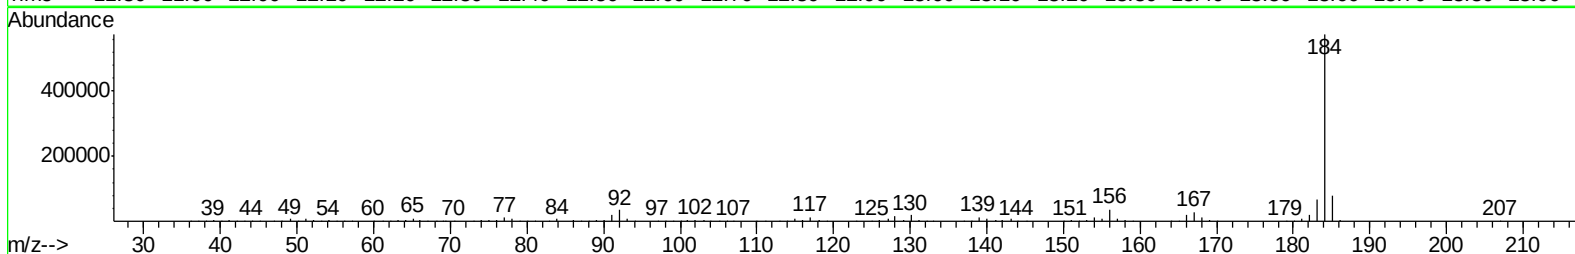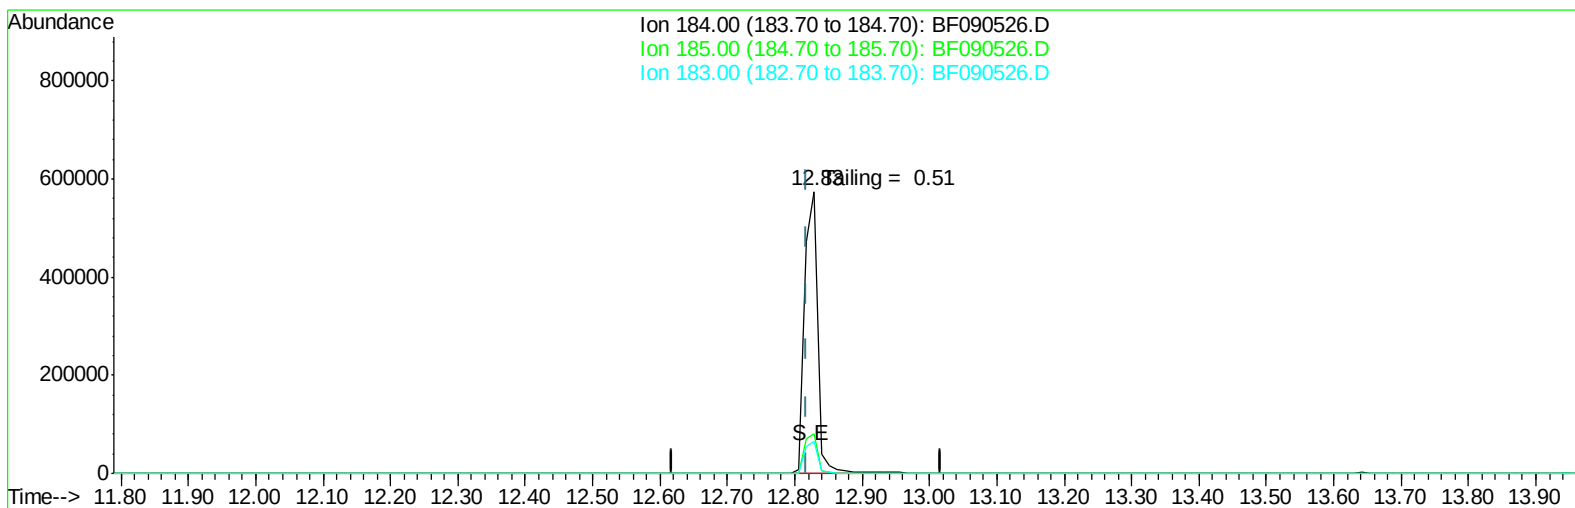

TIC: BF090526.D

(76) Benzidine

12.829min (+0.012) 41489.84ng

response 781087

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.09
183.00	12.00	11.44
0.00	0.00	0.00