


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101216\
 Data File : BF090526.D
 Acq On : 12 Oct 2016 10:31
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 11 16:14:43 2016

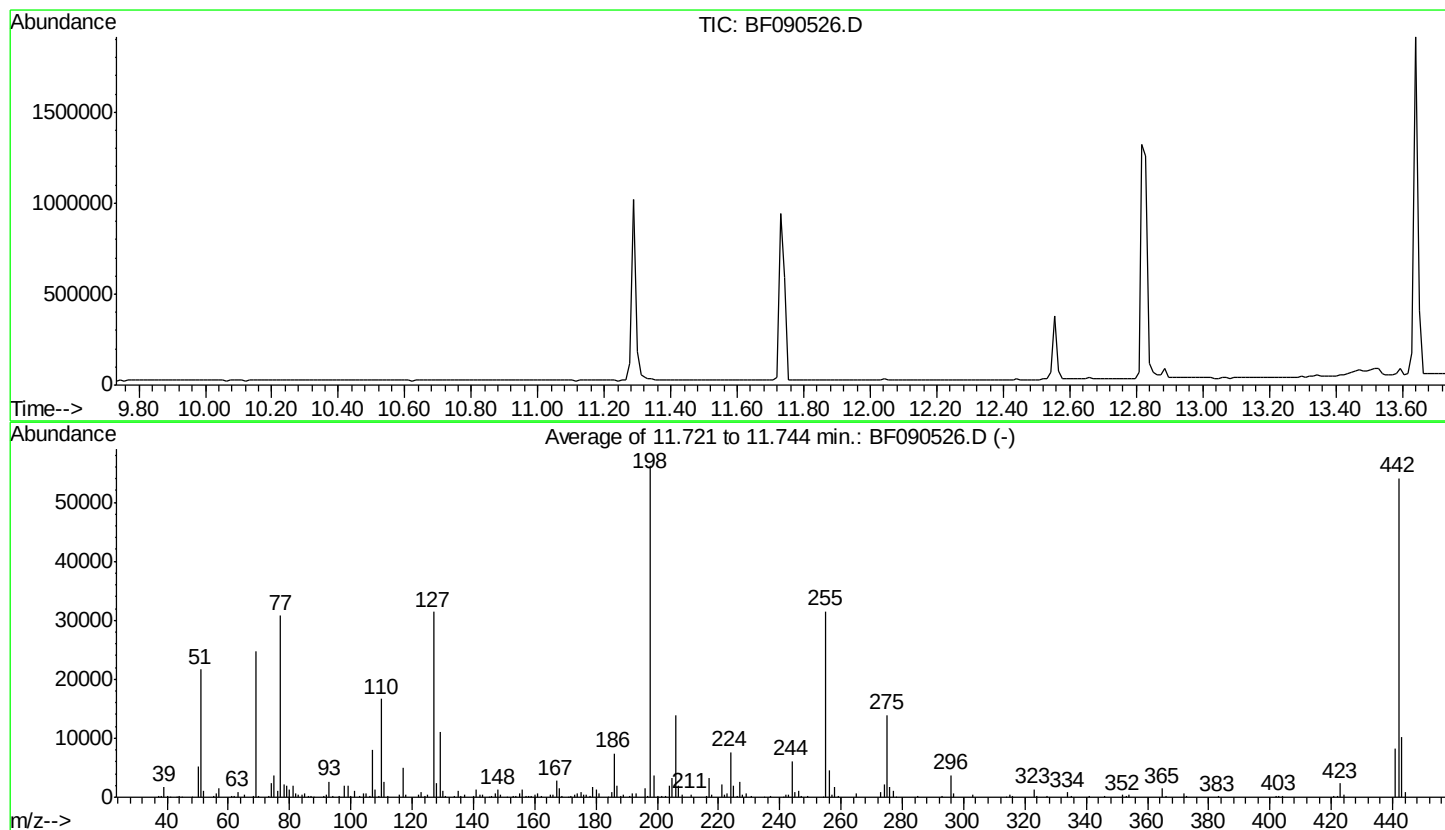

AutoFind: Scans 821, 822, 823; Background Corrected with Scan 818

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	21687	PASS
68	69	0.00	2	1.2	305	PASS
69	198	0.00	100	44.1	24785	PASS
70	69	0.00	2	0.5	136	PASS
127	198	10	80	55.9	31402	PASS
197	198	0.00	2	0.2	137	PASS
198	198	100	100	100.0	56196	PASS
199	198	5	9	6.6	3725	PASS
275	198	10	60	24.9	13968	PASS
365	198	1	100	2.7	1496	PASS
441	442	0.01	24	15.3	8273	PASS
442	198	50	100	96.2	54050	PASS
443	442	15	24	18.8	10135	PASS